

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059348.D
 Acq On : 7 Oct 2023 18:53
 Operator : MA/JU
 Sample : 04607-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBHC3

Quant Time: Oct 07 23:34:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 07 22:45:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.230	152	39104	20.000	ng/u1	0.00
20) Naphthalene-d8	11.067	136	190733	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.863	164	135493	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.713	188	713692	20.000	ng/u1	0.10
79) Chrysene-d12	21.913	240	286244	20.000	ng/u1	0.00
88) Perylene-d12	25.398	264	338481	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.529	96	5775	5.266	ng/uL	0.00
4) Pyridine-d5	3.964	84	49982	15.833	ng/u1	0.00
7) Phenol-d5	7.354	99	32592	7.548	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.548	67	101547	41.609	ng/u1	0.00
11) 2-Chlorophenol-d4	7.748	132	93672	31.019	ng/u1	0.00
15) 4-Methylphenol-d8	8.917	113	58945	17.522	ng/u1	0.00
21) Nitrobenzene-d5	9.422	128	67829	41.776	ng/u1	0.00
24) 2-Nitrophenol-d4	10.145	143	72740	41.392	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.674	165	120968	38.137	ng/u1	0.00
31) 4-Chloroaniline-d4	11.214	131	178701	35.468	ng/u1	0.00
46) Dimethylphthalate-d6	14.258	166	484208	43.621	ng/u1	0.00
49) Acenaphthylene-d8	14.563	160	559992	42.392	ng/u1	0.00
54) 4-Nitrophenol-d4	15.057	143	11430	5.495	ng/u1	0.00
60) Fluorene-d10	15.850	176	452297	42.687	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.056	200	429	0.091	ng/u1	0.09
73) Anthracene-d10	17.713	188	713692	20.385	ng/u1	0.00
81) Pyrene-d10	19.986	212	812126	46.834	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.157	264	812892	45.639	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.564	88	1632	1.394 ng/uL#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059348.D
Acq On : 7 Oct 2023 18:53
Operator : MA/JU
Sample : 04607-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHC3

Quant Time: Oct 07 23:34:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 07 22:45:22 2023
Response via : Initial Calibration

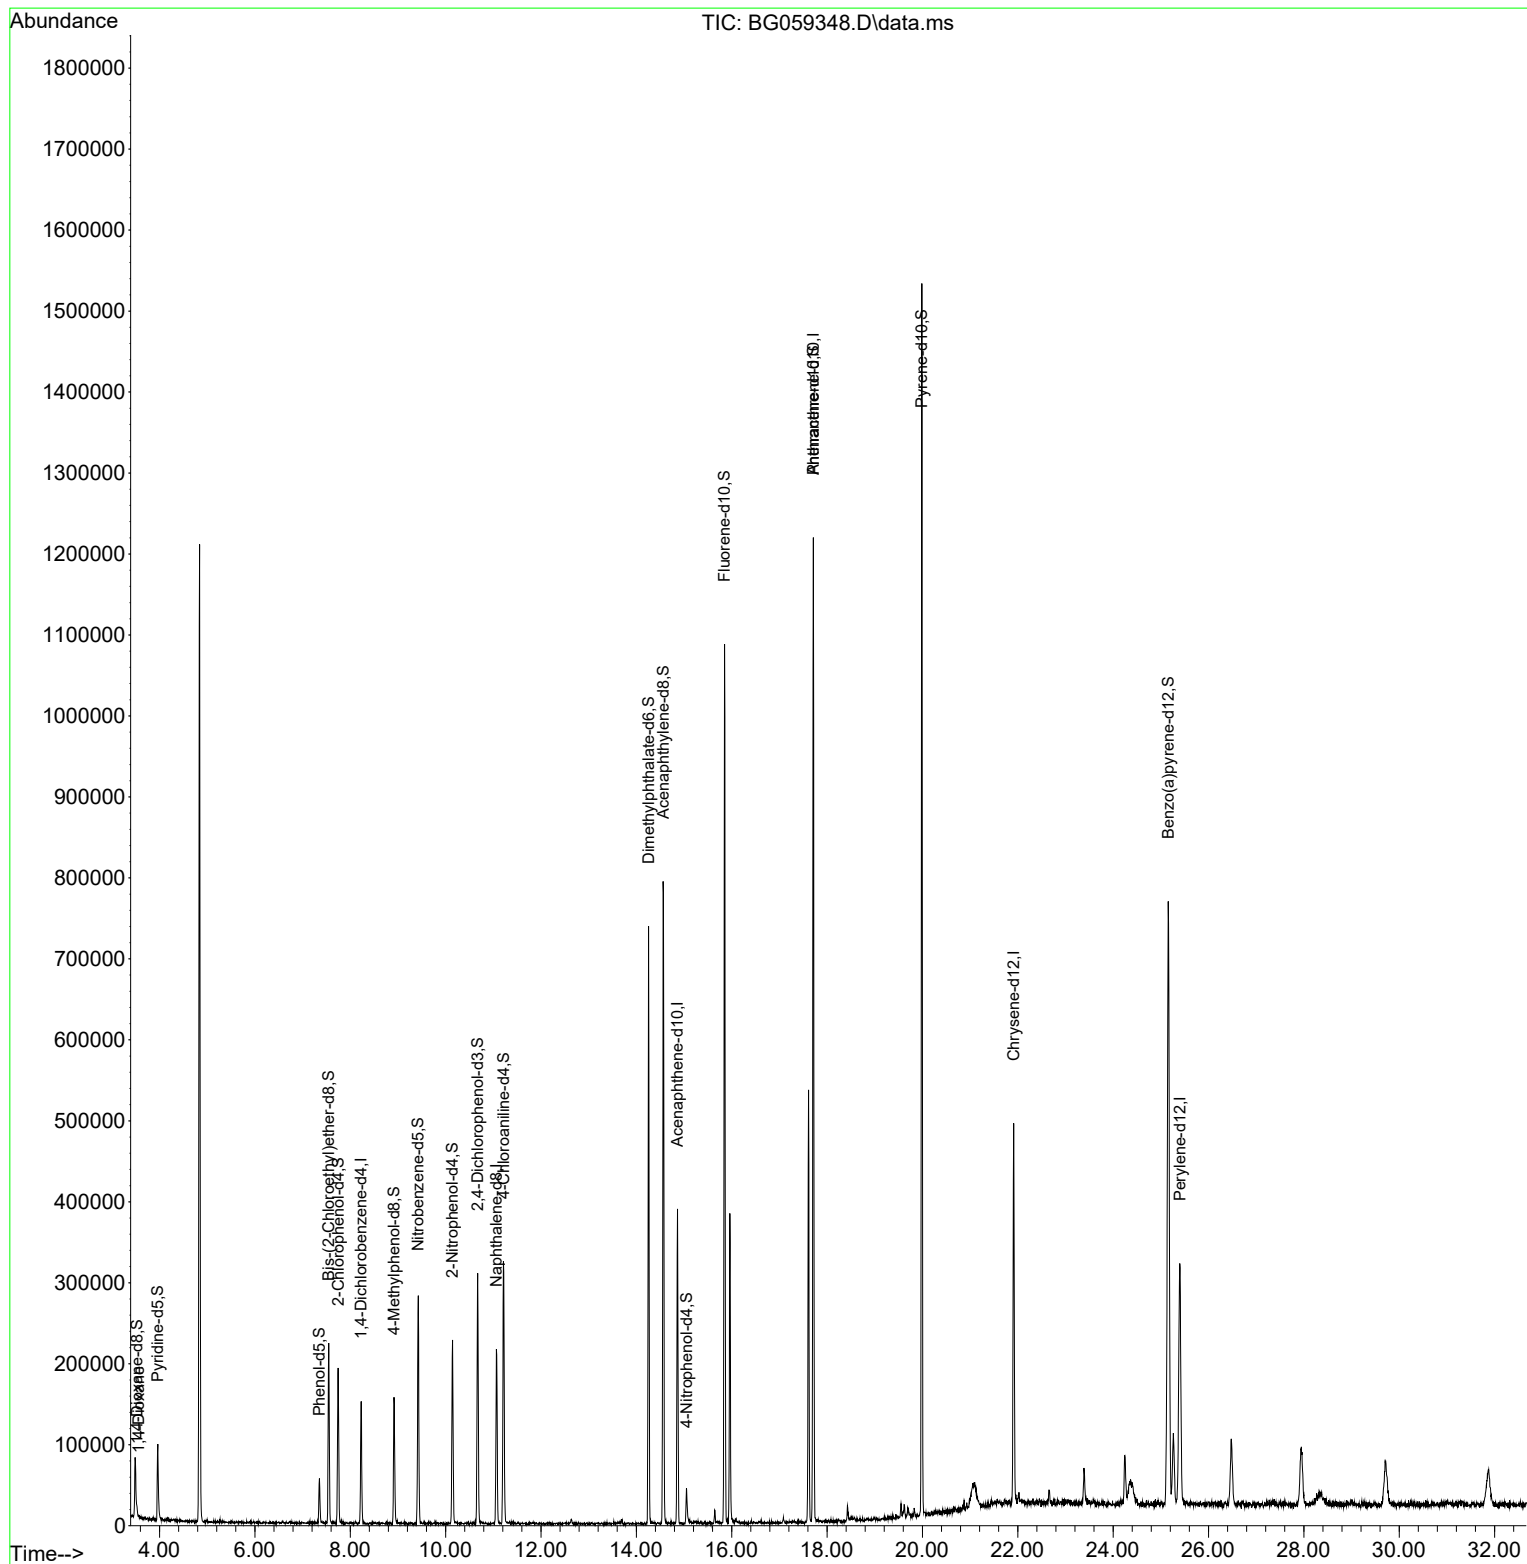

Abundance Scan 30 (3.567 min): BG059340.D\data.ms (-25)

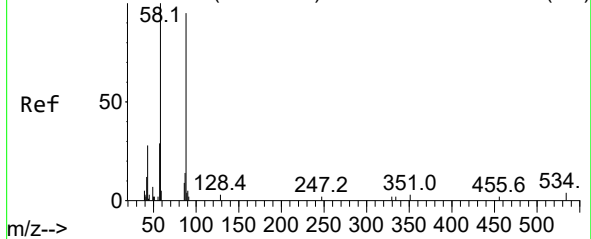

#2

1,4-Dioxane

Concen: 1.394 ng/uL

RT: 3.564 min Scan# 30

Delta R.T. -0.002 min

Lab File: BG059348.D

Acq: 7 Oct 2023 18:53


Instrument :

BNA_G

ClientSampleId :

BBHC3

Abundance Scan 30 (3.564 min): BG059348.D\data.ms

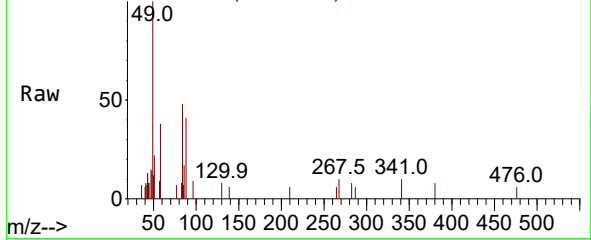

Tgt Ion: 88 Resp: 1632


Ion Ratio Lower Upper

88 100

43 63.2 25.4 38.0#

58 91.0 84.6 127.0

Abundance

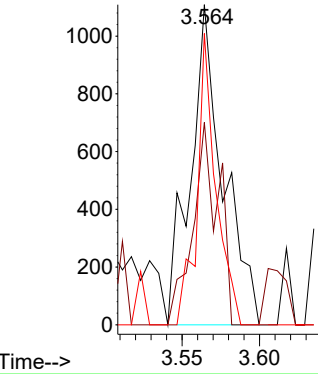

Abundance Scan 30 (3.564 min): BG059348.D\data.ms (-1)

