

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059378.D
 Acq On : 8 Oct 2023 16:33
 Operator : MA/JU
 Sample : PB155973BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK973

Quant Time: Oct 09 01:02:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 07 22:45:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.229	152	47582	20.000	ng/ul	0.00
20) Naphthalene-d8	11.067	136	247012	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.863	164	169914	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.612	188	404639	20.000	ng/ul	0.00
79) Chrysene-d12	21.913	240	367477	20.000	ng/ul	0.00
88) Perylene-d12	25.397	264	433117	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.523	96	10979	8.227	ng/uL	0.00
4) Pyridine-d5	3.958	84	156597	40.768	ng/ul	0.00
7) Phenol-d5	7.354	99	198750	37.829	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.548	67	119766	40.331	ng/ul	0.00
11) 2-Chlorophenol-d4	7.747	132	144441	39.309	ng/ul	0.00
15) 4-Methylphenol-d8	8.923	113	157826	38.555	ng/ul	0.00
21) Nitrobenzene-d5	9.428	128	80655	38.357	ng/ul	0.00
24) 2-Nitrophenol-d4	10.145	143	89521	39.335	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.673	165	153136	37.279	ng/ul	0.00
31) 4-Chloroaniline-d4	11.214	131	244342	37.447	ng/ul	0.00
46) Dimethylphthalate-d6	14.257	166	561814	40.359	ng/ul	0.00
49) Acenaphthylene-d8	14.563	160	660071	39.845	ng/ul	0.00
54) 4-Nitrophenol-d4	15.051	143	96333	36.929	ng/ul	0.00
60) Fluorene-d10	15.850	176	521049	39.214	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.961	200	95232	35.646	ng/ul	0.00
73) Anthracene-d10	17.712	188	805567	40.584	ng/ul	0.00
81) Pyrene-d10	19.986	212	899680	40.414	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.156	264	915830	40.183	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.923	70	3477	1.122 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059378.D
Acq On : 8 Oct 2023 16:33
Operator : MA/JU
Sample : PB155973BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK973


Quant Time: Oct 09 01:02:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 07 22:45:22 2023
Response via : Initial Calibration

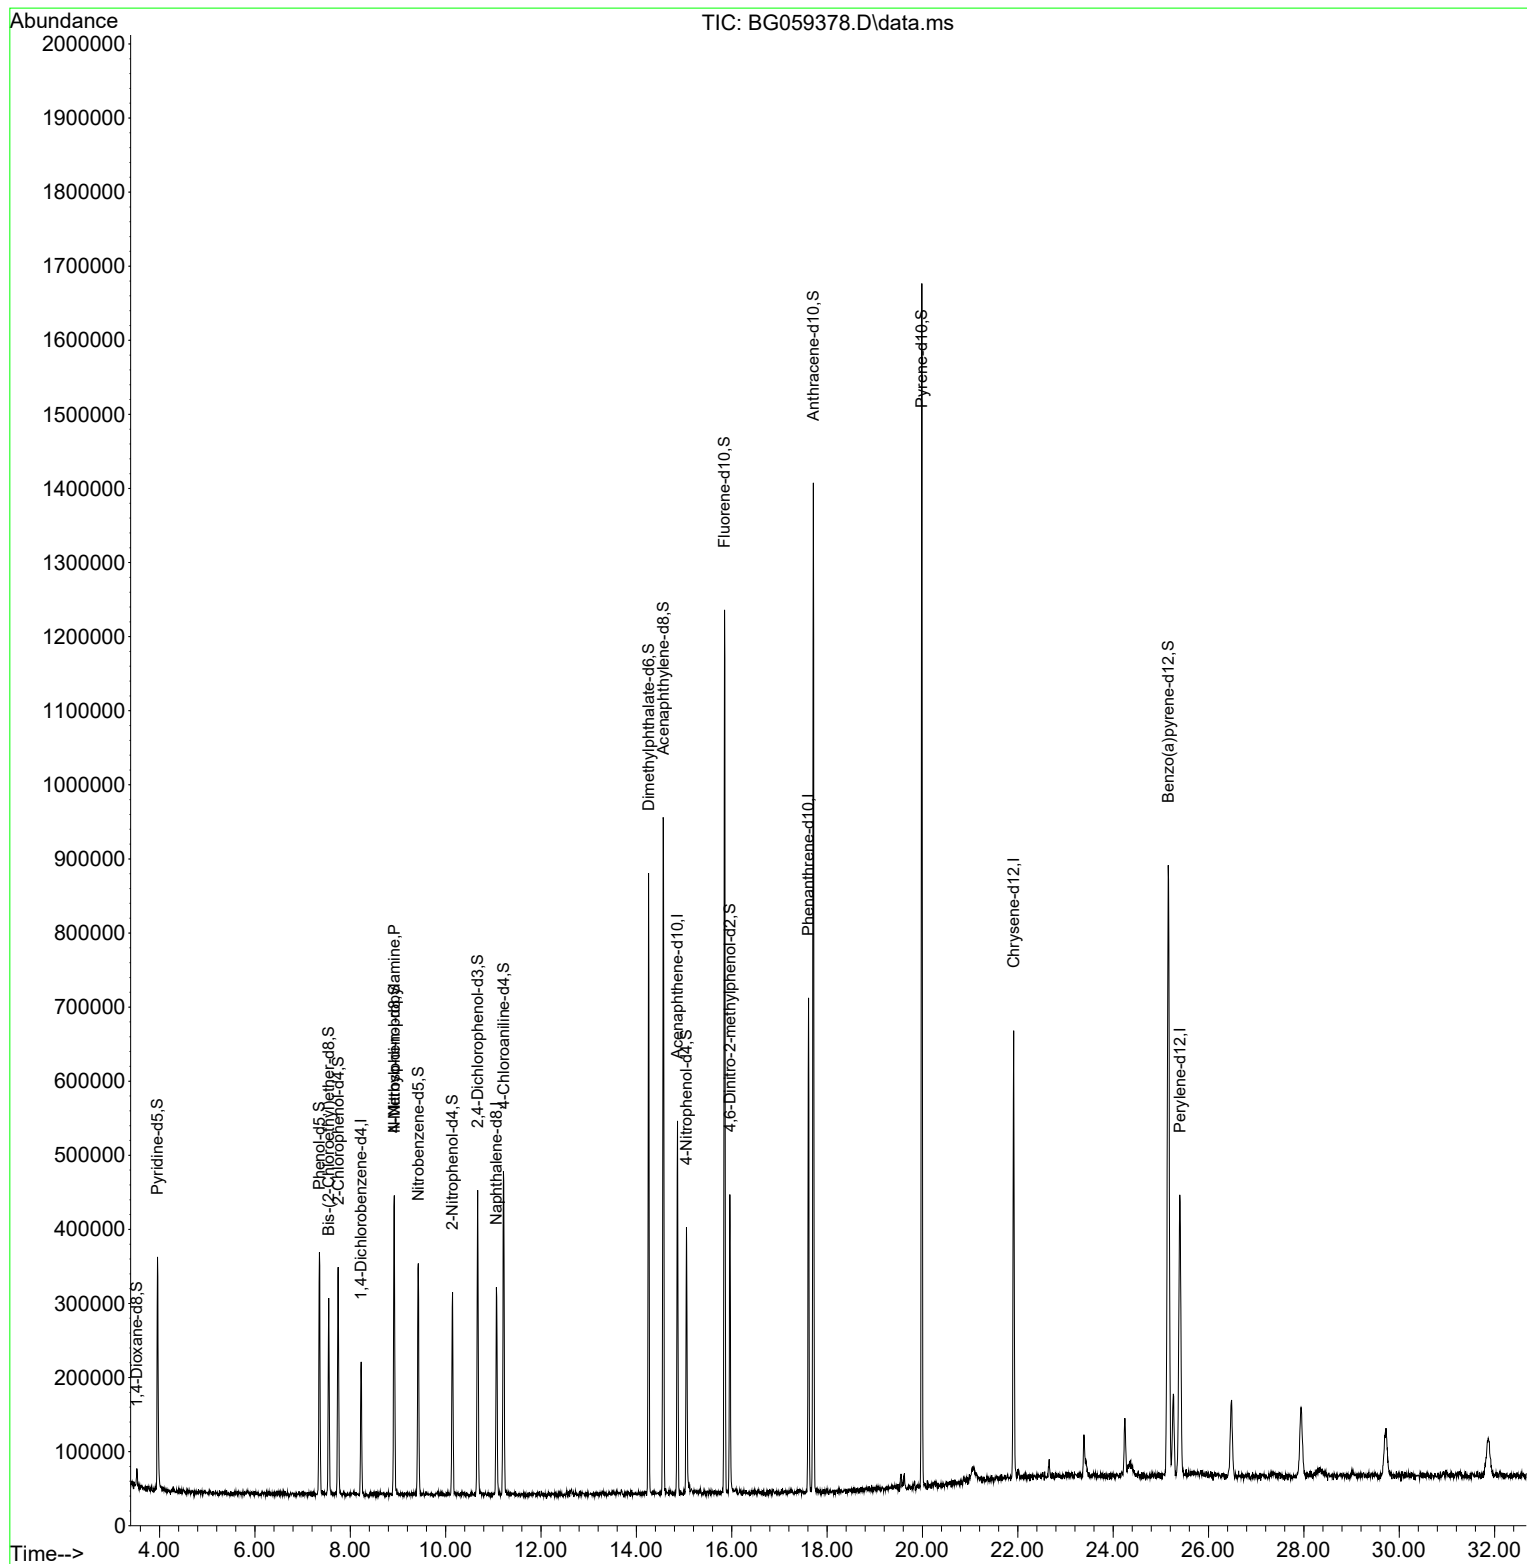

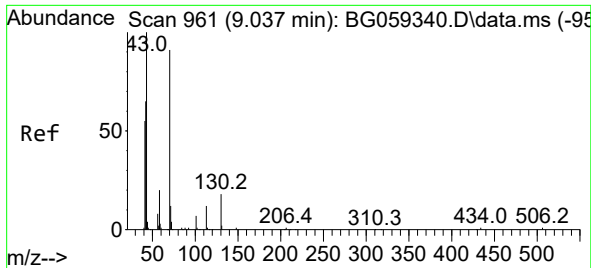

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.122 ng/ul
 RT: 8.923 min Scan# 94
 Delta R.T. -0.114 min
 Lab File: BG059378.D
 Acq: 8 Oct 2023 16:33

Instrument :
 BNA_G
 ClientSampleId :
 SBLK973

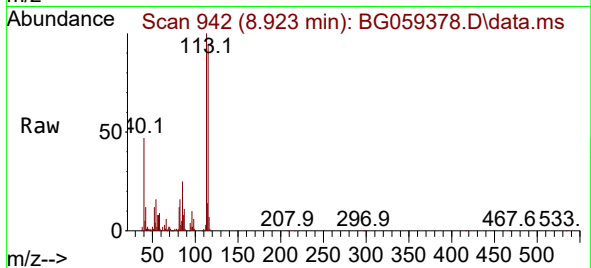

Tgt Ion: 70 Resp: 3477

Ion	Ratio	Lower	Upper
70	100		
42	508.2	58.2	87.4#
101	0.0	6.4	9.6#
130	0.0	15.4	23.0#

