

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059383.D
 Acq On : 8 Oct 2023 19:55
 Operator : MA/JU
 Sample : 04607-08
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBKB2

Quant Time: Oct 09 01:04:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 07 22:45:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.232	152	51126	20.000	ng/ul	0.00
20) Naphthalene-d8	11.069	136	242529	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.865	164	174159	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.615	188	399773	20.000	ng/ul	0.00
79) Chrysene-d12	21.916	240	364605	20.000	ng/ul	0.00
88) Perylene-d12	25.400	264	429848	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.531	96	6321	4.408	ng/uL	0.00
4) Pyridine-d5	3.966	84	24919	6.038	ng/ul	0.00
7) Phenol-d5	7.356	99	43498	7.705	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.550	67	116816	36.611	ng/ul	0.00
11) 2-Chlorophenol-d4	7.744	132	119974	30.387	ng/ul	0.00
15) 4-Methylphenol-d8	8.919	113	80226	18.240	ng/ul	0.00
21) Nitrobenzene-d5	9.430	128	83249	40.323	ng/ul	0.00
24) 2-Nitrophenol-d4	10.147	143	90468	40.486	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.670	165	149363	37.032	ng/ul	0.00
31) 4-Chloroaniline-d4	11.216	131	192650	30.070	ng/ul	0.00
46) Dimethylphthalate-d6	14.260	166	586014	41.071	ng/ul	0.00
49) Acenaphthylene-d8	14.565	160	668781	39.387	ng/ul	0.00
54) 4-Nitrophenol-d4	15.053	143	21736	8.129	ng/ul	0.00
60) Fluorene-d10	15.852	176	546705	40.142	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.964	200	113390	42.959	ng/ul	0.00
73) Anthracene-d10	17.715	188	944640	48.169	ng/ul	0.00
81) Pyrene-d10	19.988	212	1042923	47.218	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.159	264	1104596	48.834	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.309	107	13068	2.999	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059383.D
Acq On : 8 Oct 2023 19:55
Operator : MA/JU
Sample : 04607-08
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBKB2

Quant Time: Oct 09 01:04:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 07 22:45:22 2023
Response via : Initial Calibration

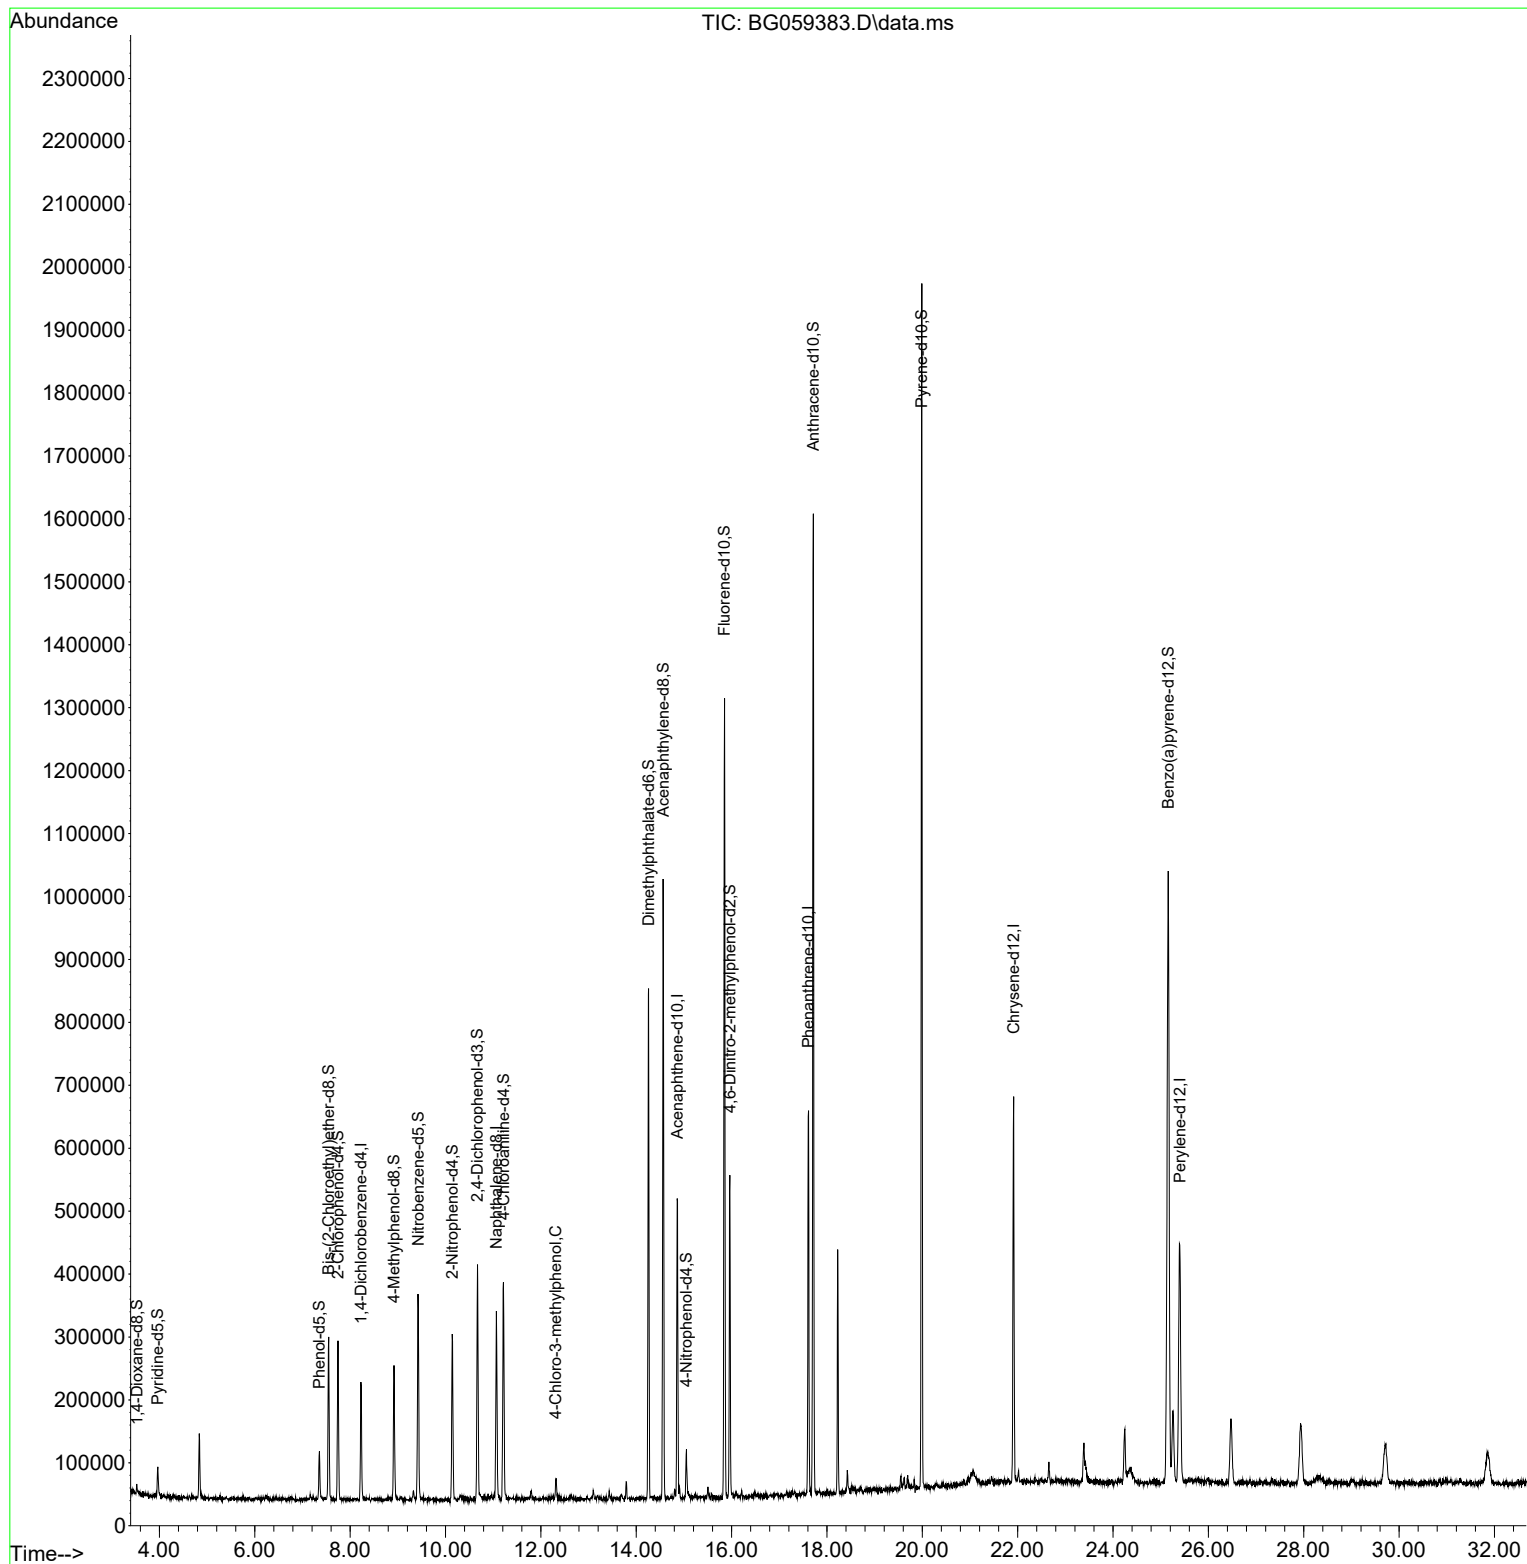

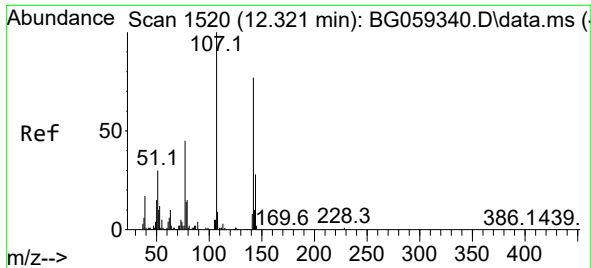

#35
 4-Chloro-3-methylphenol
 Concen: 2.999 ng/ul
 RT: 12.309 min Scan# 1
 Delta R.T. -0.012 min
 Lab File: BG059383.D
 Acq: 8 Oct 2023 19:55

Instrument :
 BNA_G
 ClientSampleId :
 BBKB2

Tgt Ion:107 Resp: 13068
 Ion Ratio Lower Upper
 107 100
 144 20.3 22.0 33.0#
 142 67.6 61.6 92.4

