

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059362.D
 Acq On : 8 Oct 2023 5:06
 Operator : MA/JU
 Sample : PB155977BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK977

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.523	19	23	28	rBV3	24051	34996	1.57%	0.167%
2	3.629	40	41	44	rVB3	4678	3691	0.17%	0.018%
3	3.664	44	47	50	rBV4	5772	7586	0.34%	0.036%
4	3.870	79	82	86	rBV3	5822	7660	0.34%	0.037%
5	3.958	92	97	106	rBV	301289	480480	21.52%	2.297%
6	4.035	109	110	114	rVB2	5978	3395	0.15%	0.016%
7	4.223	138	142	144	rBV3	3002	3877	0.17%	0.019%
8	4.305	153	156	160	rVB4	4604	6344	0.28%	0.030%
9	4.340	160	162	165	rBV4	3328	3536	0.16%	0.017%
10	4.475	183	185	187	rVB2	4639	4085	0.18%	0.020%
11	4.534	190	195	196	rVV3	4499	4056	0.18%	0.019%
12	4.716	221	226	227	rBV4	2590	3926	0.18%	0.019%
13	4.757	232	233	236	rVB	5490	3924	0.18%	0.019%
14	4.792	236	239	244	rVB6	4705	7016	0.31%	0.034%
15	4.975	268	270	272	rBV3	3910	3760	0.17%	0.018%
16	5.345	328	333	334	rBV3	3169	4469	0.20%	0.021%
17	5.527	358	364	367	rVB4	4280	9372	0.42%	0.045%
18	5.627	380	381	386	rVB2	3328	3974	0.18%	0.019%
19	6.637	551	553	556	rVB	4223	3925	0.18%	0.019%
20	6.861	590	591	596	rVB3	3908	4940	0.22%	0.024%
21	6.908	596	599	601	rBV	3252	3551	0.16%	0.017%
22	6.949	604	606	609	rBV2	3243	4139	0.19%	0.020%
23	7.060	620	625	629	rBV3	3249	7469	0.33%	0.036%
24	7.131	636	637	642	rVB3	3293	3582	0.16%	0.017%
25	7.190	642	647	652	rBV3	4633	6271	0.28%	0.030%
26	7.354	668	675	683	rBV	321420	535042	23.96%	2.558%
27	7.548	701	708	716	rVB	244121	403435	18.07%	1.929%
28	7.677	728	730	732	rBV2	4445	3580	0.16%	0.017%
29	7.748	734	742	749	rBV	293196	513213	22.98%	2.453%
30	8.000	784	785	789	rBV2	3517	3772	0.17%	0.018%
31	8.100	799	802	805	rBV	2553	3787	0.17%	0.018%
32	8.141	805	809	812	rVB	5522	4876	0.22%	0.023%
33	8.171	812	814	817	rBV	3777	5781	0.26%	0.028%
34	8.230	818	824	829	rVB	154822	259449	11.62%	1.240%
35	8.394	849	852	857	rVB	4052	7177	0.32%	0.034%
36	8.500	864	870	871	rBV2	5149	5201	0.23%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059362.D
 Acq On : 8 Oct 2023 5:06
 Operator : MA/JU
 Sample : PB155977BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK977

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	8.559	879	880	883	rBV2	3368	4222	0.19%	0.020%
38	8.635	890	893	896	rVB2	4341	3969	0.18%	0.019%
39	8.800	919	921	924	rBV2	3492	3944	0.18%	0.019%
40	8.917	935	941	952	rVB	371329	656509	29.40%	3.138%

41	9.428	1021	1028	1035	rVB	298097	526218	23.56%	2.516%
42	10.145	1142	1150	1159	rBV	253644	447093	20.02%	2.137%
43	10.227	1161	1164	1167	rVB2	2797	4276	0.19%	0.020%
44	10.327	1179	1181	1184	rVB	4244	3899	0.17%	0.019%
45	10.368	1184	1188	1189	rBV	3288	4893	0.22%	0.023%

46	10.503	1209	1211	1214	rBV	3551	4030	0.18%	0.019%
47	10.533	1214	1216	1220	rBV	3243	5043	0.23%	0.024%
48	10.674	1232	1240	1248	rVV	374449	658631	29.49%	3.149%
49	11.067	1297	1307	1314	rBV	239063	437687	19.60%	2.092%
50	11.214	1325	1332	1341	rBV	408457	731325	32.75%	3.496%

51	11.573	1392	1393	1395	rBV	4316	3803	0.17%	0.018%
52	12.037	1469	1472	1474	rBV	3869	3710	0.17%	0.018%
53	12.624	1568	1572	1573	rBV2	6268	7682	0.34%	0.037%
54	12.912	1618	1621	1623	rBV	3983	4245	0.19%	0.020%
55	13.212	1670	1672	1674	rBV	4725	4620	0.21%	0.022%

56	13.353	1695	1696	1700	rVB	4812	4523	0.20%	0.022%
57	13.441	1707	1711	1713	rVB2	5946	7809	0.35%	0.037%
58	13.465	1713	1715	1717	rBV	5573	4165	0.19%	0.020%
59	13.518	1721	1724	1728	rVB	3969	6682	0.30%	0.032%
60	13.694	1751	1754	1761	rVB2	8648	13940	0.62%	0.067%

61	13.894	1786	1788	1790	rVB	5413	4140	0.19%	0.020%
62	13.917	1790	1792	1794	rBV	5503	3612	0.16%	0.017%
63	13.952	1794	1798	1800	rBV	5416	5344	0.24%	0.026%
64	13.982	1800	1803	1804	rBV	3624	3523	0.16%	0.017%
65	14.035	1808	1812	1813	rBV	3649	4770	0.21%	0.023%

66	14.217	1839	1843	1844	rBV	2852	3541	0.16%	0.017%
67	14.258	1844	1850	1858	rVB	754618	1085873	48.62%	5.191%
68	14.405	1873	1875	1877	rBV	5789	4161	0.19%	0.020%
69	14.563	1896	1902	1909	rBV	859209	1350755	60.48%	6.457%
70	14.734	1929	1931	1933	rBV	4426	5077	0.23%	0.024%

71	14.863	1945	1953	1960	rBV	423293	652048	29.20%	3.117%
72	15.051	1979	1985	1996	rBV	338040	556839	24.93%	2.662%
73	15.227	2013	2015	2017	rBV	4653	3465	0.16%	0.017%
74	15.462	2051	2055	2056	rBV	5280	4857	0.22%	0.023%
75	15.668	2089	2090	2093	rBV	4350	3942	0.18%	0.019%

76	15.697	2093	2095	2098	rVB	5079	5193	0.23%	0.025%
----	--------	------	------	------	-----	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059362.D
 Acq On : 8 Oct 2023 5:06
 Operator : MA/JU
 Sample : PB155977BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK977

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

77	15.738	2098	2102	2105	rBV	5751	8300	0.37%	0.040%
78	15.850	2114	2121	2128	rBV	1139257	1683498	75.38%	8.048%
79	15.962	2134	2140	2146	rBV	400023	575441	25.77%	2.751%
80	16.085	2159	2161	2168	rVB3	4883	8016	0.36%	0.038%
81	16.291	2194	2196	2198	rVB	4294	3449	0.15%	0.016%
82	16.308	2198	2199	2201	rBV	3709	3473	0.16%	0.017%
83	16.508	2231	2233	2234	rBV	5267	4027	0.18%	0.019%
84	16.532	2235	2237	2241	rVB2	6324	7455	0.33%	0.036%
85	16.773	2276	2278	2279	rBV	5881	5264	0.24%	0.025%
86	16.808	2283	2284	2287	rBV	4452	4381	0.20%	0.021%
87	16.902	2299	2300	2302	rBV	4933	3701	0.17%	0.018%
88	17.613	2415	2421	2429	rBV	555049	815359	36.51%	3.898%
89	17.713	2431	2438	2448	rVB	1304844	1915815	85.79%	9.159%
90	18.194	2518	2520	2521	rBV2	5602	3873	0.17%	0.019%
91	19.181	2686	2688	2691	rVB	5435	4678	0.21%	0.022%
92	19.546	2748	2750	2755	rVB4	16847	21649	0.97%	0.103%
93	19.775	2787	2789	2791	rBV	7497	3921	0.18%	0.019%
94	19.834	2797	2799	2802	rBV4	8570	8144	0.36%	0.039%
95	19.986	2819	2825	2832	rBV	1514627	2125172	95.16%	10.159%
96	20.174	2856	2857	2859	rBV	7320	5697	0.26%	0.027%
97	21.914	3146	3153	3162	rBV2	494126	860261	38.52%	4.113%
98	24.240	3546	3549	3555	rVB5	40585	75509	3.38%	0.361%
99	25.151	3694	3704	3715	rBV2	796455	2233210	100.00%	10.676%
100	25.404	3737	3747	3756	rVB3	322825	912446	40.86%	4.362%




Sum of corrected areas: 20918134

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059362.D
Acq On : 8 Oct 2023 5:06
Operator : MA/JU
Sample : PB155977BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK977

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

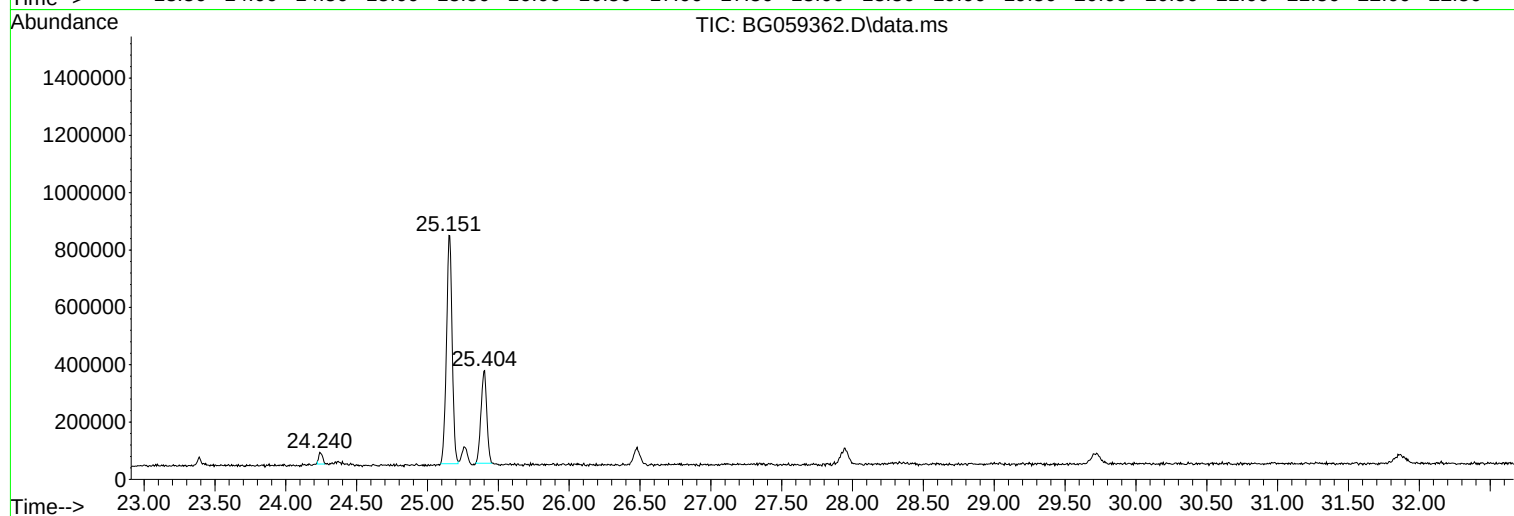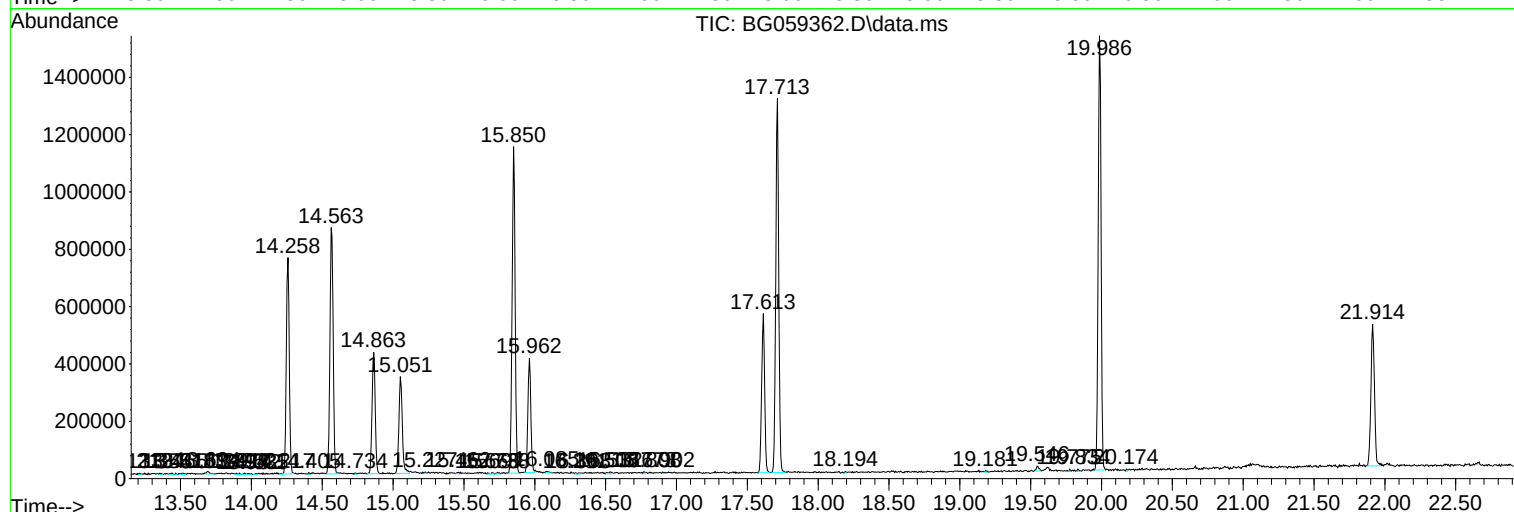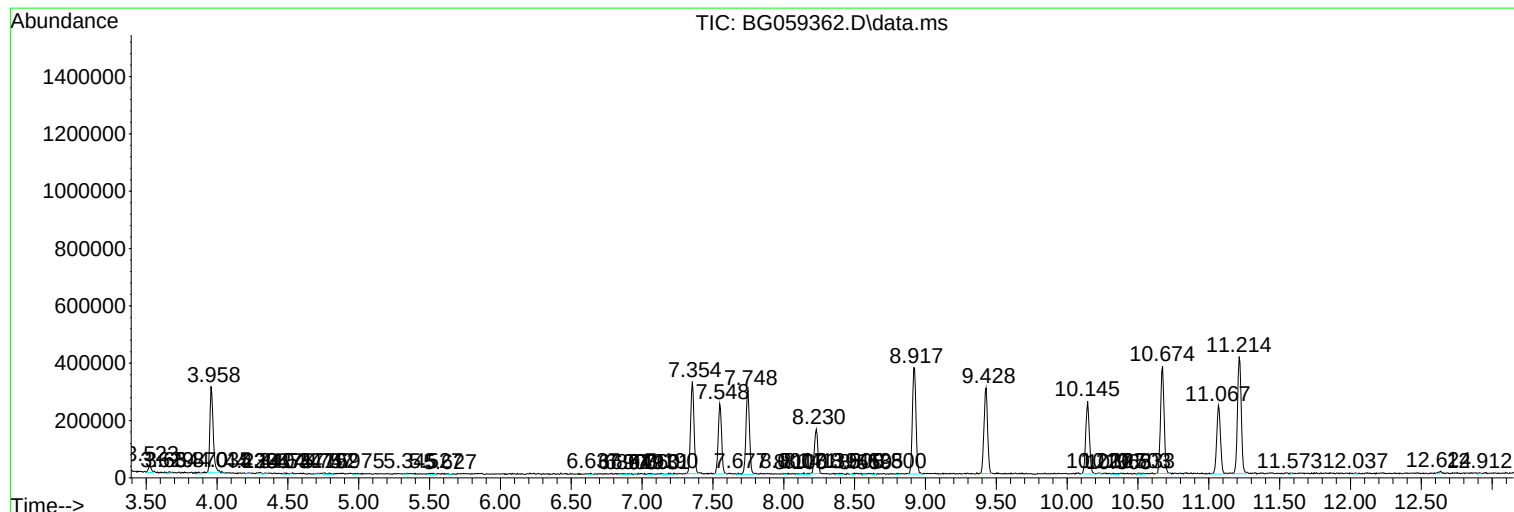

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059362.D
Acq On : 8 Oct 2023 5:06
Operator : MA/JU
Sample : PB155977BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK977

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059362.D
Acq On : 8 Oct 2023 5:06
Operator : MA/JU
Sample : PB155977BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK977

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc