

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059376.D
 Acq On : 8 Oct 2023 15:12
 Operator : MA/JU
 Sample : PB156048BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK048

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	33	34	37	rVB	9507	6745	0.30%	0.031%
2	3.963	93	98	109	rBV	305886	517191	23.11%	2.371%
3	4.175	132	134	138	rVB2	8583	7550	0.34%	0.035%
4	4.974	268	270	273	rBV	8035	8042	0.36%	0.037%
5	5.221	309	312	314	rBV	6577	9543	0.43%	0.044%
6	5.585	372	374	378	rVB2	6565	6141	0.27%	0.028%
7	5.714	394	396	397	rBV	7673	7538	0.34%	0.035%
8	5.985	439	442	444	rBV	10093	8369	0.37%	0.038%
9	6.361	504	506	509	rBV	5720	7976	0.36%	0.037%
10	6.972	608	610	615	rVB	8321	7284	0.33%	0.033%
11	7.013	615	617	620	rBV	5964	6226	0.28%	0.029%
12	7.354	668	675	684	rVV	329257	573586	25.63%	2.629%
13	7.424	685	687	691	rVB2	8252	6452	0.29%	0.030%
14	7.547	703	708	716	rVB	269254	434743	19.42%	1.993%
15	7.747	735	742	750	rVB	308792	536256	23.96%	2.458%
16	8.229	818	824	830	rVB2	182866	307255	13.73%	1.408%
17	8.628	888	892	894	rBV	5412	8371	0.37%	0.038%
18	8.664	897	898	900	rBV	8069	6775	0.30%	0.031%
19	8.922	934	942	951	rBV	402644	695145	31.06%	3.187%
20	9.428	1021	1028	1035	rVB	319648	561988	25.11%	2.576%
21	9.698	1071	1074	1075	rBV	8243	6849	0.31%	0.031%
22	10.015	1125	1128	1133	rVB	4967	7675	0.34%	0.035%
23	10.050	1133	1134	1137	rBV	6638	6324	0.28%	0.029%
24	10.144	1142	1150	1157	rVV	258661	476262	21.28%	2.183%
25	10.297	1175	1176	1179	rBV	7050	6316	0.28%	0.029%
26	10.438	1195	1200	1203	rBV	6226	11358	0.51%	0.052%
27	10.673	1233	1240	1246	rBV	385156	698437	31.20%	3.202%
28	11.067	1300	1307	1317	rVB	268055	490299	21.90%	2.248%
29	11.214	1325	1332	1339	rBV	422286	767938	34.31%	3.520%
30	11.690	1410	1413	1417	rBV	3858	6336	0.28%	0.029%
31	12.630	1569	1573	1578	rBV4	8277	13193	0.59%	0.060%
32	13.317	1687	1690	1693	rBV	5748	6938	0.31%	0.032%
33	13.693	1749	1754	1756	rVB2	12112	12997	0.58%	0.060%
34	13.805	1770	1773	1775	rBV	6543	7963	0.36%	0.037%
35	14.257	1844	1850	1858	rBV	792823	1129372	50.46%	5.177%
36	14.486	1887	1889	1892	rVB	7106	7182	0.32%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059376.D
 Acq On : 8 Oct 2023 15:12
 Operator : MA/JU
 Sample : PB156048BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK048

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	14.522	1892	1895	1896	rBV	6898	7153	0.32%	0.033%
38	14.563	1896	1902	1912	rVB2	878086	1424636	63.65%	6.531%
39	14.862	1945	1953	1959	rBV	482112	742545	33.17%	3.404%
40	15.050	1980	1985	1995	rBV	333291	547582	24.46%	2.510%
41	15.661	2086	2089	2092	rBV	6802	10183	0.45%	0.047%
42	15.849	2113	2121	2127	rBV	1201355	1761716	78.71%	8.076%
43	15.961	2134	2140	2147	rBV	403380	590626	26.39%	2.707%
44	17.612	2415	2421	2428	rVB	608055	907112	40.53%	4.158%
45	17.712	2431	2438	2446	rVV	1348178	1946834	86.98%	8.924%
46	18.388	2551	2553	2556	rBV	7580	9360	0.42%	0.043%
47	19.081	2668	2671	2672	rBV	6649	6726	0.30%	0.031%
48	19.821	2795	2797	2798	rBV	9025	6867	0.31%	0.031%
49	19.986	2819	2825	2832	rVB	1573451	2213094	98.87%	10.145%
50	20.056	2835	2837	2840	rBV2	9622	11352	0.51%	0.052%
51	21.913	3147	3153	3162	rBV	574639	965139	43.12%	4.424%
52	25.156	3696	3705	3716	rVB3	792723	2238330	100.00%	10.261%
53	25.397	3738	3746	3757	rVB2	352941	1046720	46.76%	4.798%




Sum of corrected areas: 21814590

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059376.D
Acq On : 8 Oct 2023 15:12
Operator : MA/JU
Sample : PB156048BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK048

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

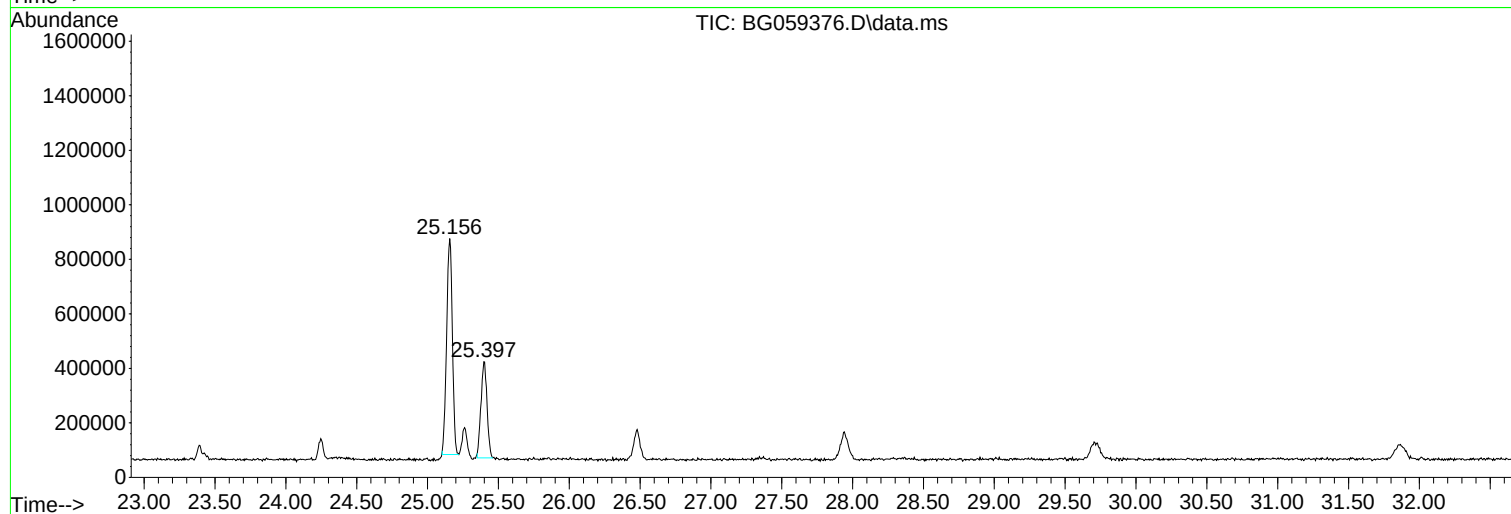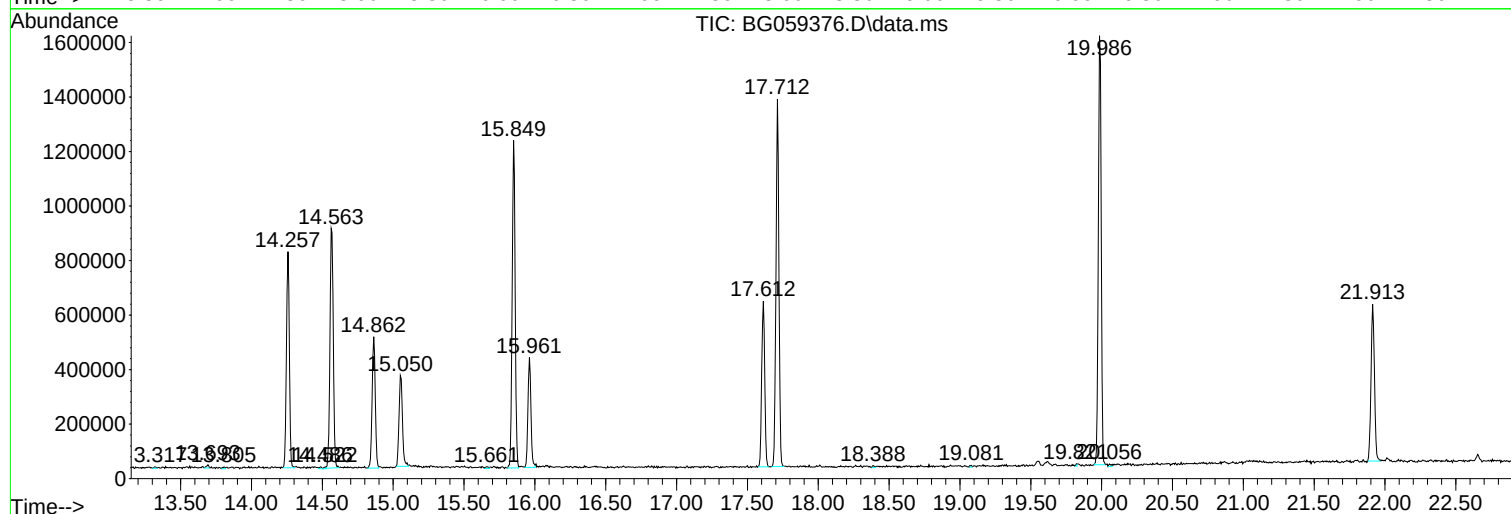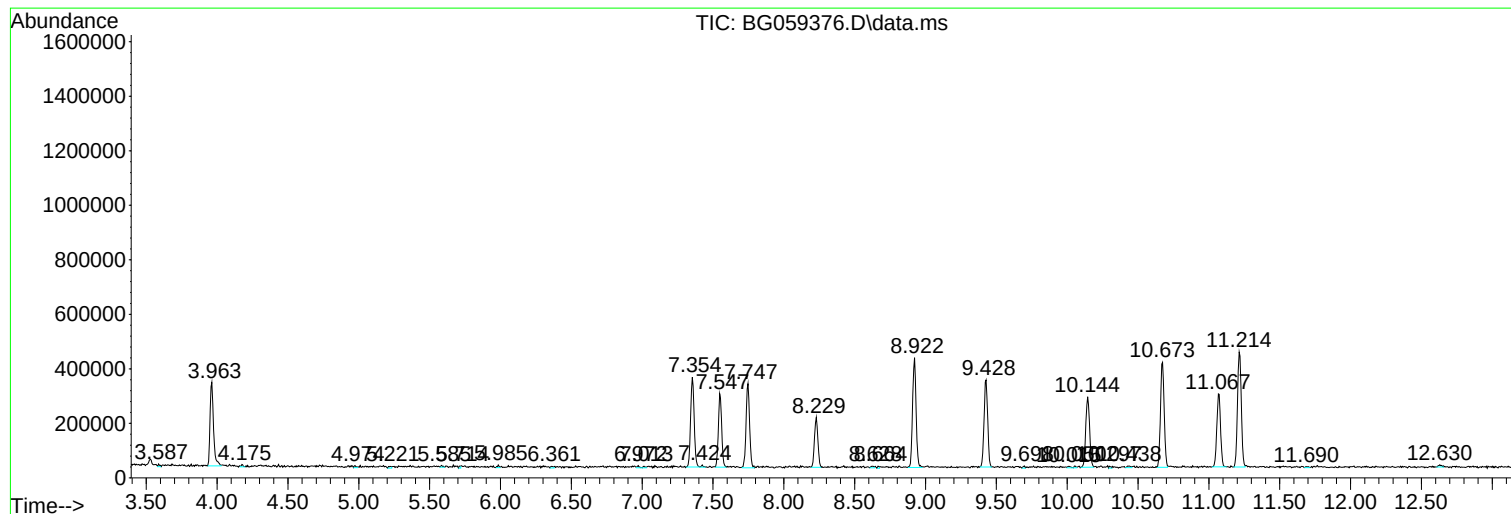

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059376.D
Acq On : 8 Oct 2023 15:12
Operator : MA/JU
Sample : PB156048BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK048

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059376.D
Acq On : 8 Oct 2023 15:12
Operator : MA/JU
Sample : PB156048BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK048

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------