

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059377.D
 Acq On : 8 Oct 2023 15:53
 Operator : MA/JU
 Sample : PB156054BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059377.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.959	92	97	107	rBV	293639	478273	22.07%	2.395%
2	5.175	301	304	307	rVB	6705	7604	0.35%	0.038%
3	5.381	337	339	344	rBV	5663	9413	0.43%	0.047%
4	5.516	360	362	364	rBV	6896	6368	0.29%	0.032%
5	6.697	560	563	566	rBV	4679	8148	0.38%	0.041%
6	7.102	629	632	634	rBV	5945	7067	0.33%	0.035%
7	7.355	668	675	682	rBV	317413	536117	24.74%	2.685%
8	7.549	702	708	717	rVB	249986	404160	18.65%	2.024%
9	7.749	735	742	749	rBV	285966	492047	22.70%	2.464%
10	8.230	817	824	830	rBV	171882	290786	13.42%	1.456%
11	8.319	838	839	843	rVB	9568	8508	0.39%	0.043%
12	8.348	843	844	847	rBV	7480	8383	0.39%	0.042%
13	8.407	850	854	857	rBV2	4700	7424	0.34%	0.037%
14	8.659	895	897	901	rVB	9568	7182	0.33%	0.036%
15	8.924	935	942	949	rVB	375331	649391	29.96%	3.252%
16	9.429	1021	1028	1035	rVB	300145	520731	24.03%	2.608%
17	9.535	1042	1046	1047	rBV	6845	8019	0.37%	0.040%
18	9.923	1108	1112	1116	rBV	5007	7688	0.35%	0.039%
19	9.981	1120	1122	1124	rBV	7866	6925	0.32%	0.035%
20	10.146	1140	1150	1158	rBV	253125	452584	20.88%	2.267%
21	10.369	1185	1188	1190	rBV	7777	7987	0.37%	0.040%
22	10.551	1216	1219	1221	rBV	8005	8422	0.39%	0.042%
23	10.616	1225	1230	1232	rBV	5212	7883	0.36%	0.039%
24	10.675	1232	1240	1246	rBV	359354	661985	30.55%	3.315%
25	10.804	1260	1262	1267	rVB	5723	7301	0.34%	0.037%
26	11.068	1301	1307	1315	rVB	258790	471480	21.76%	2.361%
27	11.215	1323	1332	1343	rBV	408745	740522	34.17%	3.709%
28	11.544	1385	1388	1390	rBV	5805	6748	0.31%	0.034%
29	11.621	1397	1401	1404	rVB	4881	7043	0.32%	0.035%
30	12.014	1467	1468	1471	rBV	5933	6504	0.30%	0.033%
31	12.584	1563	1565	1569	rBV	8996	11243	0.52%	0.056%
32	12.713	1582	1587	1588	rVB	5382	7925	0.37%	0.040%
33	12.960	1625	1629	1632	rVB	7509	11307	0.52%	0.057%
34	13.959	1798	1799	1803	rBV	6155	6048	0.28%	0.030%
35	14.259	1842	1850	1858	rBV	734945	1066346	49.20%	5.341%
36	14.441	1879	1881	1887	rVB	6872	8159	0.38%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059377.D
 Acq On : 8 Oct 2023 15:53
 Operator : MA/JU
 Sample : PB156054BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	14.511	1890	1893	1895	rVB	7159	7679	0.35%	0.038%
38	14.564	1895	1902	1911	rBV2	835962	1381168	63.73%	6.917%
39	14.864	1946	1953	1963	rVB2	439476	702895	32.43%	3.520%
40	15.052	1979	1985	1991	rBV	334907	526321	24.29%	2.636%
41	15.387	2041	2042	2045	rBV	9087	6066	0.28%	0.030%
42	15.622	2078	2082	2084	rBV	6549	9341	0.43%	0.047%
43	15.851	2115	2121	2130	rVB	1155430	1676958	77.38%	8.399%
44	15.963	2134	2140	2148	rBV2	365673	570736	26.33%	2.858%
45	17.050	2323	2325	2328	rVB	7069	6199	0.29%	0.031%
46	17.367	2378	2379	2382	rBV	7395	6939	0.32%	0.035%
47	17.525	2405	2406	2410	rVB	8422	6118	0.28%	0.031%
48	17.608	2415	2420	2427	rVB	579563	893618	41.23%	4.476%
49	17.713	2432	2438	2445	rVB	1260402	1894648	87.42%	9.489%
50	17.896	2466	2469	2472	rBV	6413	6599	0.30%	0.033%
51	18.424	2555	2559	2563	rBV2	6004	9013	0.42%	0.045%
52	18.983	2653	2654	2659	rBV	8342	13722	0.63%	0.069%
53	19.858	2802	2803	2809	rBV4	7058	11053	0.51%	0.055%
54	19.987	2819	2825	2832	rBV	1572563	2163396	99.82%	10.835%
55	21.914	3147	3153	3163	rVB	550919	953441	43.99%	4.775%
56	25.158	3696	3705	3715	rVB2	755546	2167215	100.00%	10.854%




Sum of corrected areas: 19966846

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059377.D
Acq On : 8 Oct 2023 15:53
Operator : MA/JU
Sample : PB156054BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

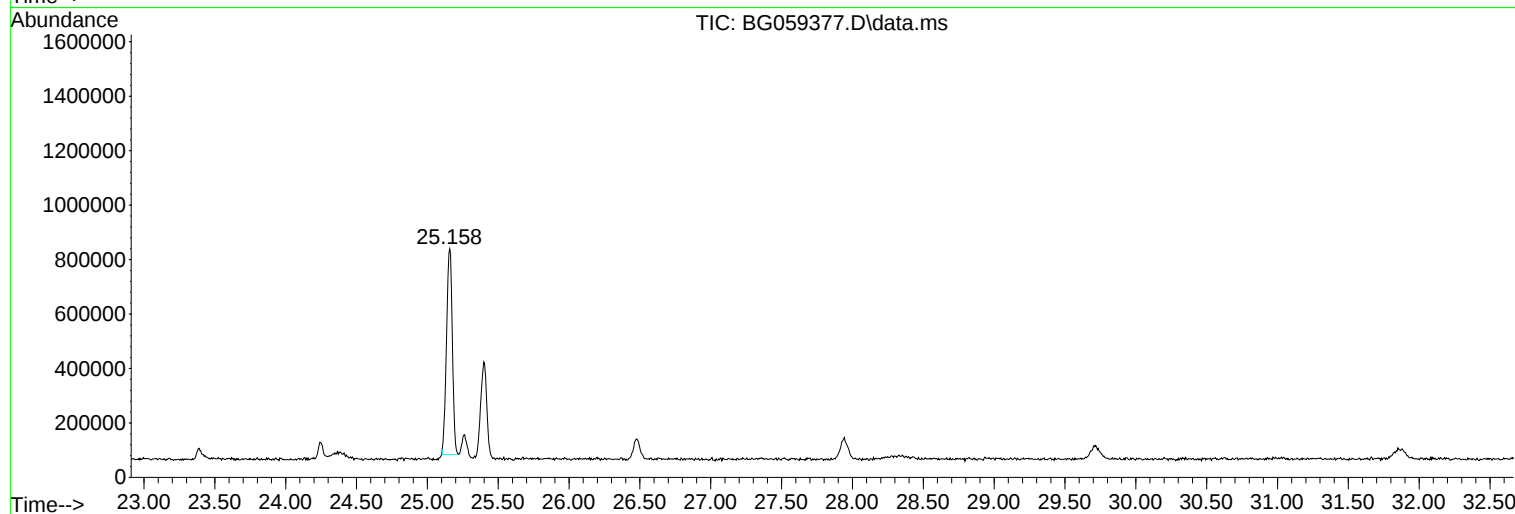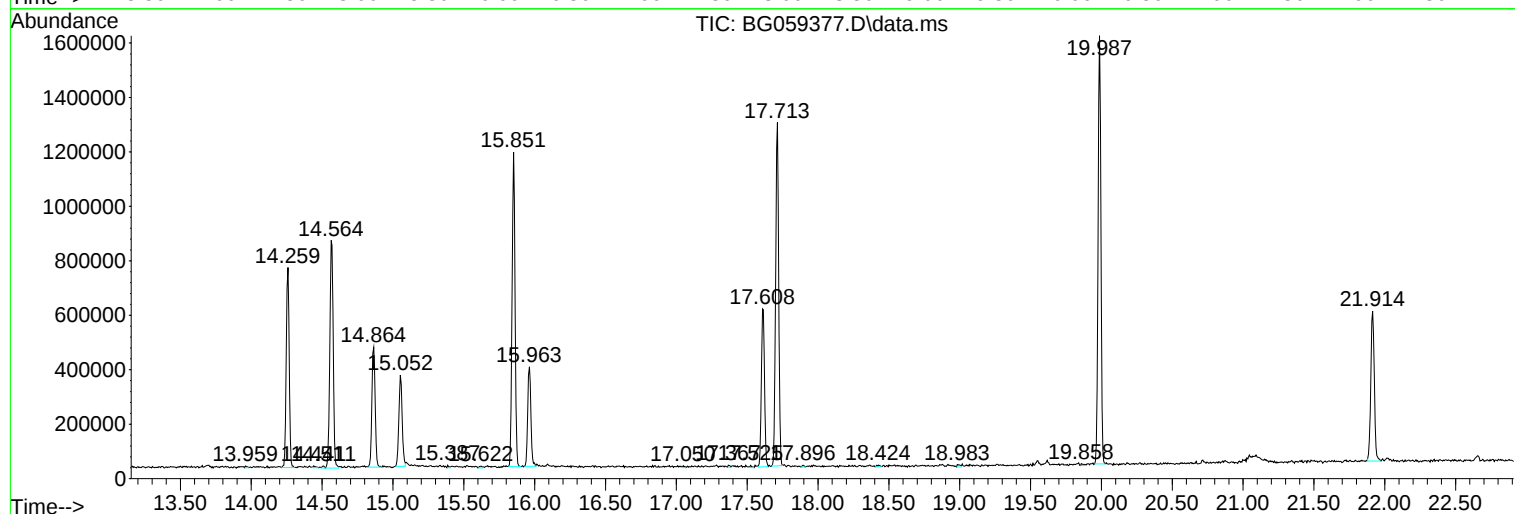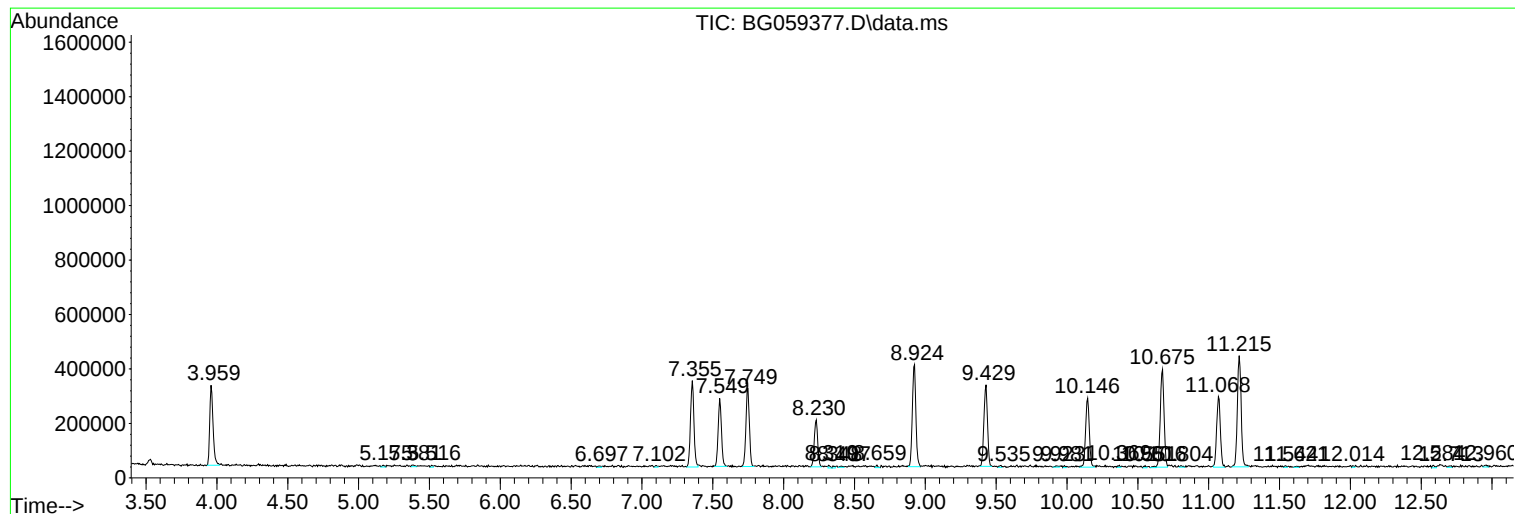

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059377.D
Acq On : 8 Oct 2023 15:53
Operator : MA/JU
Sample : PB156054BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059377.D
Acq On : 8 Oct 2023 15:53
Operator : MA/JU
Sample : PB156054BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------