

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059378.D
 Acq On : 8 Oct 2023 16:33
 Operator : MA/JU
 Sample : PB155973BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK973

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.958	93	97	108	rBV	313159	502337	20.91%	2.331%
2	4.404	170	173	176	rBV2	7716	8184	0.34%	0.038%
3	4.575	199	202	203	rBV	6376	6266	0.26%	0.029%
4	6.243	482	486	487	rVB	6807	6433	0.27%	0.030%
5	6.561	537	540	543	rVB	5077	6657	0.28%	0.031%
6	6.602	543	547	548	rBV	6281	7001	0.29%	0.032%
7	6.684	559	561	565	rVB	7746	7667	0.32%	0.036%
8	7.242	655	656	660	rVB	6578	6721	0.28%	0.031%
9	7.354	669	675	682	rVB	324728	551485	22.96%	2.559%
10	7.548	702	708	717	rVB	265460	430683	17.93%	1.998%
11	7.747	735	742	749	rBV	307291	527187	21.95%	2.446%
12	8.229	818	824	829	rBV	181338	309082	12.87%	1.434%
13	8.923	935	942	948	rBV	405146	703271	29.27%	3.263%
14	9.428	1021	1028	1035	rBV	314262	575157	23.94%	2.669%
15	10.145	1143	1150	1156	rBV	273571	480315	19.99%	2.229%
16	10.673	1232	1240	1248	rBV	414017	729580	30.37%	3.385%
17	11.067	1301	1307	1315	rVB	280154	505629	21.05%	2.346%
18	11.214	1325	1332	1339	rBV	437173	791209	32.94%	3.671%
19	12.007	1464	1467	1470	rBV	7760	7285	0.30%	0.034%
20	12.806	1600	1603	1604	rBV	6581	6372	0.27%	0.030%
21	13.153	1658	1662	1663	rBV	6753	8070	0.34%	0.037%
22	13.294	1682	1686	1689	rBV	5919	8329	0.35%	0.039%
23	13.688	1750	1753	1758	rVB2	6710	9811	0.41%	0.046%
24	13.881	1785	1786	1789	rBV	7822	8163	0.34%	0.038%
25	14.257	1843	1850	1858	rBV	840232	1184885	49.32%	5.498%
26	14.563	1896	1902	1910	rVB	913777	1478036	61.53%	6.858%
27	14.863	1946	1953	1960	rVB	505681	776421	32.32%	3.602%
28	14.992	1974	1975	1978	rBV	6779	6444	0.27%	0.030%
29	15.051	1980	1985	1994	rVV	358367	595113	24.77%	2.761%
30	15.344	2034	2035	2039	rVB	9118	8509	0.35%	0.039%
31	15.850	2115	2121	2128	rBV	1192102	1838039	76.51%	8.528%
32	15.961	2134	2140	2153	rBV	403255	636194	26.48%	2.952%
33	16.778	2277	2279	2282	rBV	7423	9185	0.38%	0.043%
34	16.866	2292	2294	2298	rBV	6614	9784	0.41%	0.045%
35	17.477	2396	2398	2401	rBV	5740	6359	0.26%	0.030%
36	17.612	2415	2421	2428	rBV	667281	962515	40.07%	4.466%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
 Data File : BG059378.D
 Acq On : 8 Oct 2023 16:33
 Operator : MA/JU
 Sample : PB155973BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK973

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	17.712	2432	2438	2447	rVB2	1361722	2053691	85.49%	9.529%
38	18.147	2510	2512	2514	rVB	6163	6506	0.27%	0.030%
39	19.551	2747	2751	2754	rBV5	18739	26452	1.10%	0.123%
40	19.986	2819	2825	2833	rBV	1624915	2317256	96.46%	10.752%
41	20.104	2844	2845	2848	rBV	12684	8624	0.36%	0.040%
42	21.913	3147	3153	3163	rVB2	603138	1023460	42.60%	4.749%
43	25.156	3695	3705	3715	rBV3	818357	2402306	100.00%	11.146%




Sum of corrected areas: 21552673

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059378.D
Acq On : 8 Oct 2023 16:33
Operator : MA/JU
Sample : PB155973BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK973

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

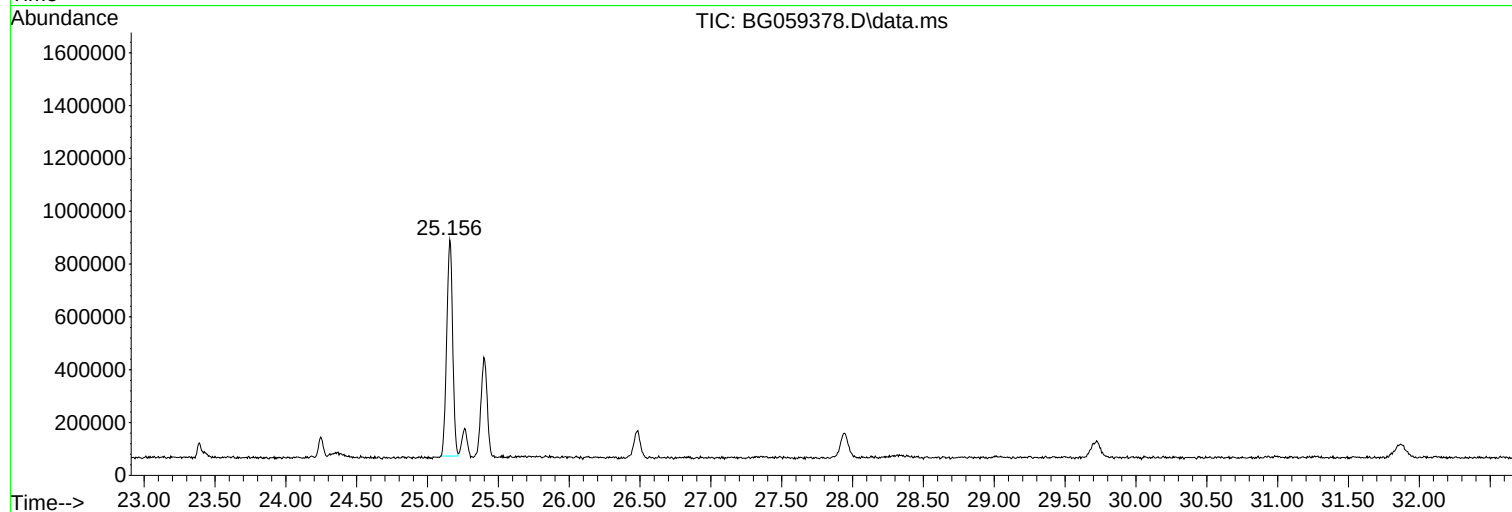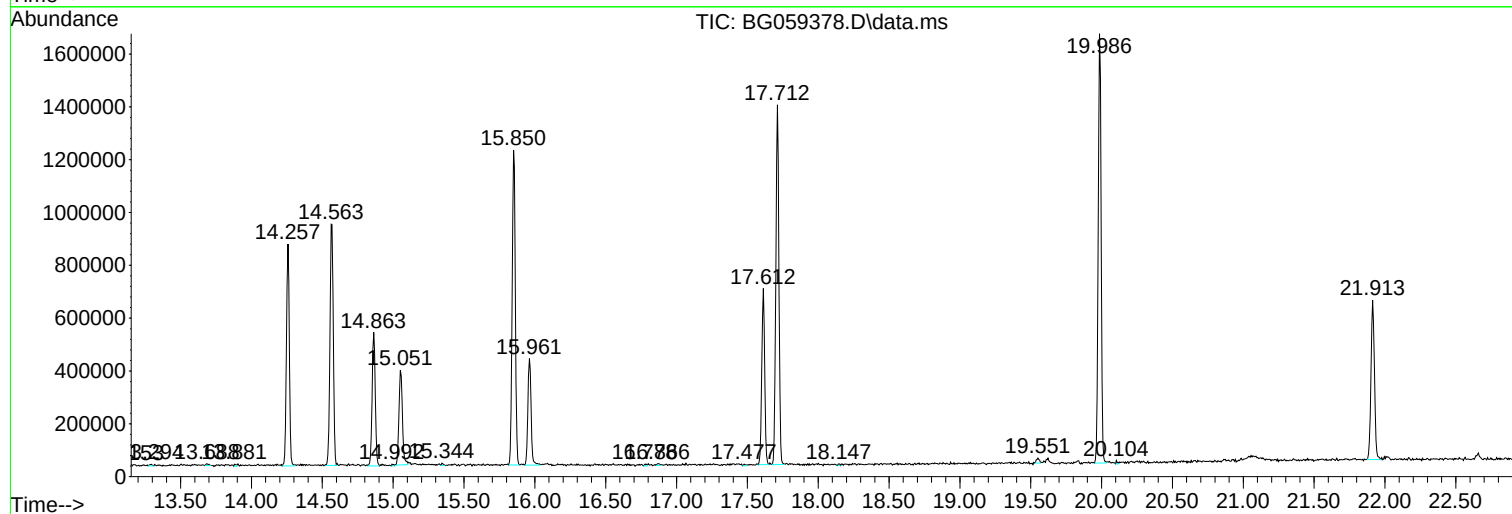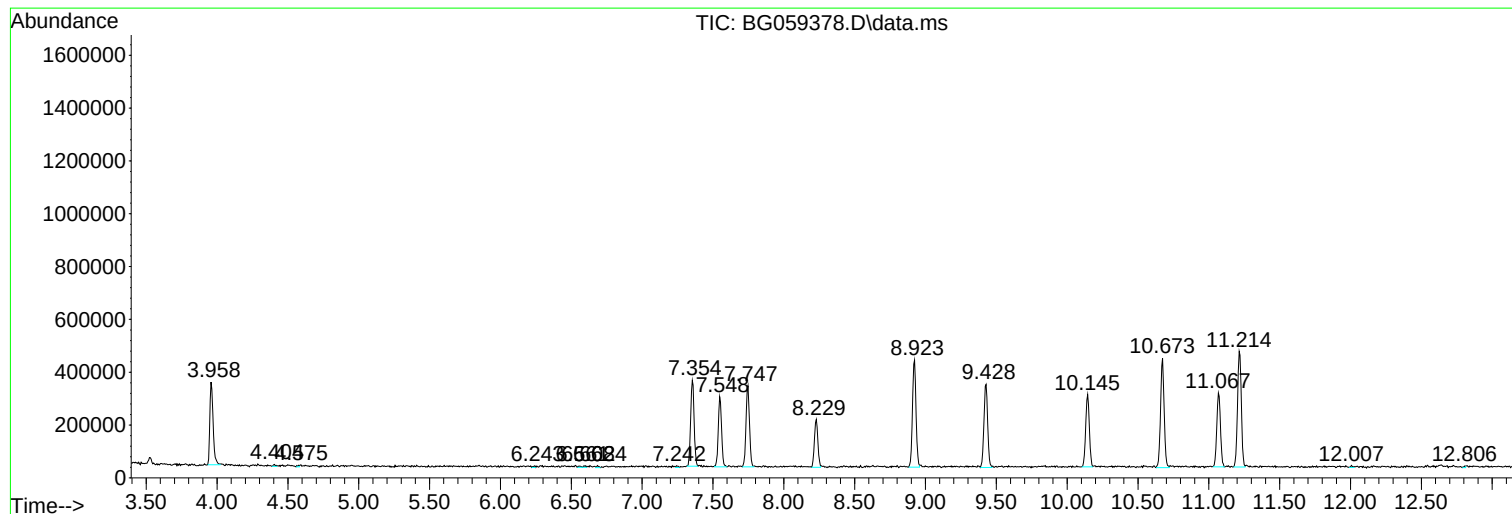

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059378.D
Acq On : 8 Oct 2023 16:33
Operator : MA/JU
Sample : PB155973BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK973

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100723\
Data File : BG059378.D
Acq On : 8 Oct 2023 16:33
Operator : MA/JU
Sample : PB155973BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK973

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc