


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100918\
 Data File : BG037221.D
 Acq On : 9 Oct 2018 16:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

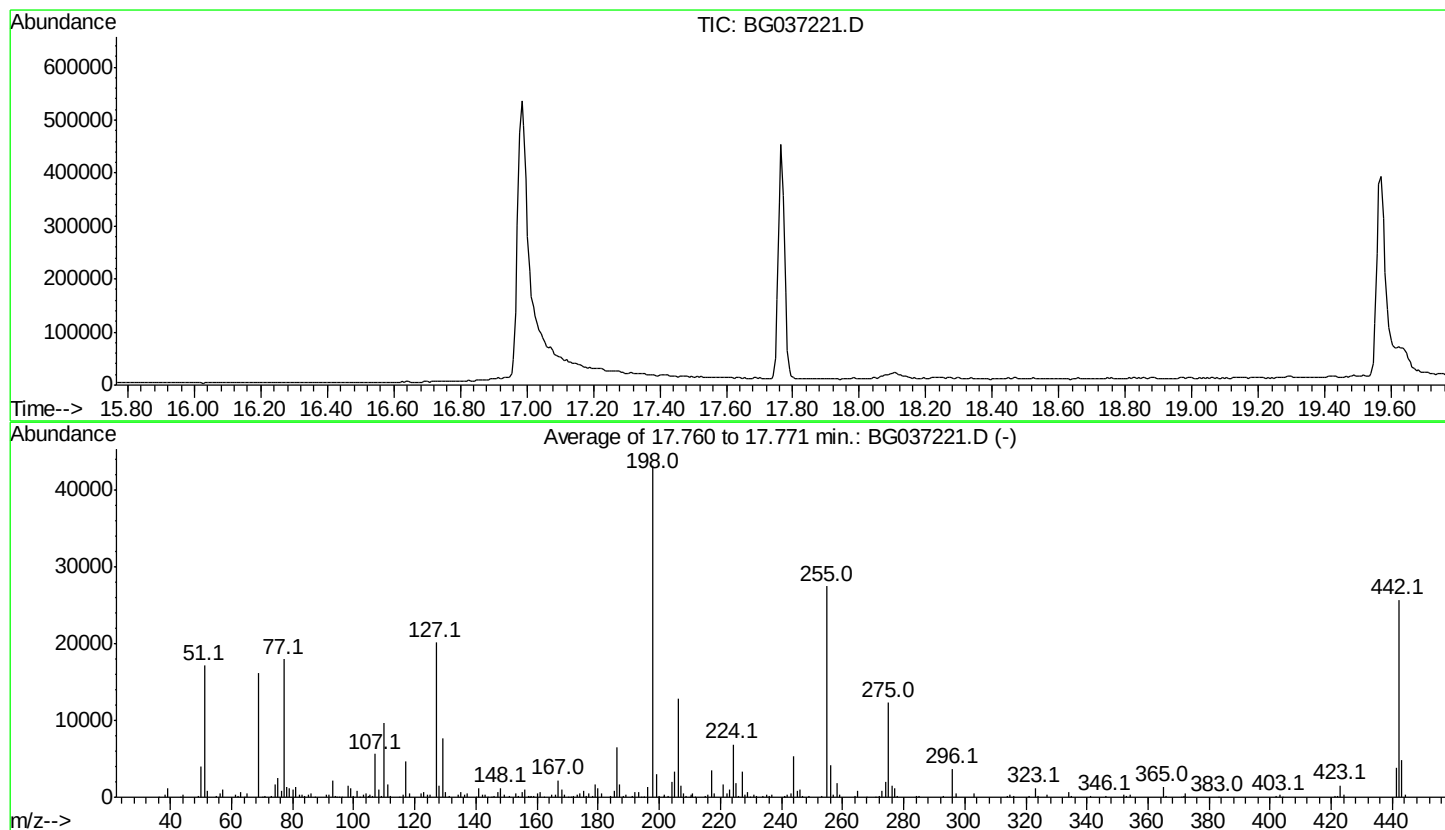

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	17076	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.3	16113	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	46.6	20121	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43144	PASS
199	198	5	9	7.0	3016	PASS
275	198	10	60	28.4	12251	PASS
365	198	1	100	3.2	1377	PASS
441	198	0.01	100	8.9	3859	PASS
442	198	50	100	59.5	25653	PASS
443	442	15	24	19.1	4904	PASS