

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100919\
 Data File : BG043123.D
 Acq On : 10 Oct 2019 4:36
 Operator : JU
 Sample : K5175-21
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 10 05:27:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 09 15:33:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	62798	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	253659	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.68	164	177348	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.42	188	451163	20.00	ng/ul	0.00
77) Chrysene-d12	21.69	240	553886	20.00	ng/ul	0.00
85) Perylene-d12	24.91	264	665098	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.50	96	6502	5.01	ng/uL	0.00
5) Phenol-d5	7.23	99	115674	24.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.38	67	71355	27.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.59	132	99770	26.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.77	113	84461	21.10	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	50526	28.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	58913	28.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	97906	22.99	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	105517	23.80	ng/ul	0.00
43) Dimethylphthalate-d6	14.08	166	384016	26.93	ng/ul	0.00
46) Acenaphthylene-d8	14.37	160	419835	27.07	ng/ul	0.00
51) 4-Nitrophenol-d4	14.89	143	30885	16.33	ng/ul	0.00
57) Fluorene-d10	15.67	176	326090	26.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.84	200	1011	0.35	ng/ul	0.06
70) Anthracene-d10	17.52	188	562599	26.40	ng/ul	0.00
78) Pyrene-d10	19.81	212	755288	27.65	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.69	264	894705	27.22	ng/ul	0.01

Target Compounds


					Ovalue
6) Phenol	7.26	94	13535	2.855 ng/ul	96
44) Dimethylphthalate	14.12	163	127742	9.276 ng/ul	98
69) Phenanthrene	17.46	178	167874	7.209 ng/ul	99
71) Anthracene	17.46	178	167788	6.963 ng/ul	99
74) Carbazole	17.83	167	29977	1.455 ng/ul	99
76) Fluoranthene	19.47	202	259824	8.745 ng/ul	99
79) Pyrene	19.83	202	221766	6.510 ng/ul	98
82) Benzo(a)anthracene	21.67	228	192240	5.187 ng/ul	98
84) Chrysene	21.74	228	145737	4.178 ng/ul	97
87) Benzo(b)fluoranthene	23.89	252	151586	3.830 ng/ul	99
88) Benzo(k)fluoranthene	23.89	252	151586	3.919 ng/ul	96
90) Benzo(a)pyrene	24.76	252	115740	3.055 ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100919\
Data File : BG043123.D
Acq On : 10 Oct 2019 4:36
Operator : JU
Sample : K5175-21
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 10 05:27:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 09 15:33:22 2019
Response via : Initial Calibration

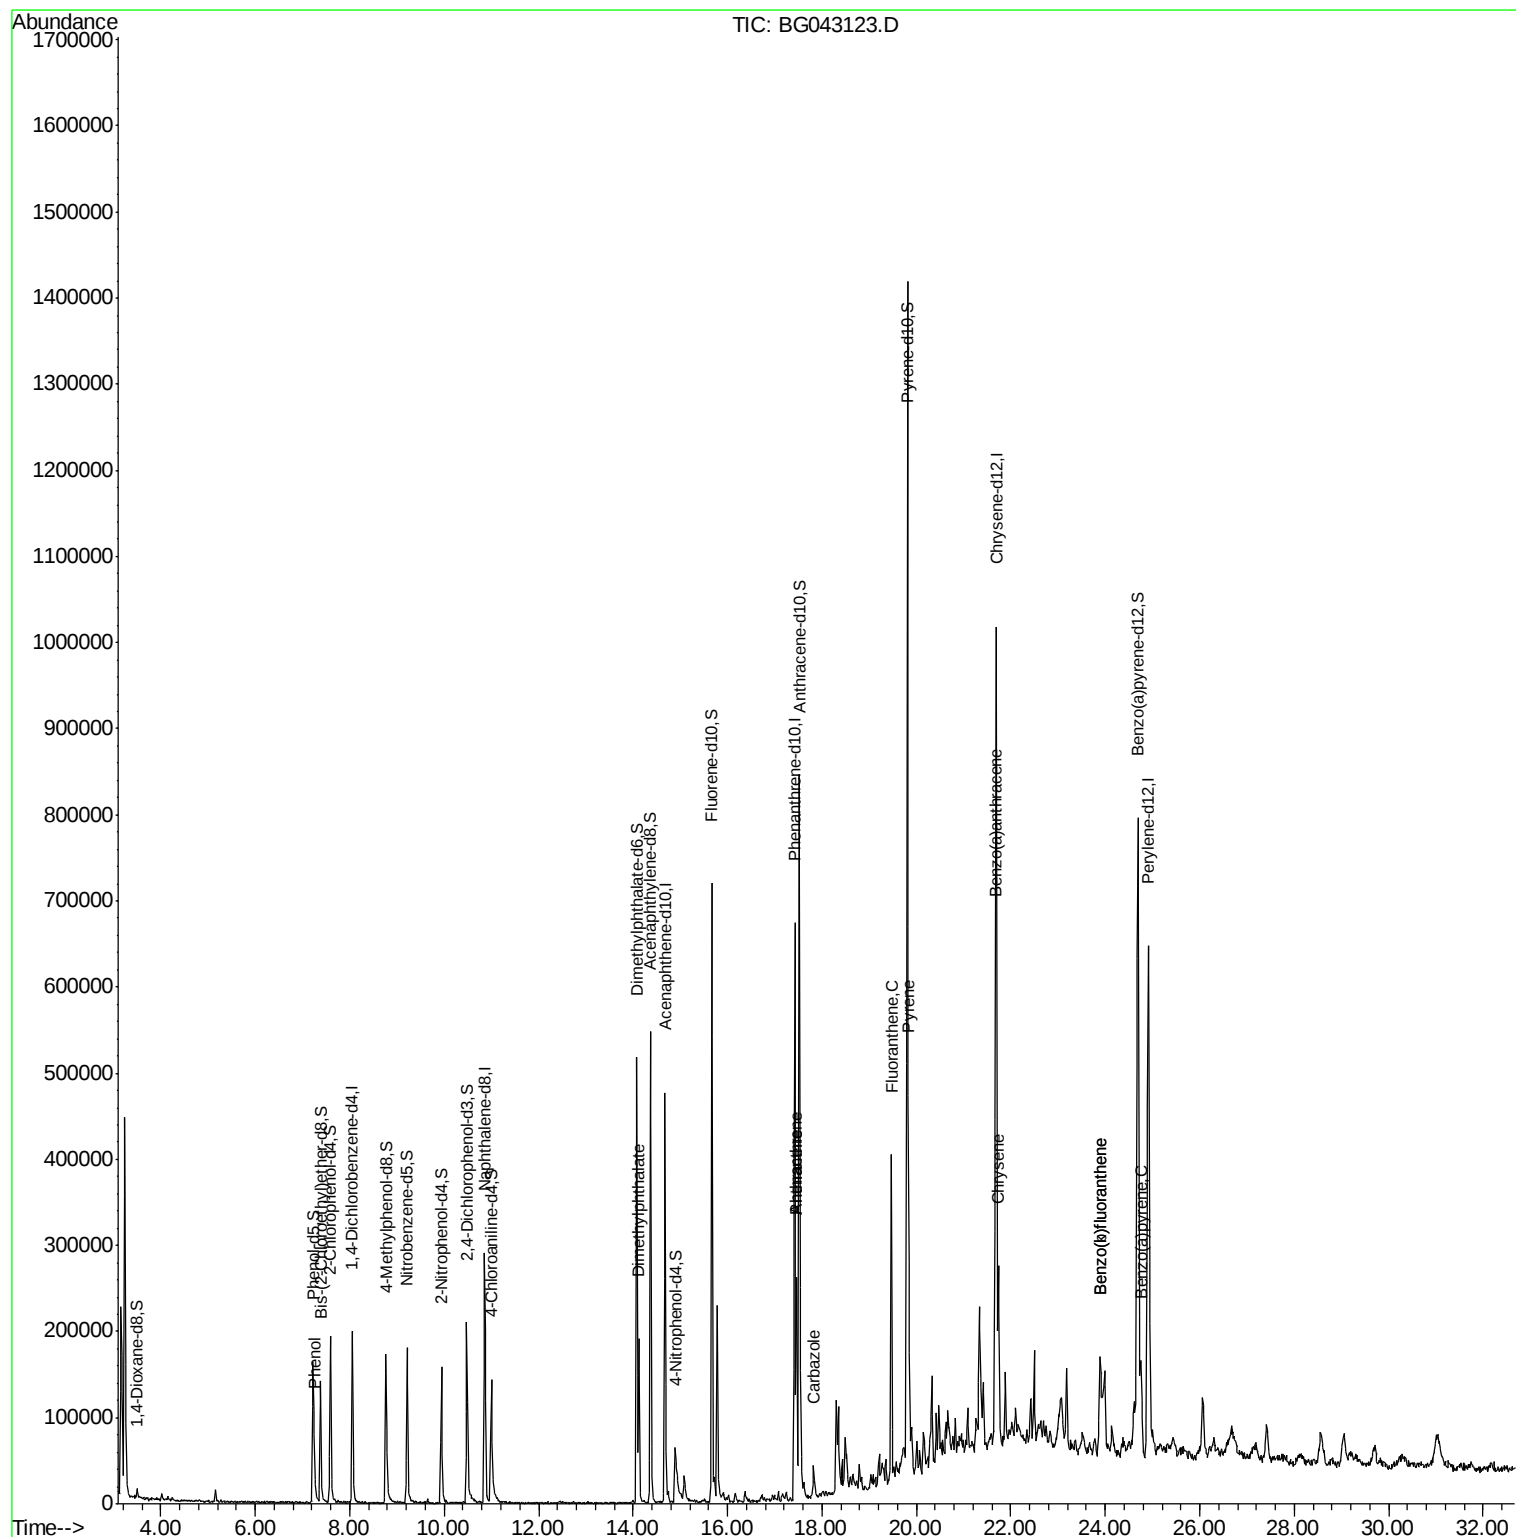



#6

Phenol

Concen: 2.855 ng/ul

RT: 7.26 min Scan# 709

Delta R.T. 0.01 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36

Instrument :

BNA_G

ClientSampleId :





Tot Ion: 94 Resp: 13535

Ion Ratio Lower Upper

94 100

65 30.8 27.2 40.8

66 50.8 38.7 58.1

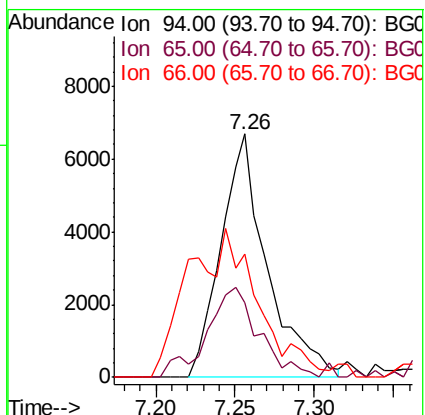

#44

Dimethylphthalate

Concen: 9.276 ng/ul

RT: 14.12 min Scan# 1878

Delta R.T. -0.00 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36




Tgt Ion: 163 Resp: 127742


Ion Ratio Lower Upper

163 100

194 3.8 3.6 5.4

164 9.9 8.6 12.8

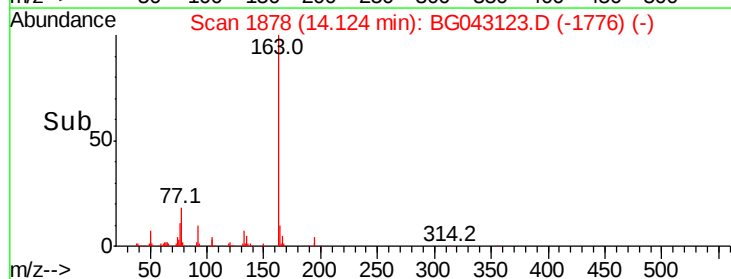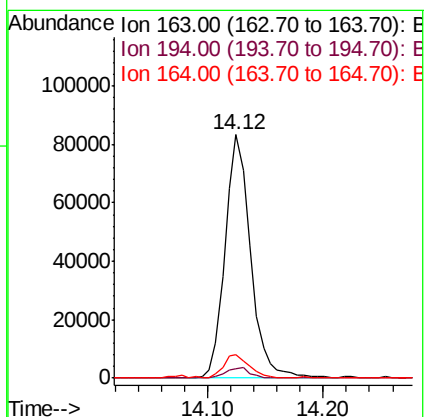



#69

Phenanthrene

Concen: 7.209 ng/ul

RT: 17.46 min Scan# 2446

Delta R.T. -0.00 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36

Instrument :

BNA_G

ClientSampleId :


Tot Ion:178 Resp: 167874

Ion Ratio Lower Upper

178 100

179 16.5 13.0 19.4




176 18.8 15.2 22.8



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

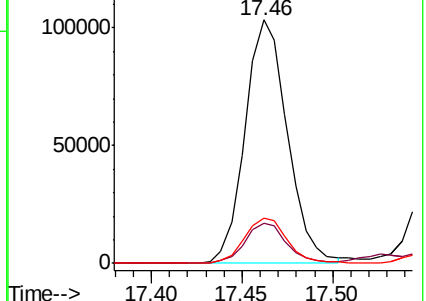

#71

Anthracene

Concen: 6.963 ng/ul

RT: 17.46 min Scan# 2446

Delta R.T. -0.09 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36


Tgt Ion:178 Resp: 167788

Ion Ratio Lower Upper

178 100

179 16.5 13.0 19.4



176 18.8 15.4 23.2




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

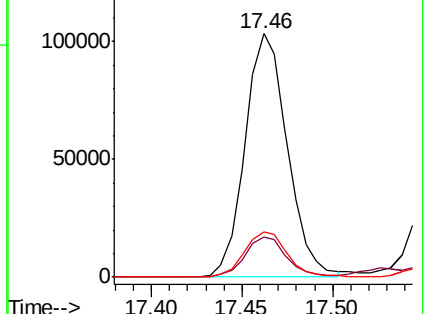



#74

Carbazole

Concen: 1.455 ng/ul

RT: 17.83 min Scan# 2508

Delta R.T. -0.00 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36


Instrument :

BNA_G

ClientSampleId :

Tot Ion:167 Resp: 29977

Ion	Ratio	Lower	Upper
167	100		
166	21.1	17.4	26.0
139	11.6	9.8	14.8



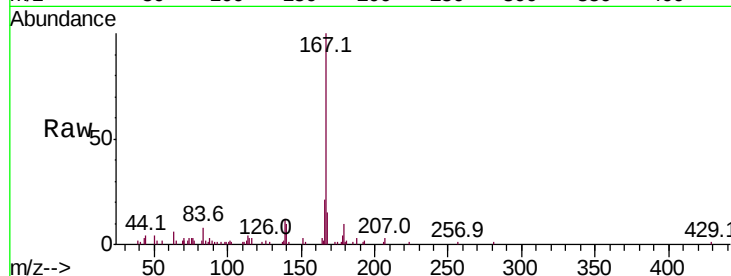


Abundance

Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

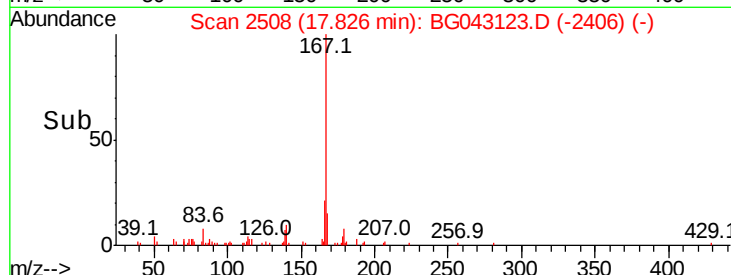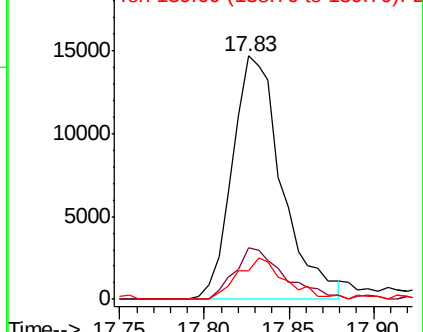

#76

Fluoranthene

Concen: 8.745 ng/ul

RT: 19.47 min Scan# 2788


Delta R.T. -0.00 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36

Tgt Ion:202 Resp: 259824

Ion	Ratio	Lower	Upper
202	100		
101	6.8	5.0	7.6
100	6.1	4.6	7.0






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B




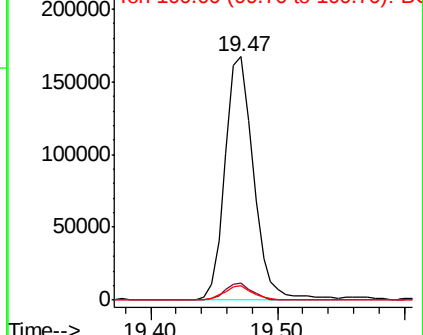


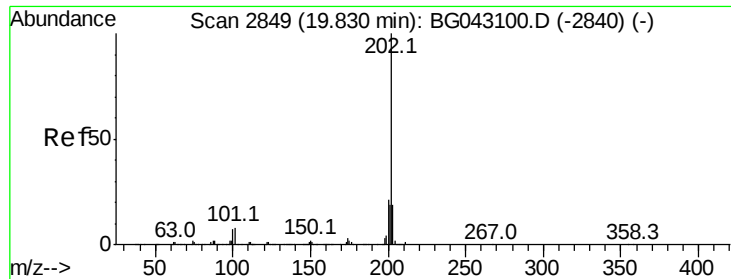

#79
 Pvrene
 Concen: 6.510 ng/ul
 RT: 19.83 min Scan# 2849
 Delta R.T. -0.00 min
 Lab File: BG043123.D
 Acq: 10 Oct 2019 4:36




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:	202	Resp:	221766
Ion	Ratio	Lower	Upper
202	100		
101	6.7	6.2	9.4
100	6.9	5.4	8.2

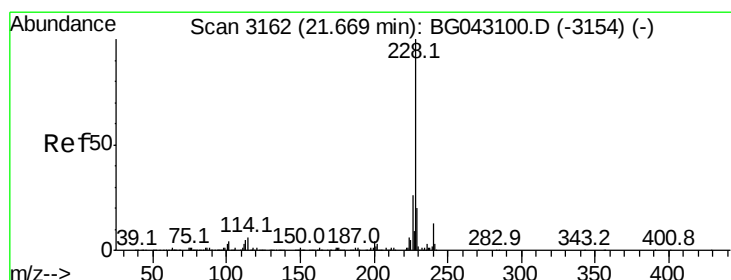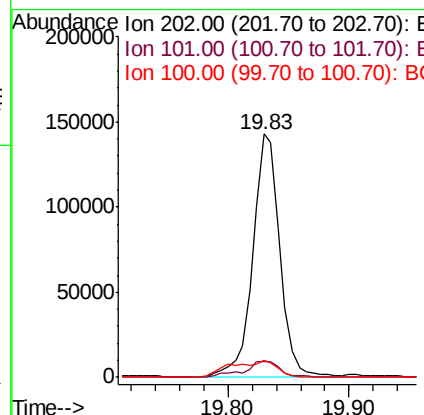

#82
 Benzo(a)anthracene
 Concen: 5.187 ng/ul
 RT: 21.67 min Scan# 3162
 Delta R.T. -0.00 min
 Lab File: BG043123.D
 Acq: 10 Oct 2019 4:36

Tgt Ion:	228	Resp:	192240
Ion	Ratio	Lower	Upper
228	100		
229	21.8	16.2	24.2
226	25.9	21.0	31.4

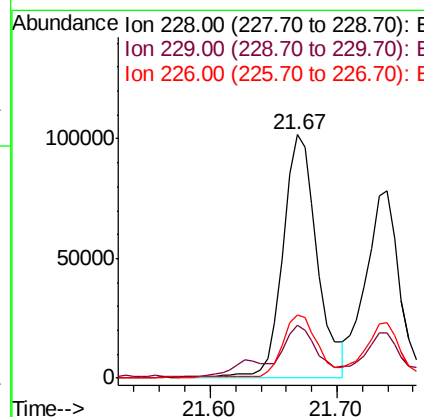

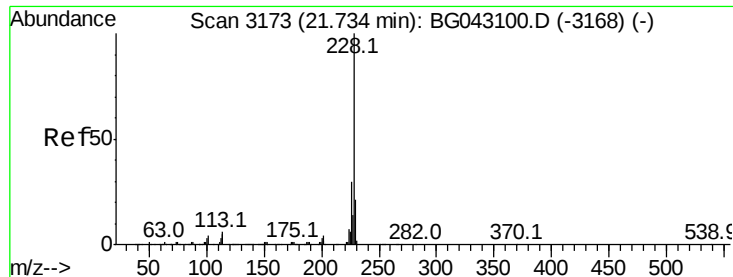

#84

Chrysene

Concen: 4.178 ng/ul

RT: 21.74 min Scan# 3174

Delta R.T. 0.01 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36


Instrument :

BNA_G

ClientSampleId :

Tot Ion:228 Resp: 145737

Ion	Ratio	Lower	Upper
228	100		
226	29.9	24.2	36.2
229	24.1	16.6	25.0



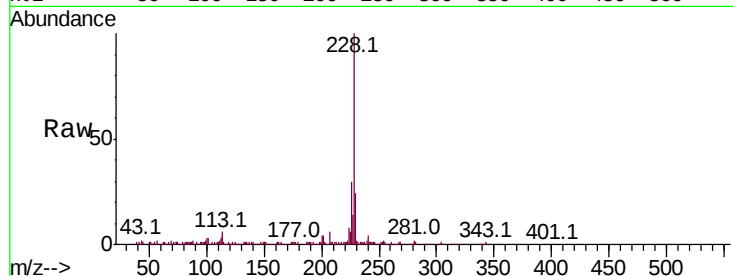


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

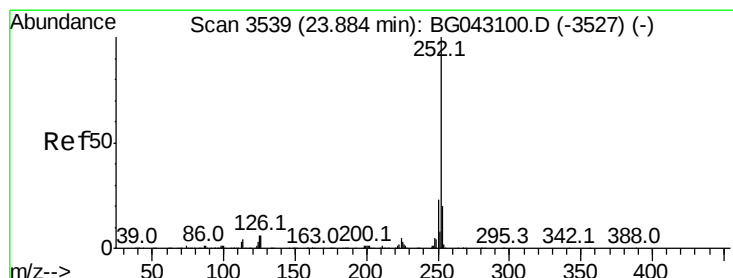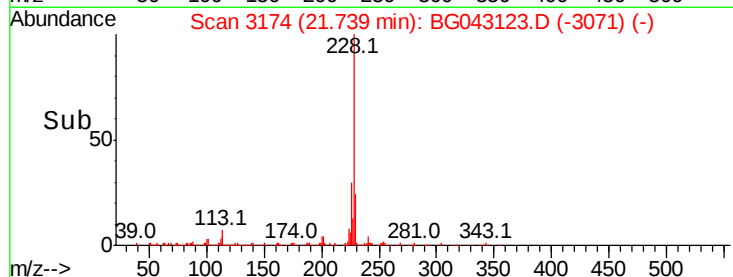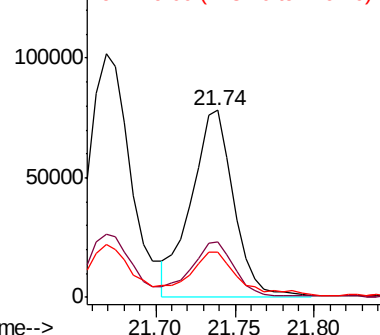

#87

Benzo(b)fluoranthene

Concen: 3.830 ng/ul

RT: 23.89 min Scan# 3540


Delta R.T. 0.01 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36

Tgt Ion:252 Resp: 151586

Ion	Ratio	Lower	Upper
252	100		
253	20.9	16.4	24.6
125	6.2	4.6	7.0


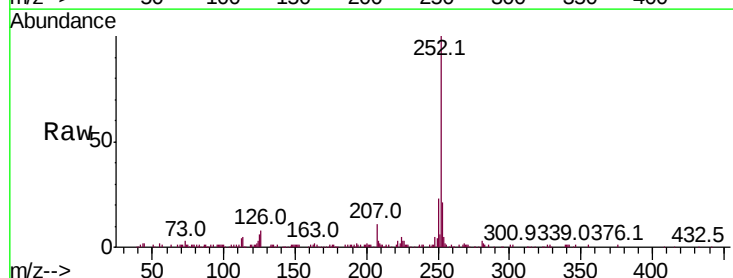



Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

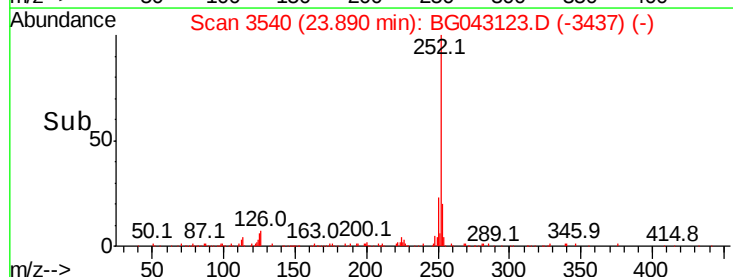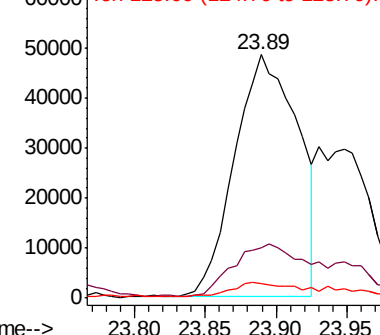



#88

Benzo(k)fluoranthene

Concen: 3.919 ng/ul

RT: 23.89 min Scan# 3540

Delta R.T. -0.07 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36

Instrument :

BNA_G

ClientSampleId :


Tot Ion:252 Resp: 151586

Ion Ratio Lower Upper

252 100

253 20.9 18.4 27.6




125 6.2 4.4 6.6

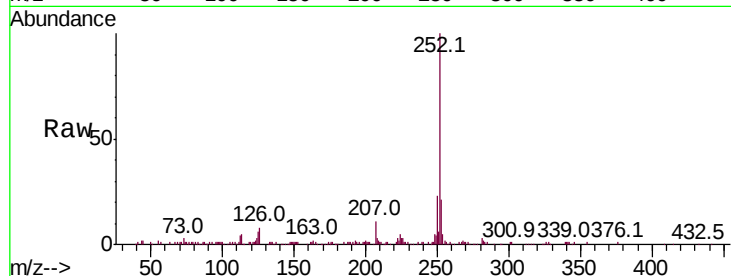

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

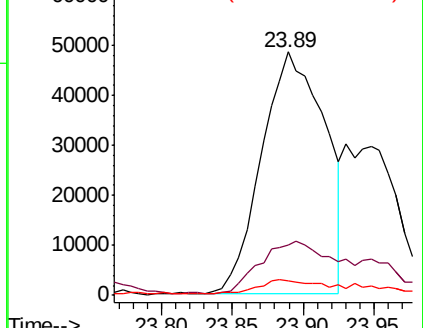

#90

Benzo(a)pyrene

Concen: 3.055 ng/ul

RT: 24.76 min Scan# 3688

Delta R.T. 0.01 min

Lab File: BG043123.D

Acq: 10 Oct 2019 4:36


Tgt Ion:252 Resp: 115740

Ion Ratio Lower Upper

252 100

253 19.9 18.9 28.3

125 7.7 5.3 7.9



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

