
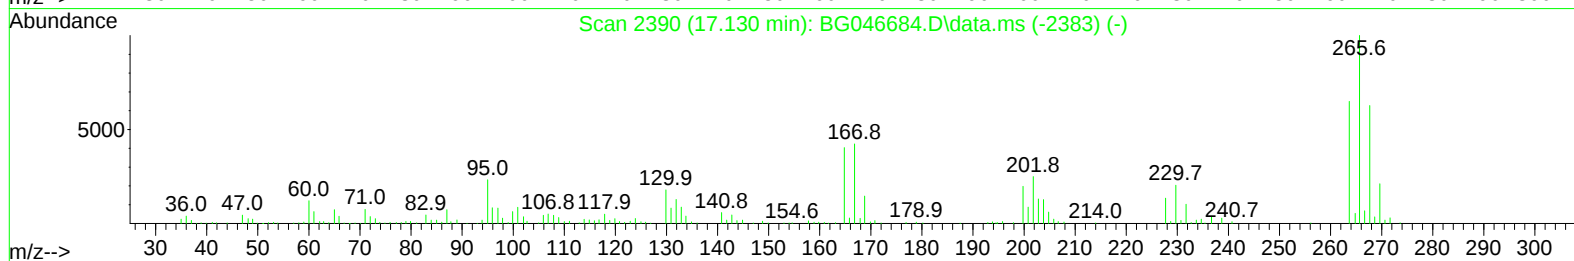
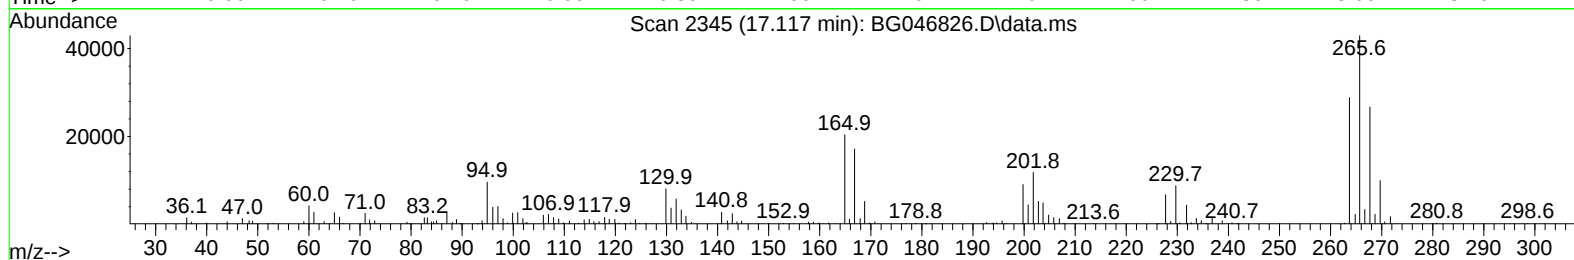


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100920\
Data File : BG046826.D
Acq On : 9 Oct 2020 8:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 06:17:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

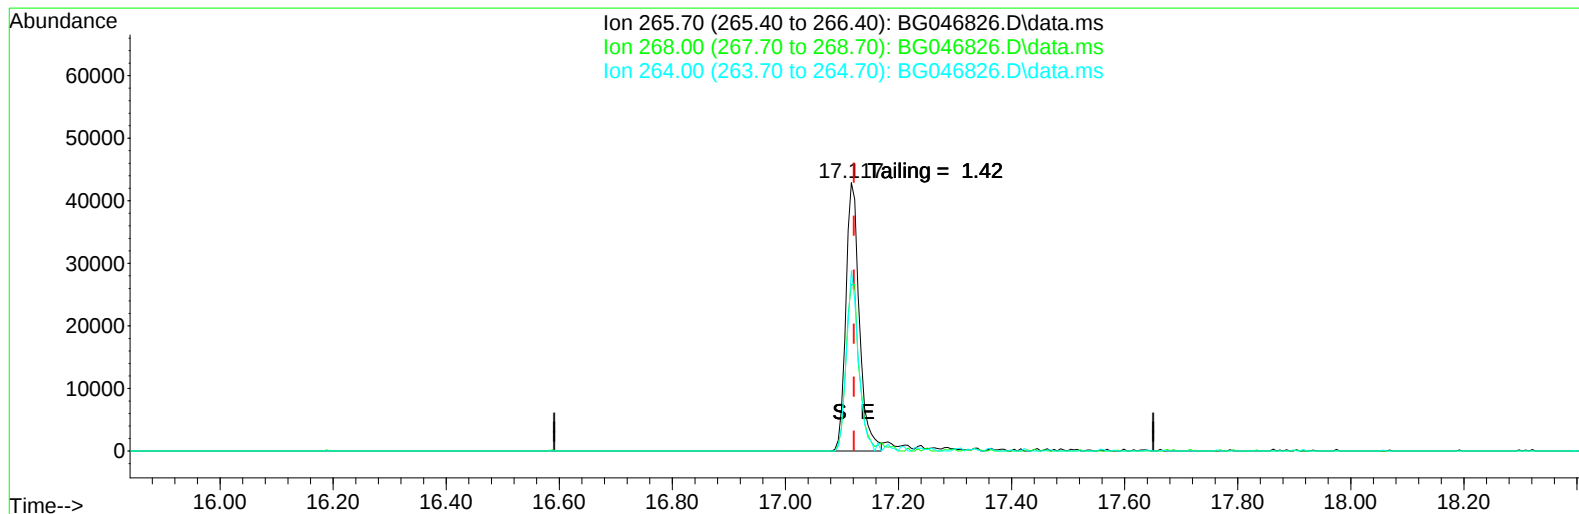

TIC: BG046826.D\data.ms

(70) Pentachlorophenol (C)




17.117min (-0.004) 122028.55 ng m

response 73739

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.15
264.00	61.60	67.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100920\
Data File : BG046826.D
Acq On : 9 Oct 2020 8:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 06:17:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

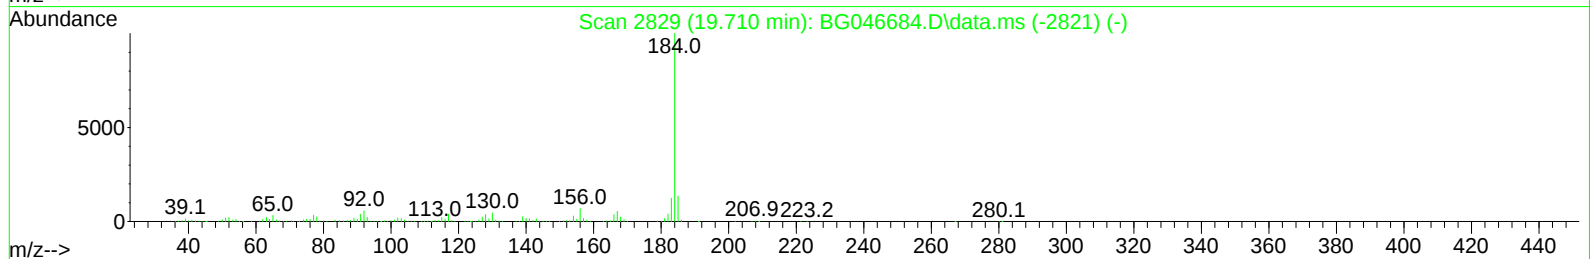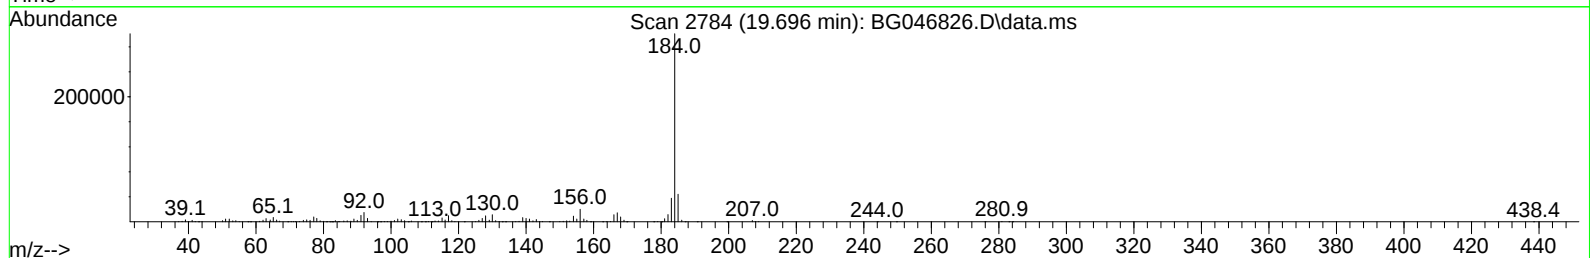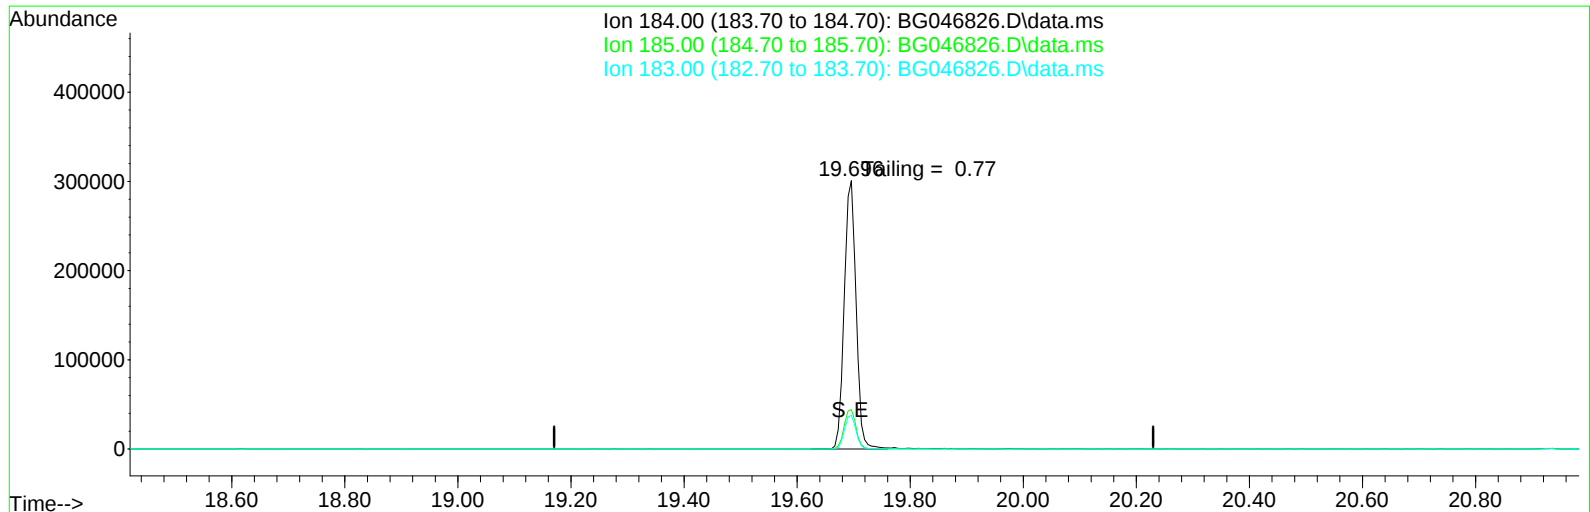

TIC: BG046826.D\data.ms

(77) Benzidine**19.696min (-0.004) 68959.87 ng m****response 437897**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	12.54
0.00	0.00	0.00