


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100920\
 Data File : BG046826.D
 Acq On : 9 Oct 2020 8:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 07 11:38:17 2020

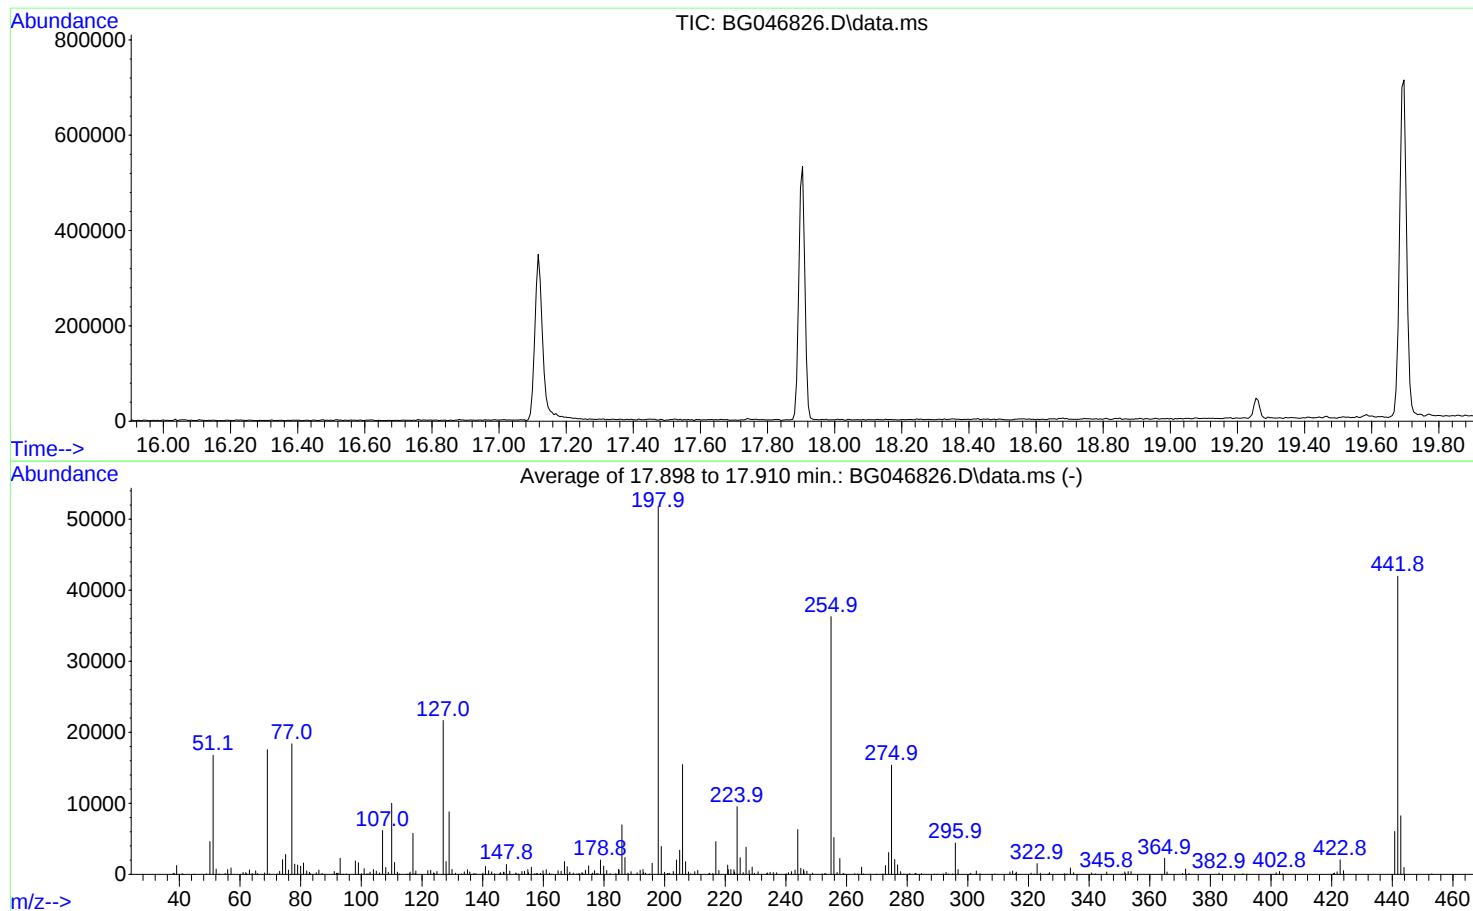

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	16767	PASS
68	69	0.00	2	1.2	208	PASS
69	198	0.00	100	33.9	17559	PASS
70	69	0.00	2	0.4	71	PASS
127	198	10	80	41.8	21661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51787	PASS
199	198	5	9	7.6	3914	PASS
275	198	10	60	29.7	15364	PASS
365	198	1	100	4.3	2251	PASS
441	198	0.01	100	11.7	6037	PASS
442	198	50	100	81.0	41973	PASS
443	442	15	24	19.6	8239	PASS