

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059393.D
 Acq On : 9 Oct 2023 11:35
 Operator : MA/JU
 Sample : PB155981BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK981

Quant Time: Oct 09 22:44:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 07 22:45:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.226	152	42809	20.000	ng/ul	0.00
20) Naphthalene-d8	11.070	136	214604	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.859	164	152487	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.609	188	356634	20.000	ng/ul	0.00
79) Chrysene-d12	21.910	240	315711	20.000	ng/ul	0.00
88) Perylene-d12	25.400	264	370426	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.525	96	10373	8.639	ng/uL	0.00
4) Pyridine-d5	3.960	84	140845	40.755	ng/ul	0.00
7) Phenol-d5	7.350	99	183162	38.749	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.544	67	107700	40.311	ng/ul	0.00
11) 2-Chlorophenol-d4	7.744	132	135915	41.113	ng/ul	0.00
15) 4-Methylphenol-d8	8.919	113	139027	37.750	ng/ul	0.00
21) Nitrobenzene-d5	9.424	128	73972	40.491	ng/ul	0.00
24) 2-Nitrophenol-d4	10.141	143	82358	41.652	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.670	165	140996	39.507	ng/ul	0.00
31) 4-Chloroaniline-d4	11.216	131	218316	38.510	ng/ul	0.00
46) Dimethylphthalate-d6	14.260	166	508162	40.677	ng/ul	0.00
49) Acenaphthylene-d8	14.565	160	582062	39.152	ng/ul	0.00
54) 4-Nitrophenol-d4	15.053	143	78598	33.573	ng/ul	0.00
60) Fluorene-d10	15.852	176	463279	38.851	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.964	200	77814	33.047	ng/ul	0.00
73) Anthracene-d10	17.709	188	725853	41.490	ng/ul	0.00
81) Pyrene-d10	19.988	212	791047	41.361	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.153	264	809879	41.548	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.919	70	2961	1.062 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059393.D
Acq On : 9 Oct 2023 11:35
Operator : MA/JU
Sample : PB155981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK981


Quant Time: Oct 09 22:44:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 07 22:45:22 2023
Response via : Initial Calibration

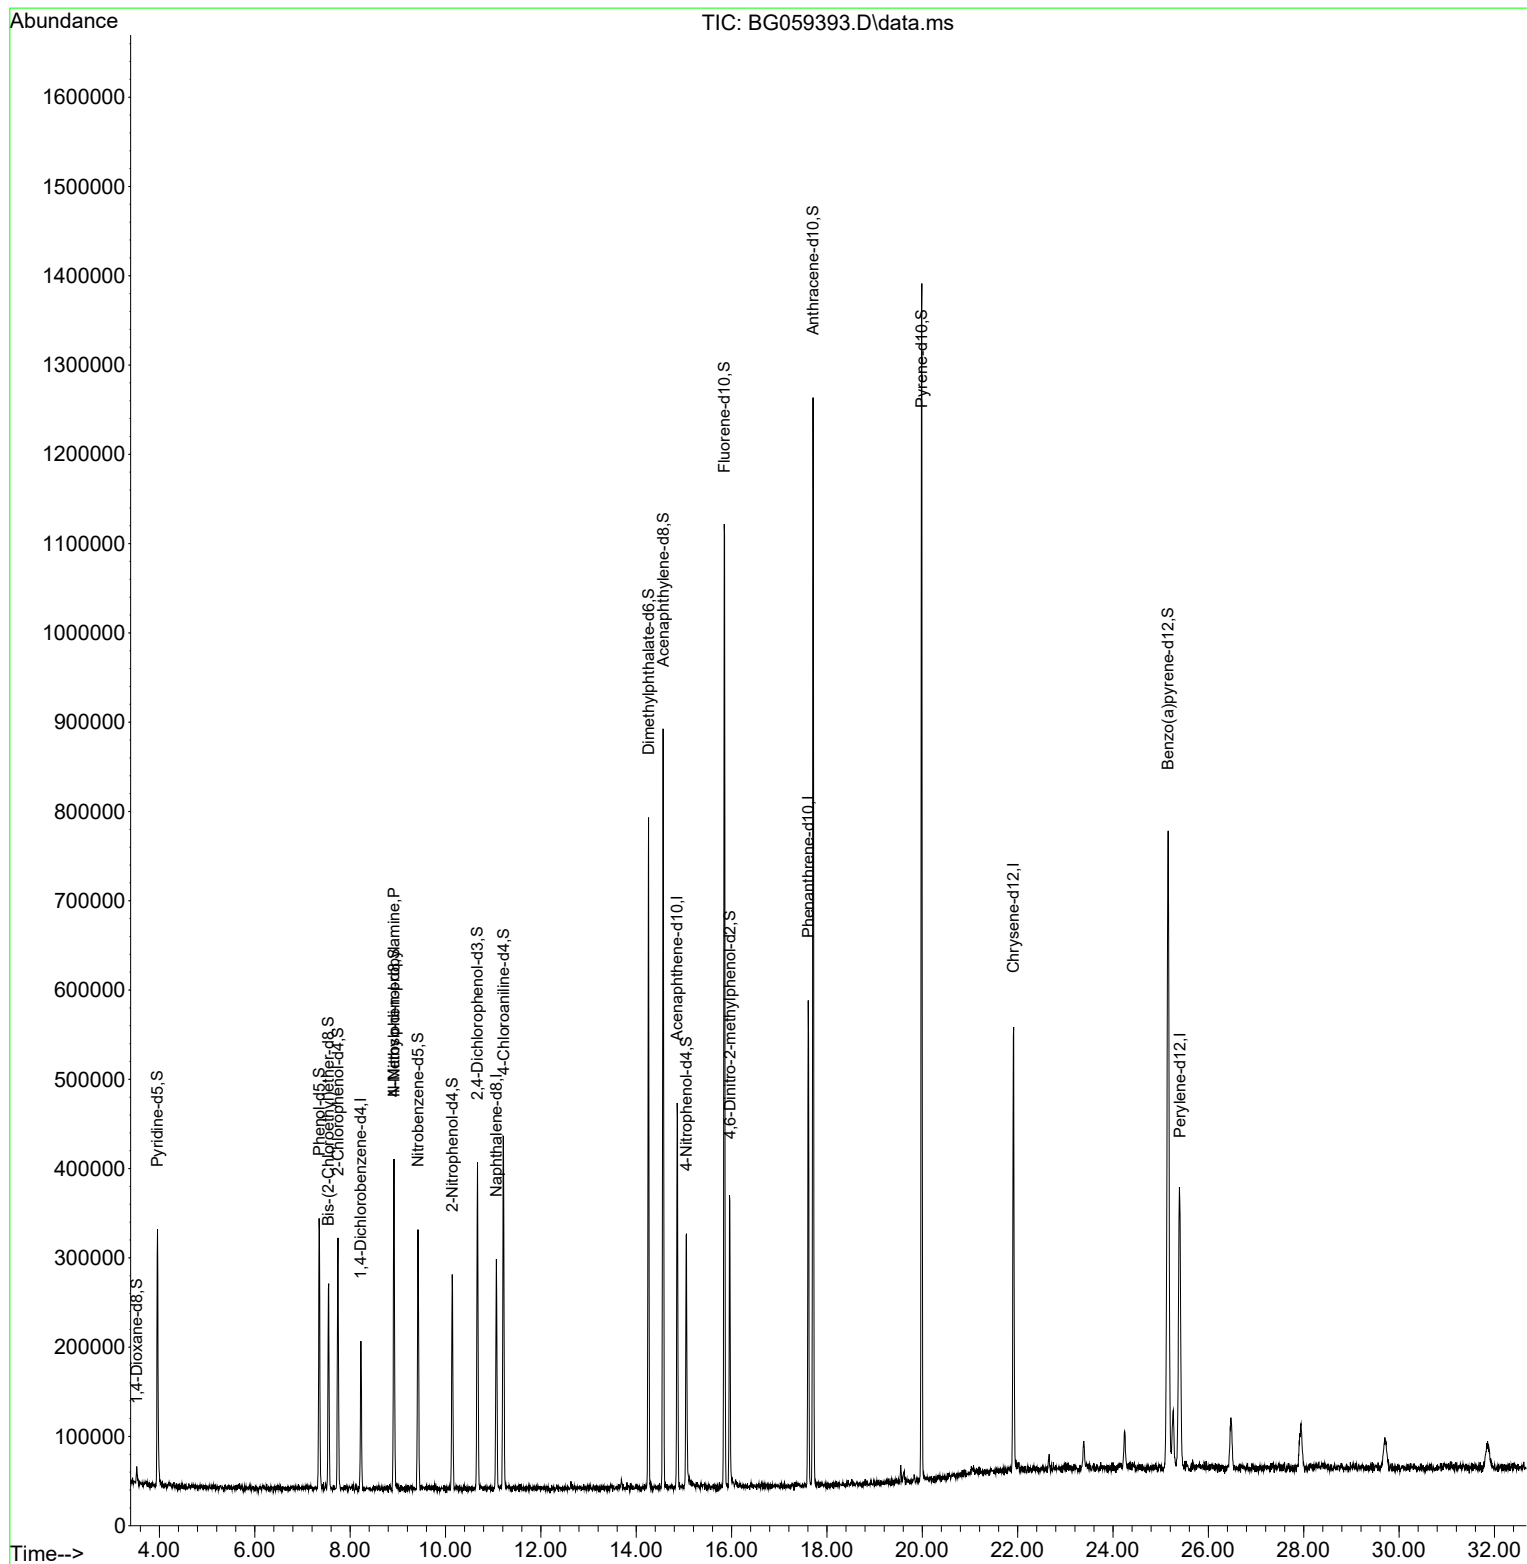

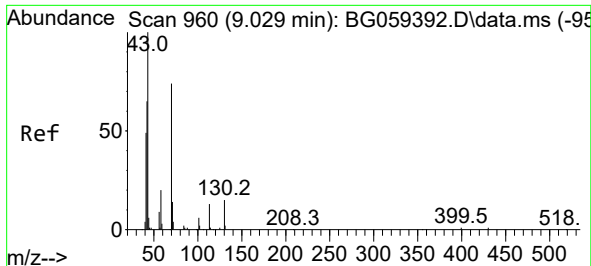

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.062 ng/ul
 RT: 8.919 min Scan# 941
 Delta R.T. -0.117 min
 Lab File: BG059393.D
 Acq: 9 Oct 2023 11:35

Instrument :
 BNA_G
 ClientSampleId :
 SBLK981

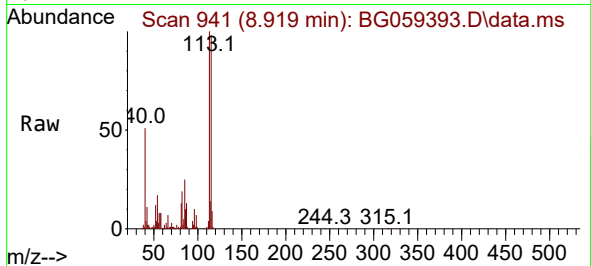

Tgt Ion:	70	Resp:	2961
Ion	Ratio	Lower	Upper
70	100		
42	352.2	58.2	87.4#
101	0.0	6.4	9.6#
130	0.0	15.4	23.0#

