

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059393.D
 Acq On : 9 Oct 2023 11:35
 Operator : MA/JU
 Sample : PB155981BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK981

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.960	92	97	107	rBV	287162	466195	23.24%	2.460%
2	4.818	240	243	244	rBV	5867	5840	0.29%	0.031%
3	6.023	445	448	450	rBV	5639	7819	0.39%	0.041%
4	6.093	457	460	462	rBV2	6066	8163	0.41%	0.043%
5	6.169	469	473	475	rBV	5600	8195	0.41%	0.043%
6	6.751	569	572	573	rBV	4965	5431	0.27%	0.029%
7	7.139	636	638	640	rBV	5393	5915	0.29%	0.031%
8	7.350	667	674	684	rVB	303387	522737	26.06%	2.759%
9	7.480	691	696	697	rBV3	5479	6583	0.33%	0.035%
10	7.550	701	708	716	rVV	230522	388838	19.38%	2.052%
11	7.650	722	725	726	rBV	7000	5820	0.29%	0.031%
12	7.744	735	741	751	rVB	282935	482830	24.07%	2.548%
13	7.979	778	781	785	rBV	5234	8585	0.43%	0.045%
14	8.108	800	803	805	rBV	6810	7164	0.36%	0.038%
15	8.226	817	823	830	rVB2	167680	282553	14.08%	1.491%
16	8.349	838	844	848	rBV2	3875	8034	0.40%	0.042%
17	8.725	906	908	911	rBV2	4202	5172	0.26%	0.027%
18	8.784	917	918	921	rVB	8251	5792	0.29%	0.031%
19	8.919	934	941	950	rBV2	372071	652343	32.52%	3.443%
20	9.166	982	983	985	rBV	7508	6921	0.34%	0.037%
21	9.424	1021	1027	1036	rVB	291504	508042	25.32%	2.681%
22	9.777	1085	1087	1089	rBV	8076	6137	0.31%	0.032%
23	10.141	1142	1149	1156	rBV	241587	428251	21.35%	2.260%
24	10.300	1173	1176	1177	rBV	6518	5760	0.29%	0.030%
25	10.670	1232	1239	1247	rVB	366528	642437	32.02%	3.390%
26	10.729	1247	1249	1252	rBV	5271	5926	0.30%	0.031%
27	10.870	1271	1273	1275	rBV	5298	6049	0.30%	0.032%
28	11.070	1300	1307	1315	rBV	256095	443684	22.12%	2.341%
29	11.211	1325	1331	1340	rBV	394752	704496	35.12%	3.718%
30	11.422	1364	1367	1368	rBV	6455	6957	0.35%	0.037%
31	11.457	1371	1373	1376	rBV	4691	5224	0.26%	0.028%
32	11.563	1387	1391	1394	rBV	8396	10150	0.51%	0.054%
33	11.769	1424	1426	1428	rBV	6012	5430	0.27%	0.029%
34	12.386	1529	1531	1533	rBV	5508	6464	0.32%	0.034%
35	12.632	1571	1573	1576	rVB3	8801	7151	0.36%	0.038%
36	13.020	1637	1639	1642	rBV	6246	7583	0.38%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059393.D
 Acq On : 9 Oct 2023 11:35
 Operator : MA/JU
 Sample : PB155981BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK981

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	13.138	1656	1659	1661	rVB	5091	5194	0.26%	0.027%
38	13.232	1673	1675	1678	rBV	5740	6871	0.34%	0.036%
39	13.279	1678	1683	1684	rVV	6005	7517	0.37%	0.040%
40	13.461	1711	1714	1716	rBV	7417	8396	0.42%	0.044%
41	13.825	1774	1776	1782	rVB	6753	13540	0.67%	0.071%
42	14.260	1843	1850	1855	rBV	750615	1043030	51.99%	5.504%
43	14.319	1858	1860	1864	rVB	6767	6290	0.31%	0.033%
44	14.565	1894	1902	1910	rBV	851202	1315198	65.56%	6.941%
45	14.859	1947	1952	1959	rVB	430565	676685	33.73%	3.571%
46	14.924	1961	1963	1968	rBV	4345	7818	0.39%	0.041%
47	15.053	1979	1985	1994	rBV2	280434	473532	23.60%	2.499%
48	15.359	2034	2037	2041	rBV	8017	10599	0.53%	0.056%
49	15.746	2099	2103	2106	rBV	8963	11639	0.58%	0.061%
50	15.846	2114	2120	2128	rBV	1077330	1624819	80.99%	8.575%
51	15.958	2133	2139	2147	rBV	327901	513942	25.62%	2.712%
52	16.681	2258	2262	2265	rBV	6272	8813	0.44%	0.047%
53	17.039	2319	2323	2324	rBV	5813	5793	0.29%	0.031%
54	17.609	2414	2420	2428	rBV	542331	835872	41.67%	4.411%
55	17.709	2431	2437	2445	rVB2	1216850	1816924	90.57%	9.588%
56	18.067	2497	2498	2501	rBV	5947	5439	0.27%	0.029%
57	18.443	2561	2562	2566	rBV	6807	5689	0.28%	0.030%
58	19.988	2819	2825	2831	rVB	1336010	1996706	99.53%	10.537%
59	21.916	3147	3153	3160	rVB	492322	852253	42.48%	4.498%
60	25.159	3696	3705	3716	rVB2	697906	2006158	100.00%	10.587%




Sum of corrected areas: 18949388

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059393.D
Acq On : 9 Oct 2023 11:35
Operator : MA/JU
Sample : PB155981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

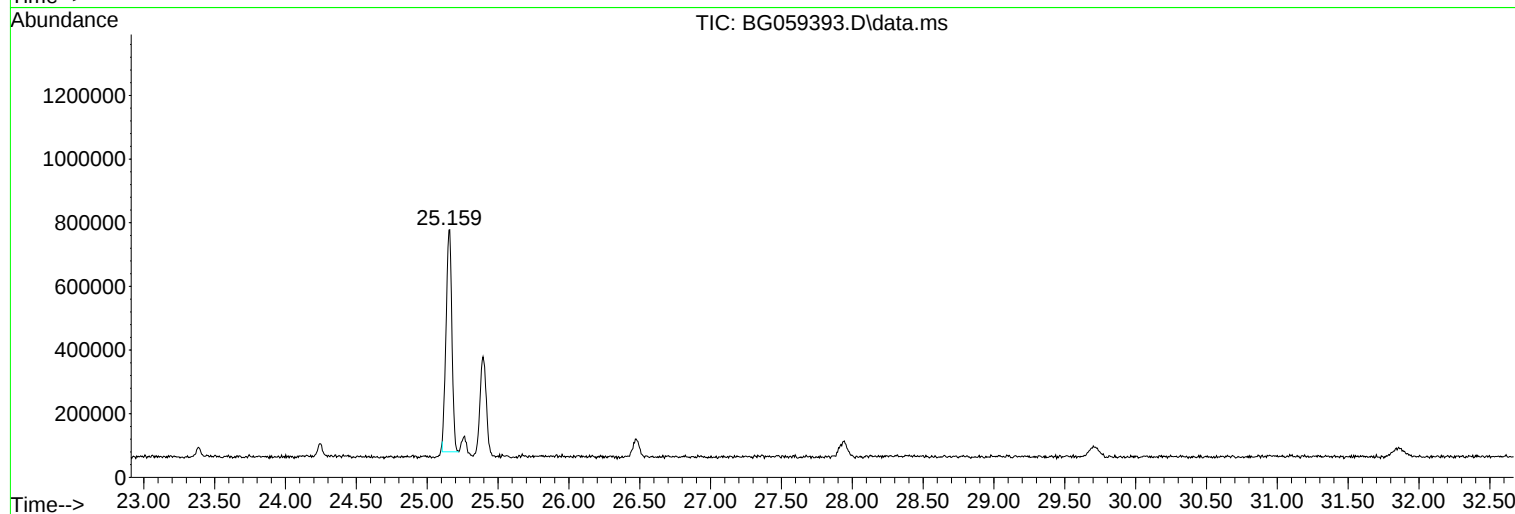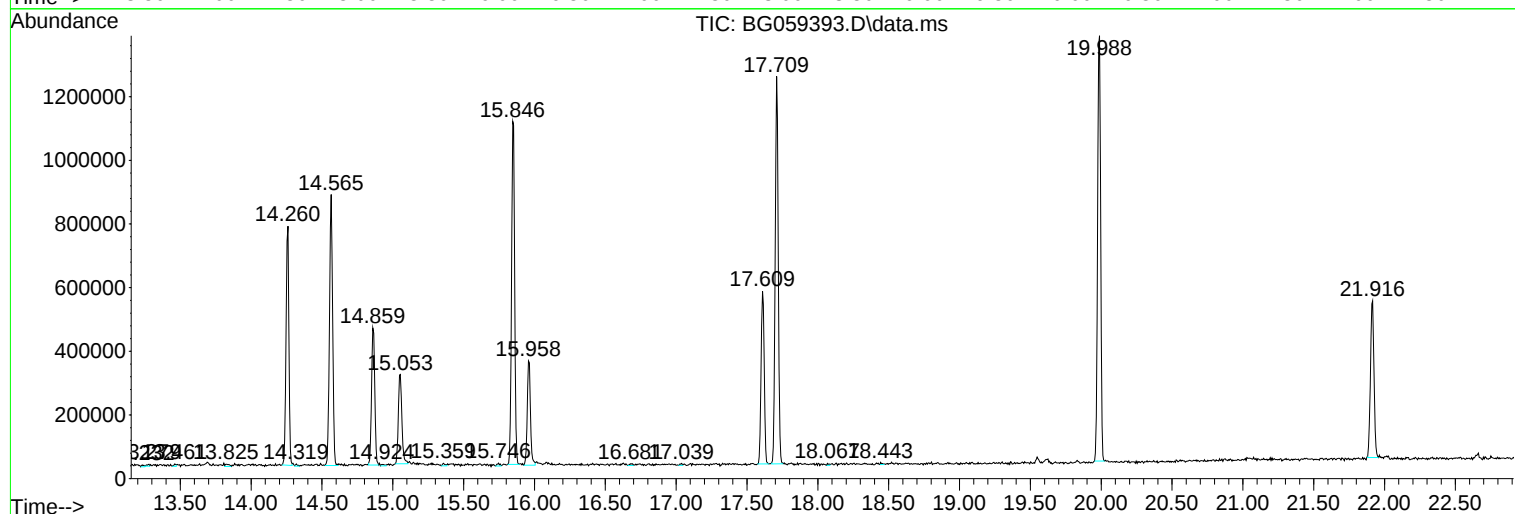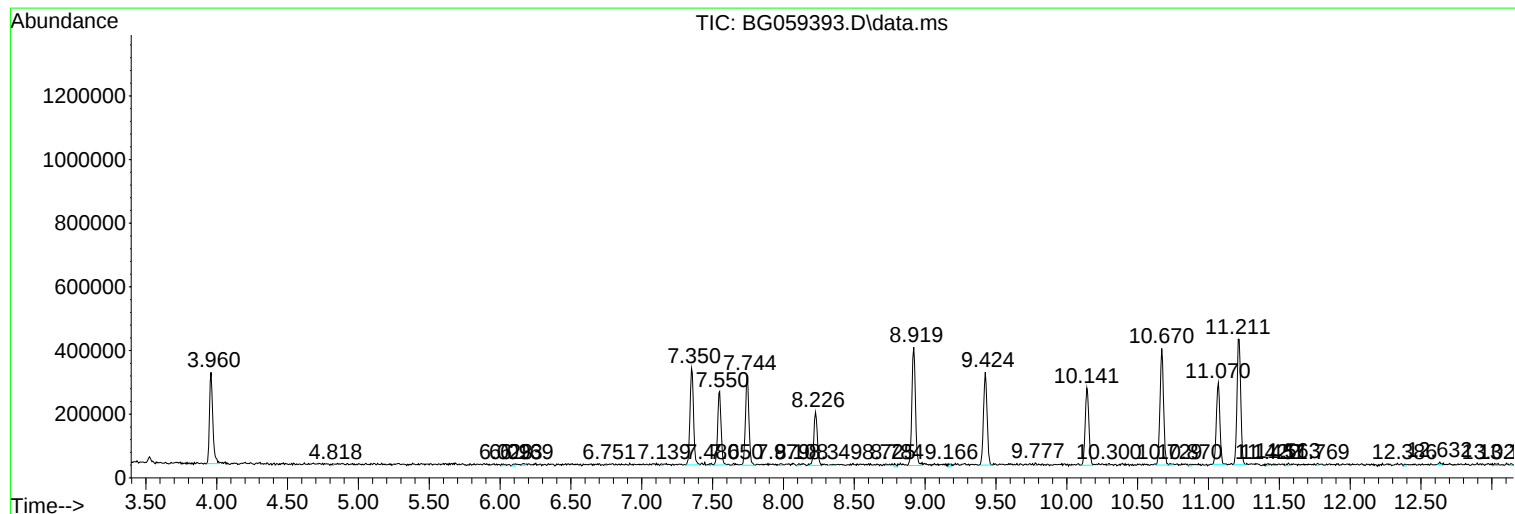

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059393.D
Acq On : 9 Oct 2023 11:35
Operator : MA/JU
Sample : PB155981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059393.D
Acq On : 9 Oct 2023 11:35
Operator : MA/JU
Sample : PB155981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc