

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059400.D
 Acq On : 9 Oct 2023 17:08
 Operator : MA/JU
 Sample : 04654-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBHD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.490	13	17	29	rVB4	54039	117938	5.34%	0.644%
2	3.961	93	97	105	rBV	93634	161678	7.32%	0.883%
3	4.060	113	114	117	rBV	6370	5321	0.24%	0.029%
4	4.301	151	155	160	rVB2	6324	12442	0.56%	0.068%
5	4.836	239	246	259	rBV	1330353	2208933	100.00%	12.063%
6	5.300	324	325	330	rBV	7517	9698	0.44%	0.053%
7	5.741	399	400	403	rVB	7941	5784	0.26%	0.032%
8	5.805	408	411	412	rBV2	5951	5849	0.26%	0.032%
9	6.722	565	567	570	rBV	5463	7772	0.35%	0.042%
10	6.787	574	578	583	rVB2	8266	12523	0.57%	0.068%
11	6.834	583	586	587	rBV2	5961	5331	0.24%	0.029%
12	7.057	622	624	627	rBV2	4782	6460	0.29%	0.035%
13	7.180	642	645	646	rBV	6531	7101	0.32%	0.039%
14	7.357	669	675	683	rVB3	53845	101282	4.59%	0.553%
15	7.545	702	707	716	rVB	217354	366764	16.60%	2.003%
16	7.686	729	731	734	rBV	4137	5620	0.25%	0.031%
17	7.744	734	741	747	rVB2	184957	333916	15.12%	1.823%
18	8.038	789	791	795	rVB	7496	6953	0.31%	0.038%
19	8.079	795	798	801	rBV	6108	6014	0.27%	0.033%
20	8.226	816	823	832	rBV	139466	232830	10.54%	1.271%
21	8.555	877	879	882	rVB	5957	6190	0.28%	0.034%
22	8.784	915	918	919	rBV	7281	6825	0.31%	0.037%
23	8.919	935	941	947	rBV	168688	277771	12.57%	1.517%
24	9.002	953	955	959	rBV	5637	6038	0.27%	0.033%
25	9.360	1014	1016	1019	rBV	5565	6327	0.29%	0.035%
26	9.425	1020	1027	1034	rVV	271782	464937	21.05%	2.539%
27	9.854	1099	1100	1106	rVB	6701	8426	0.38%	0.046%
28	9.989	1122	1123	1126	rBV	6394	5835	0.26%	0.032%
29	10.142	1143	1149	1158	rVB	206677	370069	16.75%	2.021%
30	10.670	1232	1239	1246	rBV	293639	516521	23.38%	2.821%
31	10.864	1270	1272	1277	rBV	4864	7348	0.33%	0.040%
32	11.070	1299	1307	1312	rBV	212678	376811	17.06%	2.058%
33	11.217	1325	1332	1342	rVB	302340	577072	26.12%	3.151%
34	11.281	1342	1343	1345	rBV	6676	5386	0.24%	0.029%
35	11.411	1363	1365	1368	rBV	5784	7516	0.34%	0.041%
36	11.651	1404	1406	1408	rBV	9055	8797	0.40%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059400.D
 Acq On : 9 Oct 2023 17:08
 Operator : MA/JU
 Sample : 04654-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBHD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	11.957	1456	1458	1461	rVB	6630	5858	0.27%	0.032%
38	12.633	1569	1573	1579	rBV3	11328	22821	1.03%	0.125%
39	12.944	1623	1626	1629	rBV	3897	5979	0.27%	0.033%
40	13.003	1634	1636	1641	rVB	6467	9409	0.43%	0.051%
41	13.050	1641	1644	1646	rBV	6113	6180	0.28%	0.034%
42	13.602	1735	1738	1741	rBV	4661	5923	0.27%	0.032%
43	13.679	1748	1751	1757	rBV3	7155	14049	0.64%	0.077%
44	13.796	1770	1771	1775	rVB	6885	6820	0.31%	0.037%
45	13.878	1782	1785	1786	rBV	7818	7565	0.34%	0.041%
46	13.908	1786	1790	1792	rBV	5056	7426	0.34%	0.041%
47	14.078	1814	1819	1821	rVB	6238	10587	0.48%	0.058%
48	14.254	1843	1849	1857	rBV	671630	959937	43.46%	5.242%
49	14.566	1895	1902	1909	rBV	761872	1191973	53.96%	6.509%
50	14.860	1946	1952	1959	rBV	364200	556289	25.18%	3.038%
51	15.053	1980	1985	1991	rBV2	45706	84813	3.84%	0.463%
52	15.664	2087	2089	2091	rBV	4509	5662	0.26%	0.031%
53	15.847	2114	2120	2128	rVB	977554	1515072	68.59%	8.274%
54	15.958	2133	2139	2146	rBV2	327865	517189	23.41%	2.824%
55	17.075	2327	2329	2333	rBV3	7948	7984	0.36%	0.044%
56	17.609	2413	2420	2427	rBV	458286	690902	31.28%	3.773%
57	17.662	2427	2429	2430	rBV	6789	5779	0.26%	0.032%
58	17.709	2431	2437	2444	rVV	1160259	1718992	77.82%	9.387%
59	17.985	2483	2484	2488	rBV	10571	14087	0.64%	0.077%
60	18.426	2555	2559	2563	rBV4	17884	34602	1.57%	0.189%
61	19.548	2746	2750	2755	rBV4	19240	32551	1.47%	0.178%
62	19.983	2818	2824	2831	rVB	1382141	1977146	89.51%	10.797%
63	21.910	3147	3152	3160	rVB2	401232	684448	30.99%	3.738%
64	25.147	3696	3703	3715	rVB3	670327	1939763	87.81%	10.593%




Sum of corrected areas: 18311884

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059400.D
Acq On : 9 Oct 2023 17:08
Operator : MA/JU
Sample : 04654-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

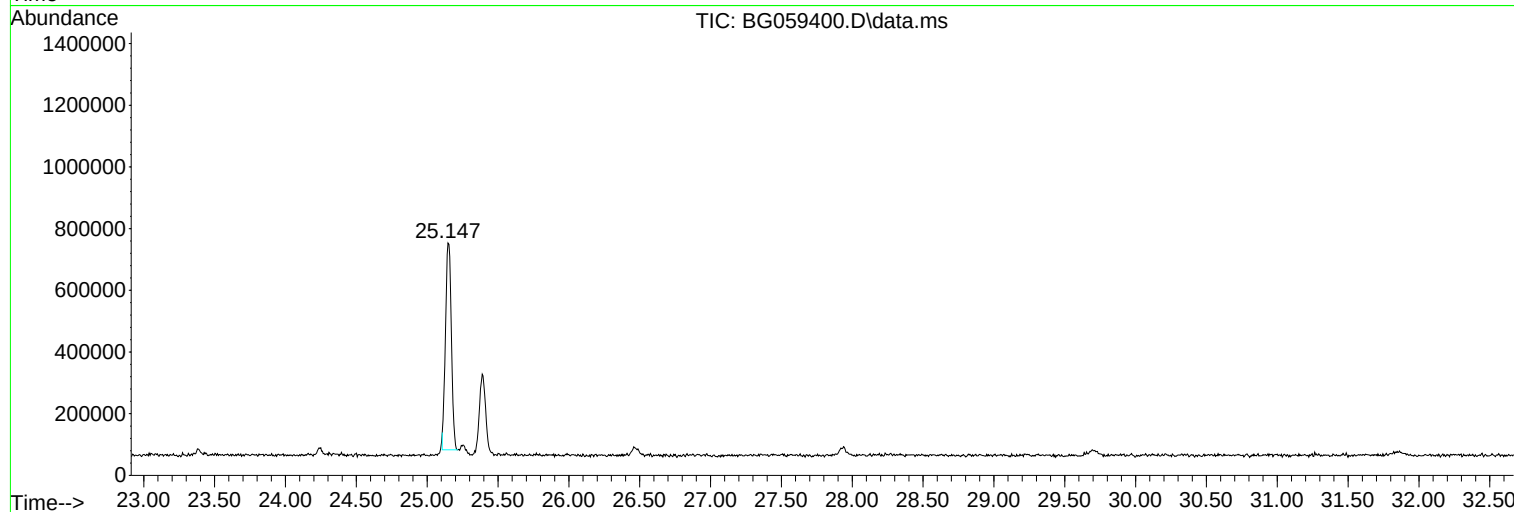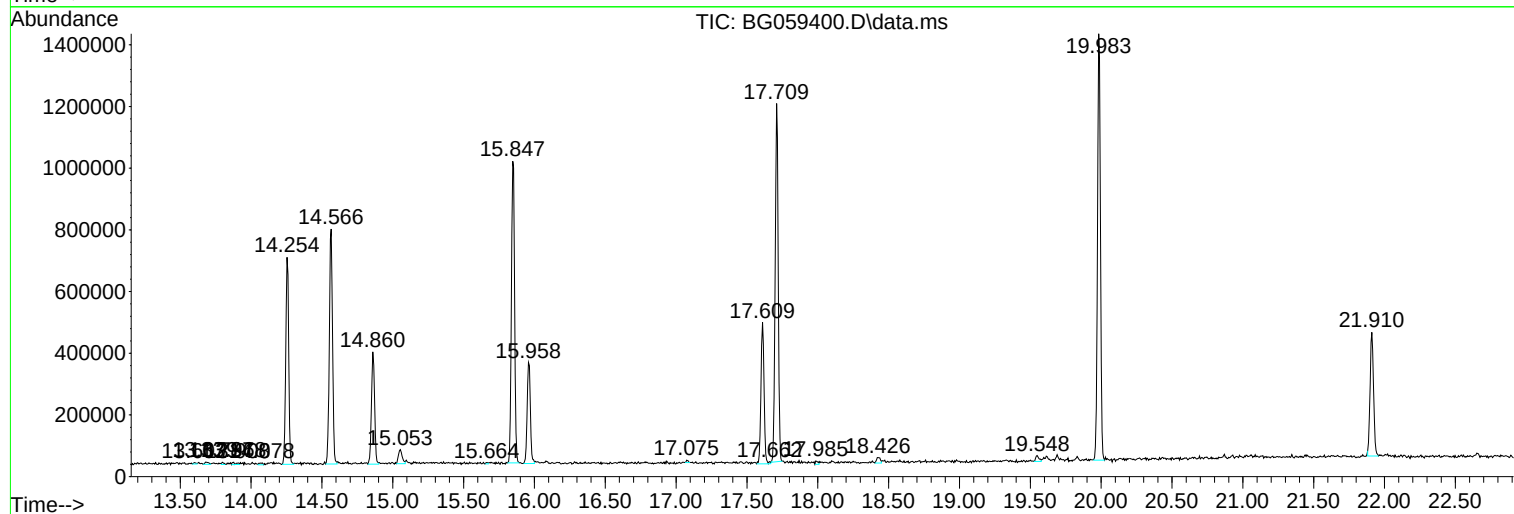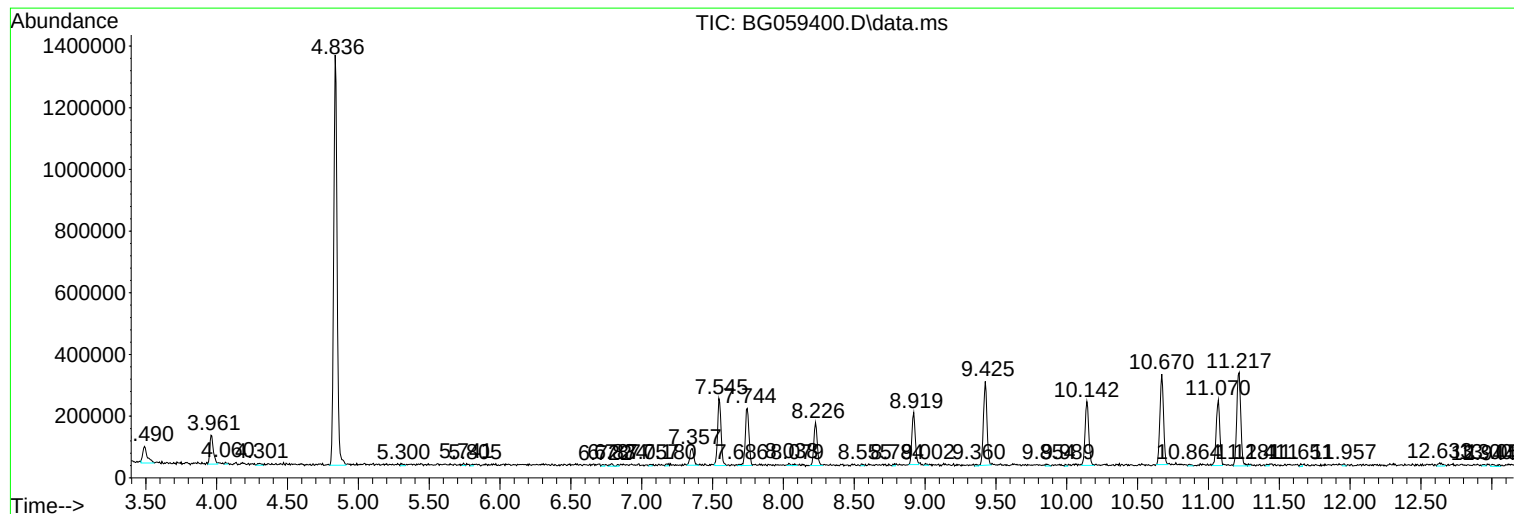

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059400.D
Acq On : 9 Oct 2023 17:08
Operator : MA/JU
Sample : 04654-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHD1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.836	189.75 ng/ul	2208930	1,4-Dichlorobenzene-d4	8.226

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

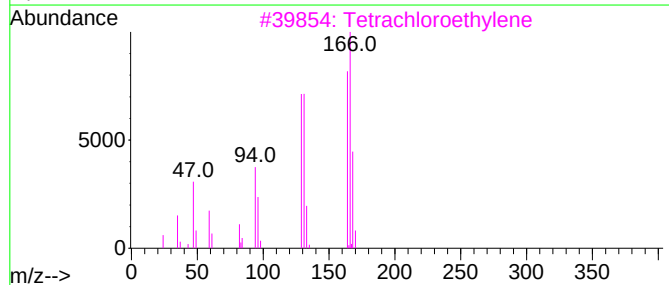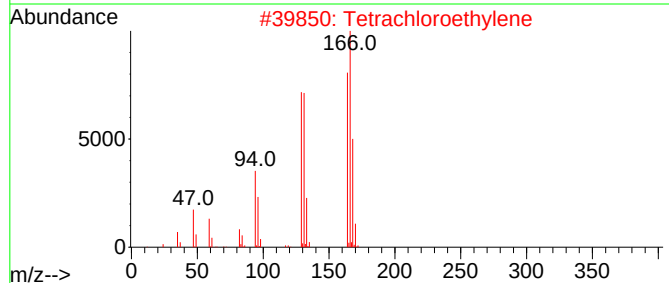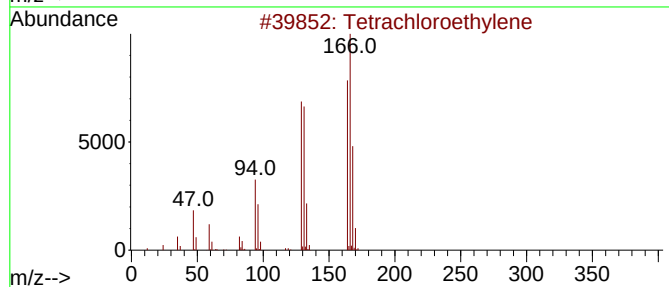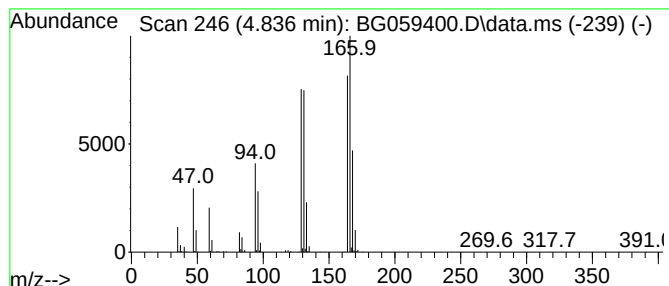

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059400.D
Acq On : 9 Oct 2023 17:08
Operator : MA/JU
Sample : 04654-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.836	189.8	ng/ul	2208930	1	8.226	232830	20.0