

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059402.D
 Acq On : 9 Oct 2023 18:34
 Operator : MA/JU
 Sample : PB156170BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.960	93	97	107	rBV	248298	407477	23.38%	2.720%
2	5.576	369	372	374	rBV	8217	7788	0.45%	0.052%
3	6.698	559	563	568	rBV	6615	11274	0.65%	0.075%
4	7.356	666	675	682	rBV	252782	451791	25.93%	3.016%
5	7.421	685	686	691	rVB	6402	5861	0.34%	0.039%
6	7.550	702	708	714	rVV	194385	328708	18.86%	2.195%
7	7.620	718	720	721	rBV	7202	4846	0.28%	0.032%
8	7.744	734	741	749	rBV	236519	405145	23.25%	2.705%
9	7.844	755	758	759	rBV	5166	4658	0.27%	0.031%
10	8.032	789	790	794	rVB	7100	6419	0.37%	0.043%
11	8.132	804	807	808	rBV	5093	5081	0.29%	0.034%
12	8.226	811	823	832	rBV	169392	306704	17.60%	2.048%
13	8.308	835	837	840	rVV	8648	8349	0.48%	0.056%
14	8.349	843	844	850	rVV	8124	8847	0.51%	0.059%
15	8.402	850	853	857	rVB	4366	6803	0.39%	0.045%
16	8.537	873	876	883	rBV	5226	9150	0.53%	0.061%
17	8.666	896	898	899	rBV	6413	5394	0.31%	0.036%
18	8.860	928	931	933	rVB	8981	9403	0.54%	0.063%
19	8.919	933	941	949	rBV	327949	561191	32.20%	3.747%
20	8.978	949	951	953	rVB	9439	5971	0.34%	0.040%
21	9.172	981	984	986	rBV	4892	5259	0.30%	0.035%
22	9.260	998	999	1002	rBV	5689	5477	0.31%	0.037%
23	9.289	1002	1004	1006	rBV	5220	5672	0.33%	0.038%
24	9.424	1020	1027	1036	rVB	246436	434535	24.94%	2.901%
25	10.141	1143	1149	1156	rVB3	199983	361116	20.72%	2.411%
26	10.264	1168	1170	1173	rVB	6255	5632	0.32%	0.038%
27	10.353	1183	1185	1190	rBV	5057	6506	0.37%	0.043%
28	10.411	1192	1195	1197	rBV	5529	5640	0.32%	0.038%
29	10.670	1232	1239	1246	rBV	307169	553224	31.75%	3.694%
30	11.022	1297	1299	1300	rBV	5974	5890	0.34%	0.039%
31	11.064	1300	1306	1314	rVB	254551	460388	26.42%	3.074%
32	11.216	1324	1332	1341	rBV	317435	599721	34.42%	4.004%
33	11.440	1367	1370	1372	rBV	4991	5929	0.34%	0.040%
34	11.481	1374	1377	1381	rVB	5061	7219	0.41%	0.048%
35	11.792	1427	1430	1432	rBV	4128	5701	0.33%	0.038%
36	12.309	1515	1518	1521	rBV	4544	5163	0.30%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059402.D
 Acq On : 9 Oct 2023 18:34
 Operator : MA/JU
 Sample : PB156170BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	12.415	1531	1536	1537	rBV	4528	6554	0.38%	0.044%
38	12.738	1588	1591	1592	rBV	5282	5534	0.32%	0.037%
39	12.967	1628	1630	1633	rVB	7739	6750	0.39%	0.045%
40	12.991	1633	1634	1636	rBV	6893	5041	0.29%	0.034%
41	13.273	1678	1682	1683	rVB	5190	5672	0.33%	0.038%
42	13.373	1697	1699	1702	rBV	6337	5568	0.32%	0.037%
43	13.678	1747	1751	1752	rBV	9616	8927	0.51%	0.060%
44	13.907	1788	1790	1793	rBV	6161	5877	0.34%	0.039%
45	14.254	1839	1849	1855	rBV	601476	879427	50.47%	5.871%
46	14.418	1876	1877	1879	rBV	6706	5145	0.30%	0.034%
47	14.565	1895	1902	1911	rBV2	697466	1110112	63.70%	7.412%
48	14.859	1946	1952	1959	rVB	431747	651676	37.40%	4.351%
49	15.000	1974	1976	1978	rBV	6423	4988	0.29%	0.033%
50	15.053	1979	1985	1999	rVB3	241510	428355	24.58%	2.860%
51	15.529	2063	2066	2069	rBV	7533	8181	0.47%	0.055%
52	15.682	2090	2092	2093	rBV	6708	4728	0.27%	0.032%
53	15.846	2113	2120	2126	rBV	915812	1365306	78.35%	9.115%
54	15.958	2133	2139	2147	rBV	285172	432390	24.81%	2.887%
55	16.698	2264	2265	2267	rBV	7855	5920	0.34%	0.040%
56	17.203	2350	2351	2353	rBV	5460	4747	0.27%	0.032%
57	17.321	2368	2371	2373	rBV	6007	7900	0.45%	0.053%
58	17.609	2414	2420	2426	rVB	547327	832889	47.80%	5.561%
59	17.709	2431	2437	2444	rBV2	1024604	1536436	88.17%	10.258%
60	17.908	2468	2471	2473	rBV	5746	7561	0.43%	0.050%
61	18.273	2530	2533	2535	rBV	6694	7033	0.40%	0.047%
62	19.548	2747	2750	2754	rVB5	13955	18161	1.04%	0.121%
63	19.982	2818	2824	2834	rBV	1207408	1742590	100.00%	11.634%
64	21.910	3146	3152	3159	rBV2	508950	840789	48.25%	5.613%




Sum of corrected areas: 14978189

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059402.D
Acq On : 9 Oct 2023 18:34
Operator : MA/JU
Sample : PB156170BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

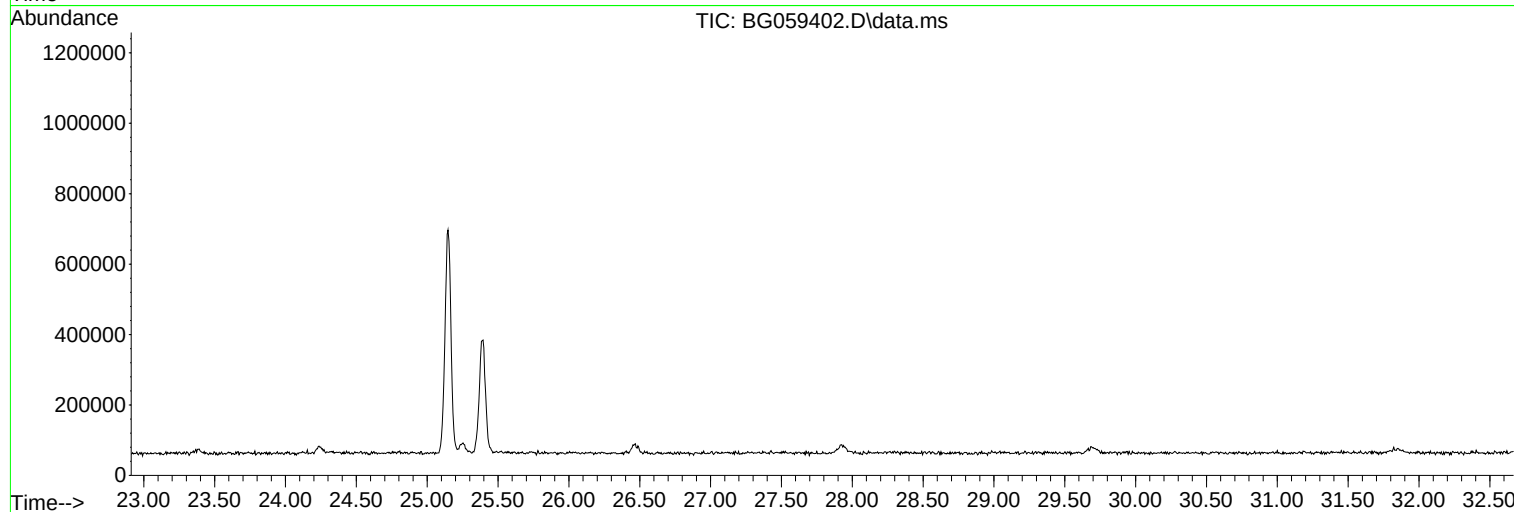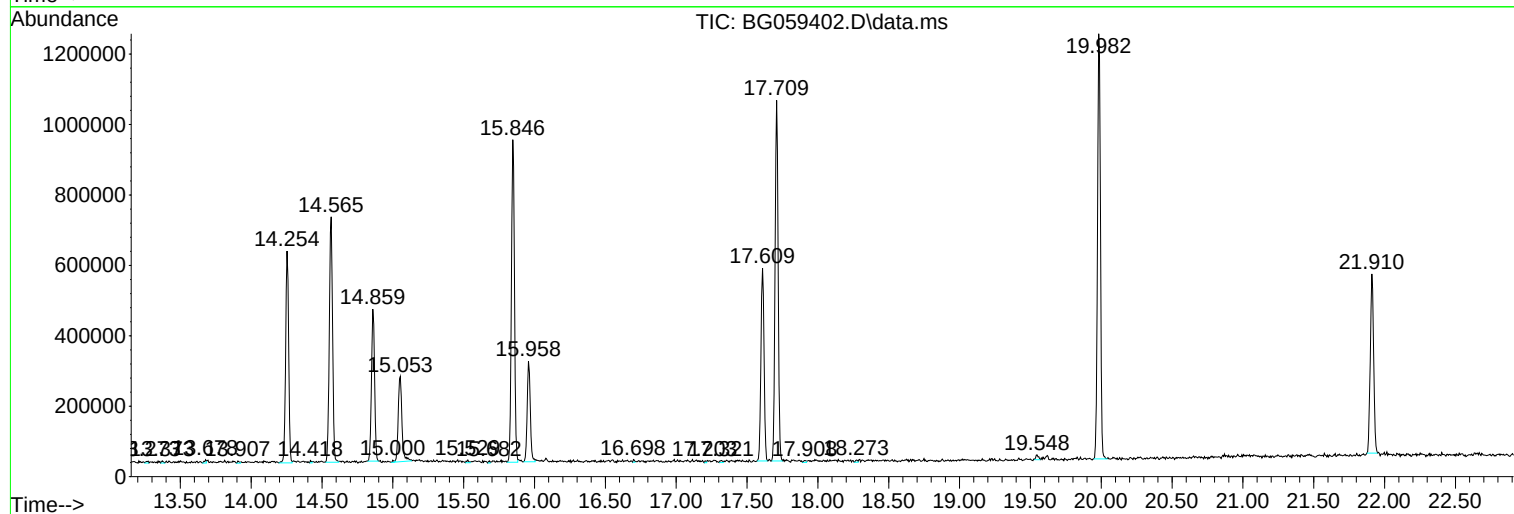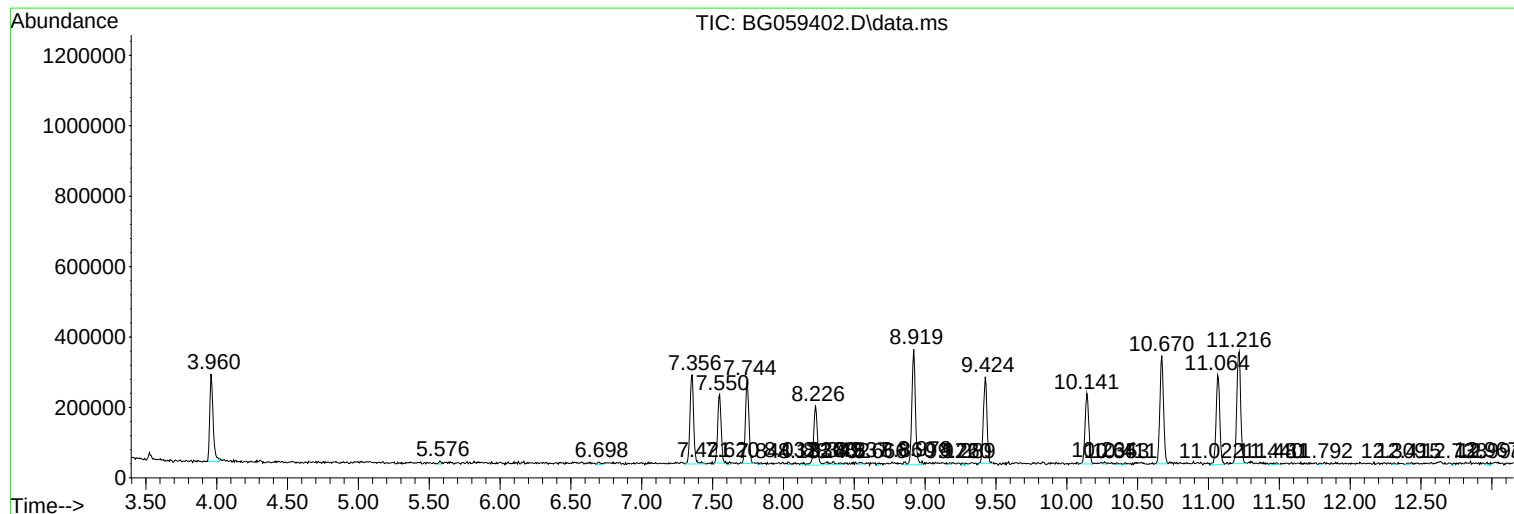

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059402.D
Acq On : 9 Oct 2023 18:34
Operator : MA/JU
Sample : PB156170BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059402.D
Acq On : 9 Oct 2023 18:34
Operator : MA/JU
Sample : PB156170BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK170

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc