

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059403.D
 Acq On : 9 Oct 2023 19:18
 Operator : MA/JU
 Sample : PB156200BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.958	92	97	108	rBV	246625	407928	24.57%	2.608%
2	4.904	256	258	261	rBV	7753	11508	0.69%	0.074%
3	4.980	268	271	273	rBV	9885	11871	0.72%	0.076%
4	5.039	279	281	283	rBV2	4699	4517	0.27%	0.029%
5	5.057	283	284	286	rVB	9202	6215	0.37%	0.040%
6	5.104	288	292	295	rBV3	4233	6069	0.37%	0.039%
7	5.421	344	346	349	rBV2	5503	4675	0.28%	0.030%
8	5.509	358	361	363	rBV	5155	5411	0.33%	0.035%
9	5.650	383	385	387	rVB	6321	4558	0.27%	0.029%
10	5.733	398	399	404	rBV	5863	5530	0.33%	0.035%
11	5.832	413	416	418	rBV3	4018	5253	0.32%	0.034%
12	5.874	421	423	425	rBV	5728	4528	0.27%	0.029%
13	5.985	441	442	445	rBV2	4906	5376	0.32%	0.034%
14	6.584	542	544	547	rVB	6161	5396	0.33%	0.034%
15	6.620	547	550	551	rBV	7310	5655	0.34%	0.036%
16	6.720	563	567	568	rBV2	4469	4815	0.29%	0.031%
17	6.878	593	594	598	rBV	6035	7644	0.46%	0.049%
18	6.931	601	603	605	rBV	6234	4770	0.29%	0.030%
19	6.990	611	613	615	rBV	5839	5236	0.32%	0.033%
20	7.190	646	647	650	rBV2	5194	5430	0.33%	0.035%
21	7.354	668	675	682	rVB	256256	427055	25.72%	2.730%
22	7.548	700	708	715	rVB	196088	337368	20.32%	2.157%
23	7.742	734	741	749	rBV2	234570	404945	24.39%	2.589%
24	7.818	752	754	757	rBV	6412	7377	0.44%	0.047%
25	7.989	781	783	785	rVB	6913	5495	0.33%	0.035%
26	8.106	801	803	806	rVB	6052	5166	0.31%	0.033%
27	8.136	806	808	811	rVB	5833	6368	0.38%	0.041%
28	8.159	811	812	815	rBV	7936	5181	0.31%	0.033%
29	8.224	818	823	829	rVB2	125429	201703	12.15%	1.290%
30	8.312	834	838	840	rBV	5774	6570	0.40%	0.042%
31	8.459	861	863	866	rVB	7355	6803	0.41%	0.043%
32	8.488	866	868	869	rBV	6165	4489	0.27%	0.029%
33	8.529	874	875	878	rVB	5749	5120	0.31%	0.033%
34	8.559	878	880	882	rBV	6515	5861	0.35%	0.037%
35	8.664	896	898	900	rVB	5538	4758	0.29%	0.030%
36	8.694	900	903	904	rBV	5696	5723	0.34%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059403.D
 Acq On : 9 Oct 2023 19:18
 Operator : MA/JU
 Sample : PB156200BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	8.741	907	911	913	rVV	3919	5323	0.32%	0.034%
38	8.917	933	941	949	rBV	311825	538411	32.43%	3.442%
39	9.299	1005	1006	1009	rBV	5668	6414	0.39%	0.041%
40	9.422	1020	1027	1037	rBV	244200	424474	25.57%	2.714%

41	9.563	1049	1051	1054	rBV	5562	6071	0.37%	0.039%
42	9.646	1063	1065	1066	rBV	6589	5729	0.35%	0.037%
43	9.722	1077	1078	1080	rBV	6446	4482	0.27%	0.029%
44	10.004	1125	1126	1129	rBV	5946	5100	0.31%	0.033%
45	10.098	1140	1142	1144	rBV	7308	6774	0.41%	0.043%

46	10.139	1144	1149	1158	rVB	196541	359172	21.63%	2.296%
47	10.268	1169	1171	1174	rVB	5135	5322	0.32%	0.034%
48	10.368	1187	1188	1191	rBV	4861	5626	0.34%	0.036%
49	10.439	1197	1200	1201	rBV	5718	5021	0.30%	0.032%
50	10.597	1224	1227	1229	rVB	6172	6237	0.38%	0.040%

51	10.668	1233	1239	1248	rVB	311049	548022	33.01%	3.504%
52	11.067	1300	1307	1316	rVB	193689	342955	20.66%	2.193%
53	11.214	1325	1332	1339	rBV	329999	576182	34.71%	3.684%
54	11.496	1379	1380	1384	rBV	5187	5671	0.34%	0.036%
55	11.749	1420	1423	1424	rBV	5869	5427	0.33%	0.035%

56	11.925	1452	1453	1455	rBV	6523	4821	0.29%	0.031%
57	12.149	1487	1491	1493	rBV2	5070	8018	0.48%	0.051%
58	12.295	1514	1516	1518	rBV	5485	4543	0.27%	0.029%
59	12.378	1527	1530	1532	rBV	6958	5558	0.33%	0.036%
60	12.460	1541	1544	1546	rVB	5841	6245	0.38%	0.040%

61	12.630	1570	1573	1578	rBV3	8007	13540	0.82%	0.087%
62	12.812	1600	1604	1605	rBV	4017	4756	0.29%	0.030%
63	12.942	1625	1626	1631	rVB	5093	4644	0.28%	0.030%
64	13.065	1646	1647	1651	rBV	5211	5619	0.34%	0.036%
65	13.100	1651	1653	1655	rBV	5369	4483	0.27%	0.029%

66	13.235	1674	1676	1677	rBV	6540	5882	0.35%	0.038%
67	13.318	1687	1690	1693	rBV	4567	4741	0.29%	0.030%
68	13.453	1712	1713	1716	rBV	7230	6332	0.38%	0.040%
69	13.582	1732	1735	1738	rBV	7440	7809	0.47%	0.050%
70	13.688	1747	1753	1757	rBV3	9574	20225	1.22%	0.129%

71	13.817	1773	1775	1777	rBV	5276	5299	0.32%	0.034%
72	13.870	1783	1784	1787	rBV	6968	6181	0.37%	0.040%
73	14.017	1808	1809	1812	rBV	9720	6574	0.40%	0.042%
74	14.258	1842	1850	1856	rBV	582688	865029	52.10%	5.530%
75	14.358	1866	1867	1869	rBV	6176	4654	0.28%	0.030%

76	14.563	1896	1902	1909	rBV	699684	1072389	64.59%	6.856%
----	--------	------	------	------	-----	--------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059403.D
 Acq On : 9 Oct 2023 19:18
 Operator : MA/JU
 Sample : PB156200BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

77	14.863	1947	1953	1960	rVB	320085	503490	30.33%	3.219%
78	14.981	1972	1973	1976	rBV	9135	7677	0.46%	0.049%
79	15.004	1976	1977	1979	rBV	4964	4601	0.28%	0.029%
80	15.051	1979	1985	1993	rVV2	229082	391098	23.56%	2.500%
81	15.850	2114	2121	2128	rBV	902977	1347145	81.14%	8.613%
82	15.962	2134	2140	2148	rBV	260203	418088	25.18%	2.673%
83	16.255	2189	2190	2193	rBV	8592	7741	0.47%	0.049%
84	16.291	2193	2196	2200	rVB	7456	10040	0.60%	0.064%
85	16.455	2220	2224	2227	rBV	7679	13390	0.81%	0.086%
86	17.607	2414	2420	2426	rBV	400333	618898	37.28%	3.957%
87	17.707	2431	2437	2448	rVB	991893	1494413	90.01%	9.554%
88	19.040	2663	2664	2667	rBV	7438	7393	0.45%	0.047%
89	19.986	2819	2825	2831	rVB	1160147	1651928	99.50%	10.561%
90	21.908	3147	3152	3159	rVB2	363818	613169	36.93%	3.920%
91	25.145	3696	3703	3714	rVB2	582762	1660189	100.00%	10.614%




Sum of corrected areas: 15641382

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059403.D
Acq On : 9 Oct 2023 19:18
Operator : MA/JU
Sample : PB156200BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

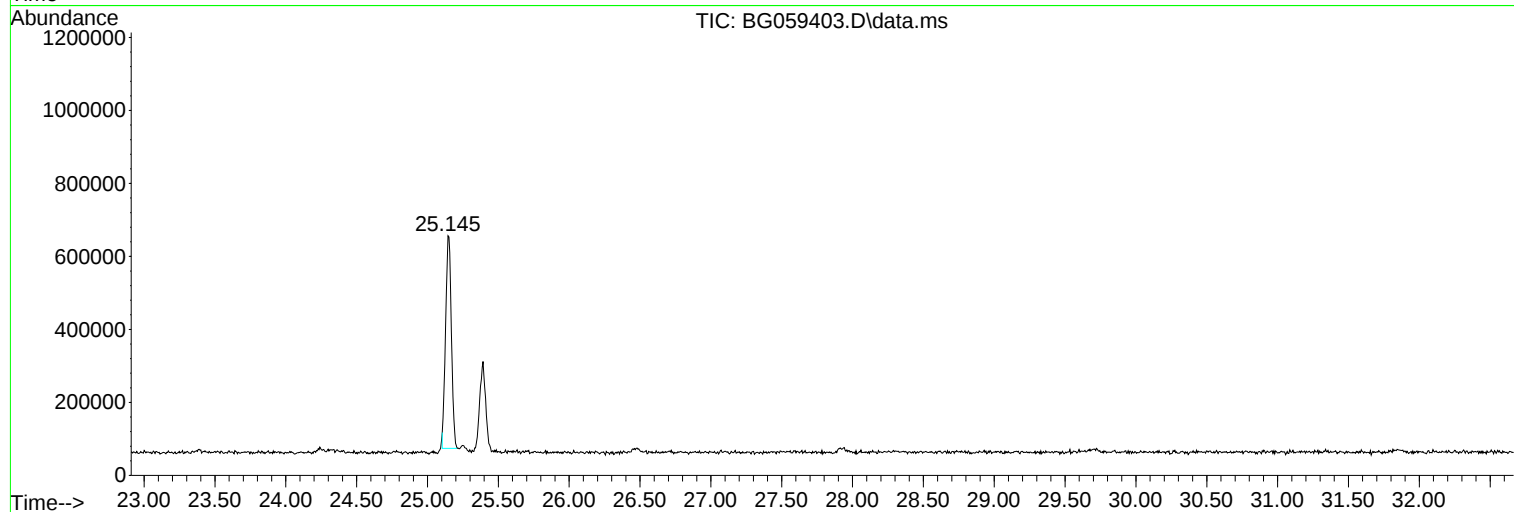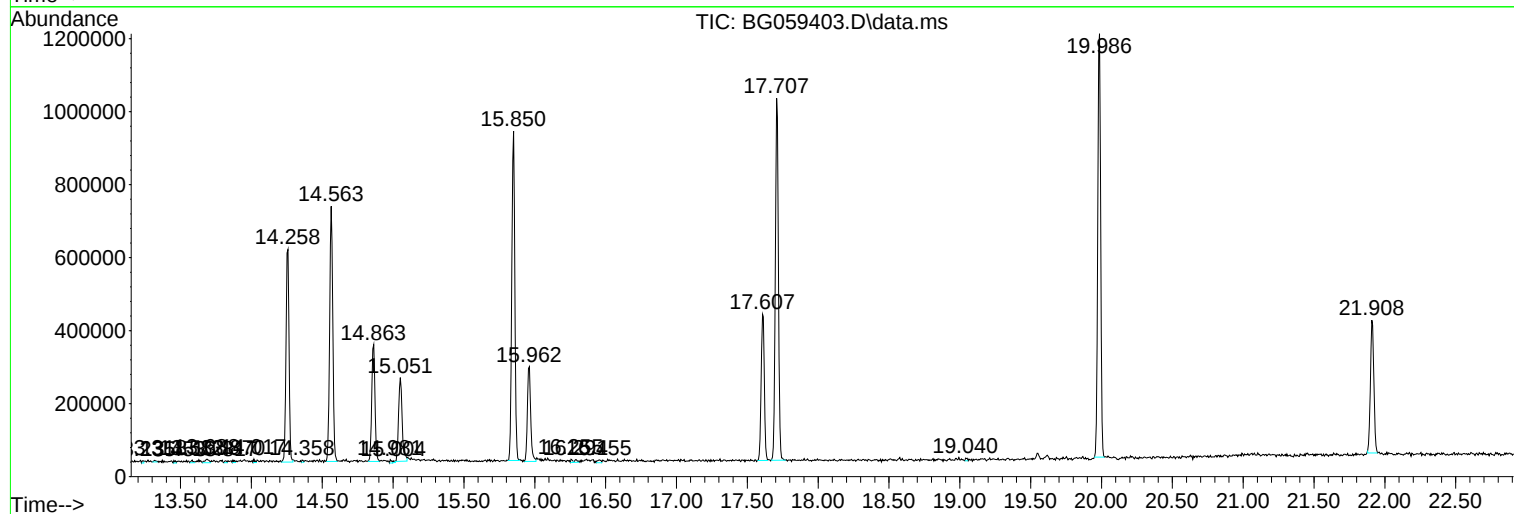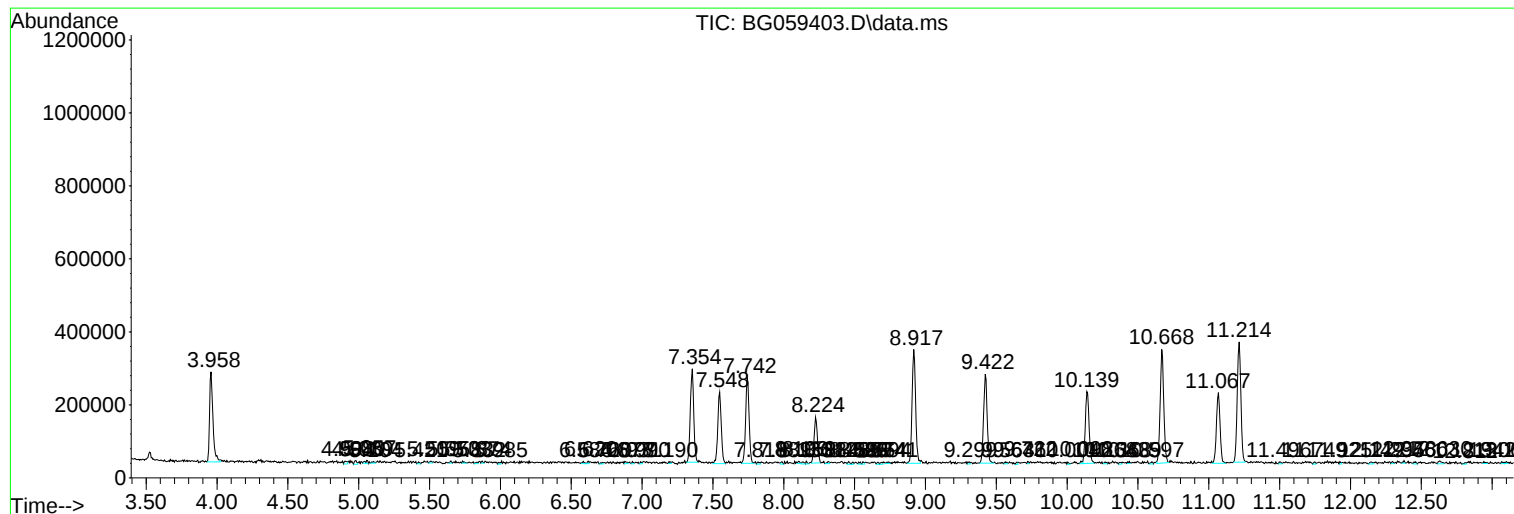

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059403.D
Acq On : 9 Oct 2023 19:18
Operator : MA/JU
Sample : PB156200BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059403.D
Acq On : 9 Oct 2023 19:18
Operator : MA/JU
Sample : PB156200BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------