

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059417.D
 Acq On : 10 Oct 2023 6:09
 Operator : MA/JU
 Sample : PB156059BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.523	19	23	28	rBV4	19407	37312	1.97%	0.218%
2	3.793	67	69	74	rBV3	4239	5216	0.28%	0.030%
3	3.957	93	97	106	rBV	242293	412645	21.79%	2.406%
4	4.627	210	211	215	rBV2	5561	6401	0.34%	0.037%
5	4.674	217	219	221	rBV2	4434	5498	0.29%	0.032%
6	4.927	259	262	264	rVB	5212	5528	0.29%	0.032%
7	6.296	490	495	498	rBV2	3866	6079	0.32%	0.035%
8	6.384	505	510	513	rBV	6438	10552	0.56%	0.062%
9	6.484	526	527	532	rBV	5426	6080	0.32%	0.035%
10	6.701	562	564	566	rVB	5429	5045	0.27%	0.029%
11	6.731	566	569	571	rBV	5002	5746	0.30%	0.034%
12	7.177	641	645	648	rVB2	4690	6306	0.33%	0.037%
13	7.353	667	675	683	rBV	279973	487233	25.73%	2.841%
14	7.547	702	708	716	rVB	214256	342970	18.11%	2.000%
15	7.741	735	741	748	rBV	253084	427241	22.56%	2.492%
16	8.005	784	786	791	rBV	4018	6313	0.33%	0.037%
17	8.223	818	823	832	rVB2	142685	241339	12.74%	1.407%
18	8.417	855	856	860	rVB	7197	6912	0.36%	0.040%
19	8.916	935	941	953	rVB	319892	575668	30.40%	3.357%
20	9.421	1021	1027	1034	rVB	260633	456082	24.08%	2.660%
21	9.604	1056	1058	1060	rVB	6955	5272	0.28%	0.031%
22	9.621	1060	1061	1063	rBV	8166	6022	0.32%	0.035%
23	10.144	1142	1150	1158	rBV2	217128	397901	21.01%	2.320%
24	10.667	1232	1239	1248	rBV	333608	599967	31.68%	3.499%
25	10.937	1283	1285	1290	rVB2	6967	10742	0.57%	0.063%
26	11.067	1300	1307	1314	rVB	219132	391771	20.69%	2.285%
27	11.213	1323	1332	1341	rBV	346623	636808	33.62%	3.714%
28	11.496	1379	1380	1383	rBV	5482	5582	0.29%	0.033%
29	11.590	1394	1396	1398	rBV	6890	6316	0.33%	0.037%
30	11.660	1405	1408	1409	rBV	6101	5635	0.30%	0.033%
31	11.678	1409	1411	1416	rVB	5787	7396	0.39%	0.043%
32	11.907	1447	1450	1452	rBV	7439	10931	0.58%	0.064%
33	11.960	1455	1459	1461	rVV	6430	6846	0.36%	0.040%
34	12.101	1481	1483	1486	rVB	7254	5458	0.29%	0.032%
35	12.253	1505	1509	1513	rBV	4681	8908	0.47%	0.052%
36	12.629	1569	1573	1574	rBV2	7753	8746	0.46%	0.051%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059417.D
 Acq On : 10 Oct 2023 6:09
 Operator : MA/JU
 Sample : PB156059BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	12.682	1581	1582	1585	rBV	5451	5336	0.28%	0.031%
38	12.888	1615	1617	1620	rBV	6624	7025	0.37%	0.041%
39	13.100	1650	1653	1654	rVB	6708	5002	0.26%	0.029%
40	13.393	1701	1703	1706	rVB	8192	8410	0.44%	0.049%
41	13.429	1706	1709	1712	rBV	7303	9350	0.49%	0.055%
42	13.452	1712	1713	1715	rBV	6661	5535	0.29%	0.032%
43	13.781	1766	1769	1770	rBV	6439	6249	0.33%	0.036%
44	13.963	1799	1800	1803	rBV	6722	5665	0.30%	0.033%
45	14.257	1844	1850	1856	rVB	631506	929142	49.06%	5.418%
46	14.563	1895	1902	1910	rBV2	781728	1171375	61.85%	6.831%
47	14.862	1946	1953	1960	rBV	353431	584396	30.86%	3.408%
48	15.050	1980	1985	1993	rBV3	264599	430488	22.73%	2.510%
49	15.215	2010	2013	2014	rBV	7016	7286	0.38%	0.042%
50	15.403	2043	2045	2047	rBV	7404	6776	0.36%	0.040%
51	15.849	2114	2121	2130	rVB	1004758	1455961	76.88%	8.491%
52	15.961	2134	2140	2153	rVB	269151	423478	22.36%	2.470%
53	16.402	2211	2215	2216	rBV	6043	6975	0.37%	0.041%
54	16.713	2265	2268	2270	rBV	6687	6981	0.37%	0.041%
55	17.606	2414	2420	2428	rVB	485492	726652	38.37%	4.238%
56	17.712	2431	2438	2446	rVB2	1034864	1641600	86.68%	9.573%
57	18.205	2519	2522	2523	rBV	6554	5946	0.31%	0.035%
58	19.821	2795	2797	2801	rVB2	13628	13066	0.69%	0.076%
59	19.986	2819	2825	2834	rVB	1301116	1871997	98.85%	10.917%
60	21.907	3147	3152	3160	rVB	446496	748695	39.53%	4.366%
61	25.150	3694	3704	3717	rVB2	664223	1893861	100.00%	11.044%




Sum of corrected areas: 17147714

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059417.D
Acq On : 10 Oct 2023 6:09
Operator : MA/JU
Sample : PB156059BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

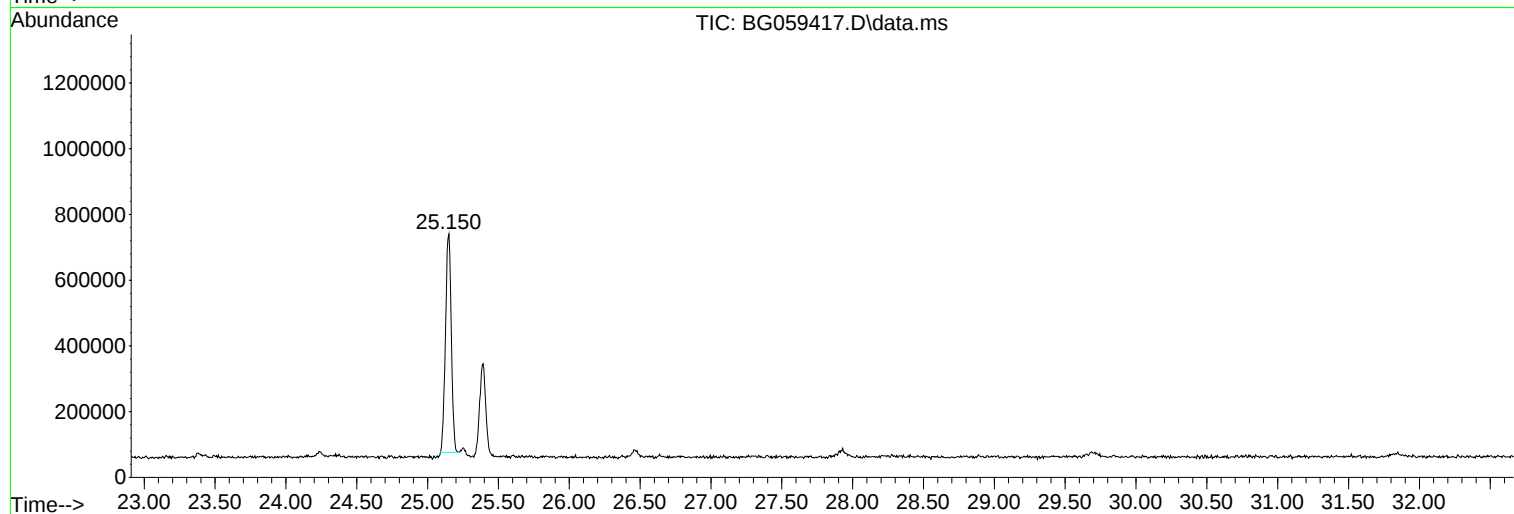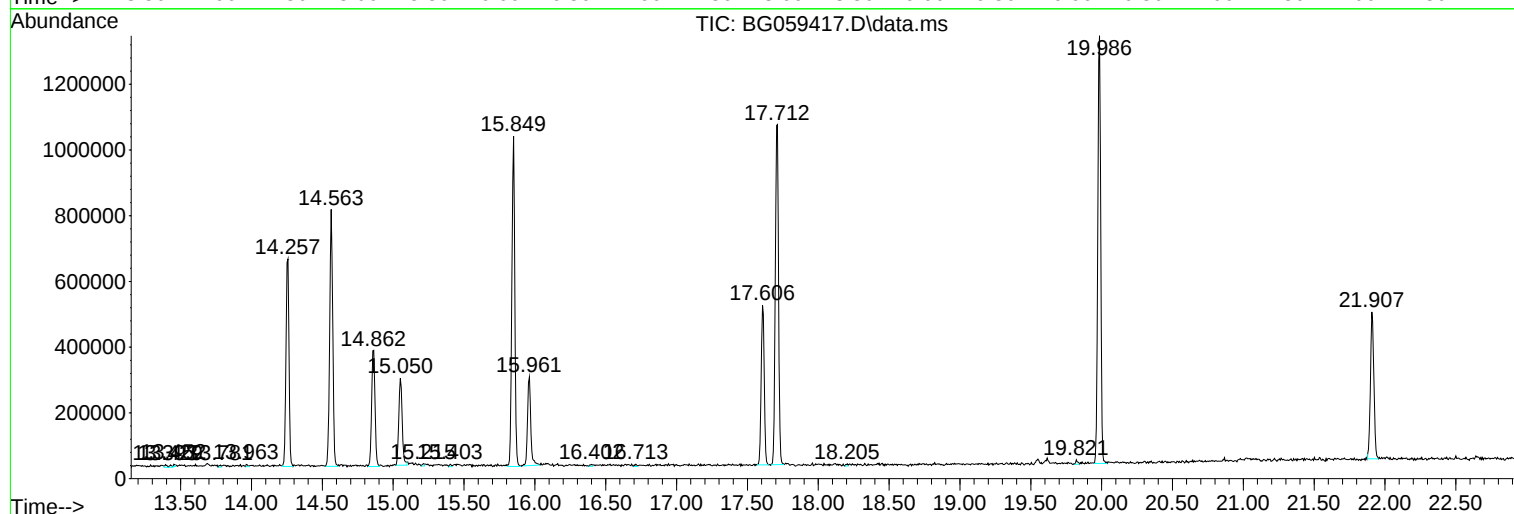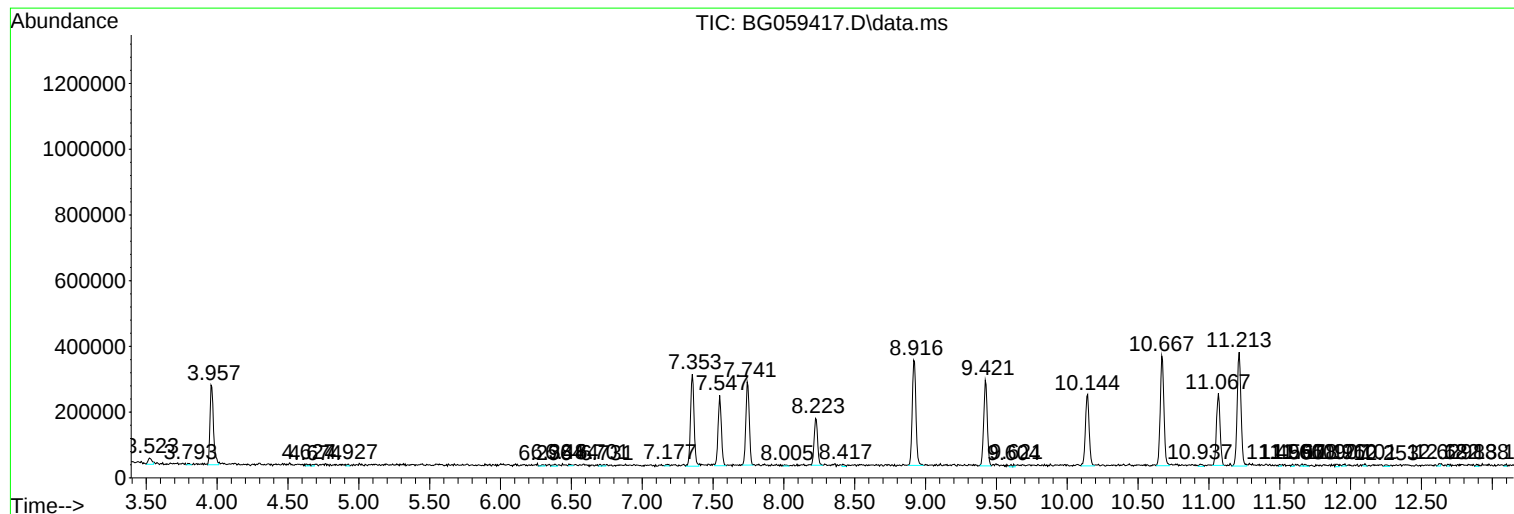

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059417.D
Acq On : 10 Oct 2023 6:09
Operator : MA/JU
Sample : PB156059BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059417.D
Acq On : 10 Oct 2023 6:09
Operator : MA/JU
Sample : PB156059BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------