

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059421.D
 Acq On : 10 Oct 2023 8:51
 Operator : MA/JU
 Sample : 04654-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.646	42	44	47	rBV2	6712	7002	0.34%	0.042%
2	3.793	68	69	72	rVB	8141	5610	0.27%	0.034%
3	3.963	93	98	109	rBV2	94246	170138	8.23%	1.031%
4	4.521	191	193	198	rBV2	5318	6562	0.32%	0.040%
5	4.662	215	217	220	rBV	6050	6436	0.31%	0.039%
6	5.320	327	329	333	rBV	6887	8003	0.39%	0.049%
7	5.602	375	377	380	rBV2	7013	8055	0.39%	0.049%
8	5.820	412	414	417	rBV	4832	6355	0.31%	0.039%
9	5.867	420	422	425	rBV	5660	8229	0.40%	0.050%
10	6.066	453	456	459	rBV2	5686	7603	0.37%	0.046%
11	6.295	492	495	499	rBV	6588	9230	0.45%	0.056%
12	6.360	503	506	510	rVB2	5476	6375	0.31%	0.039%
13	6.625	549	551	553	rBV	6043	6821	0.33%	0.041%
14	6.948	603	606	607	rBV	7284	7505	0.36%	0.045%
15	7.353	669	675	681	rBV2	67947	109752	5.31%	0.665%
16	7.547	702	708	715	rBV	238850	387112	18.73%	2.346%
17	7.741	734	741	749	rBV	215807	373779	18.08%	2.265%
18	7.888	765	766	770	rBV	5194	5601	0.27%	0.034%
19	8.052	792	794	796	rBV	6936	5938	0.29%	0.036%
20	8.223	817	823	831	rVB2	132859	240970	11.66%	1.460%
21	8.481	865	867	868	rBV	6272	5417	0.26%	0.033%
22	8.881	933	935	936	rBV	7533	6084	0.29%	0.037%
23	8.916	936	941	952	rVB	186084	342688	16.58%	2.077%
24	9.345	1011	1014	1015	rBV	6322	6170	0.30%	0.037%
25	9.421	1020	1027	1035	rVB	289725	507539	24.56%	3.076%
26	9.609	1056	1059	1062	rBV	5426	8496	0.41%	0.051%
27	10.144	1142	1150	1159	rBV2	229139	431055	20.86%	2.612%
28	10.232	1164	1165	1167	rBV	6705	5455	0.26%	0.033%
29	10.261	1167	1170	1172	rVB	6123	6367	0.31%	0.039%
30	10.667	1233	1239	1246	rBV	341274	594282	28.75%	3.602%
31	11.066	1300	1307	1313	rBV	212430	380249	18.40%	2.305%
32	11.149	1319	1321	1325	rBV	6292	8049	0.39%	0.049%
33	11.213	1325	1332	1340	rVV2	262645	496820	24.04%	3.011%
34	11.719	1416	1418	1421	rBV	4967	6711	0.32%	0.041%
35	12.024	1468	1470	1473	rVB	7861	7059	0.34%	0.043%
36	12.183	1495	1497	1502	rVB	5303	5900	0.29%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
 Data File : BG059421.D
 Acq On : 10 Oct 2023 8:51
 Operator : MA/JU
 Sample : 04654-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBK63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	12.288	1514	1515	1518	rBV	4717	5896	0.29%	0.036%
38	12.406	1533	1535	1539	rBV	5585	7191	0.35%	0.044%
39	12.753	1591	1594	1595	rBV	5896	5617	0.27%	0.034%
40	12.888	1616	1617	1620	rVB	7624	6273	0.30%	0.038%
41	12.917	1620	1622	1626	rBV	7090	8635	0.42%	0.052%
42	13.076	1647	1649	1652	rVB	7001	5856	0.28%	0.035%
43	13.105	1652	1654	1656	rBV	5708	6208	0.30%	0.038%
44	13.693	1750	1754	1758	rVB2	11742	19448	0.94%	0.118%
45	14.075	1817	1819	1824	rVB2	8123	11245	0.54%	0.068%
46	14.257	1843	1850	1855	rBV	657402	977239	47.28%	5.923%
47	14.351	1865	1866	1870	rBV	6992	7945	0.38%	0.048%
48	14.562	1895	1902	1911	rBV2	826008	1287498	62.29%	7.803%
49	14.815	1940	1945	1947	rBV	5896	9019	0.44%	0.055%
50	14.856	1947	1952	1960	rVV	357969	554426	26.83%	3.360%
51	15.050	1981	1985	1989	rBV4	34751	59076	2.86%	0.358%
52	15.849	2114	2121	2127	rBV	1065995	1598915	77.36%	9.690%
53	15.961	2135	2140	2149	rBV	247200	407928	19.74%	2.472%
54	16.531	2234	2237	2238	rBV	7652	7560	0.37%	0.046%
55	16.583	2242	2246	2247	rBV	6836	8356	0.40%	0.051%
56	17.271	2360	2363	2367	rBV	9543	14091	0.68%	0.085%
57	17.606	2415	2420	2428	rVB	443126	685386	33.16%	4.154%
58	17.706	2431	2437	2443	rBV2	1194753	1804231	87.30%	10.935%
59	19.985	2819	2825	2831	rVB	1402618	2028656	98.15%	12.295%
60	21.907	3147	3152	3161	rVB2	404566	701293	33.93%	4.250%
61	25.144	3694	3703	3715	rVB2	723136	2066813	100.00%	12.526%




Sum of corrected areas: 16500218

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059421.D
Acq On : 10 Oct 2023 8:51
Operator : MA/JU
Sample : 04654-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBK63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

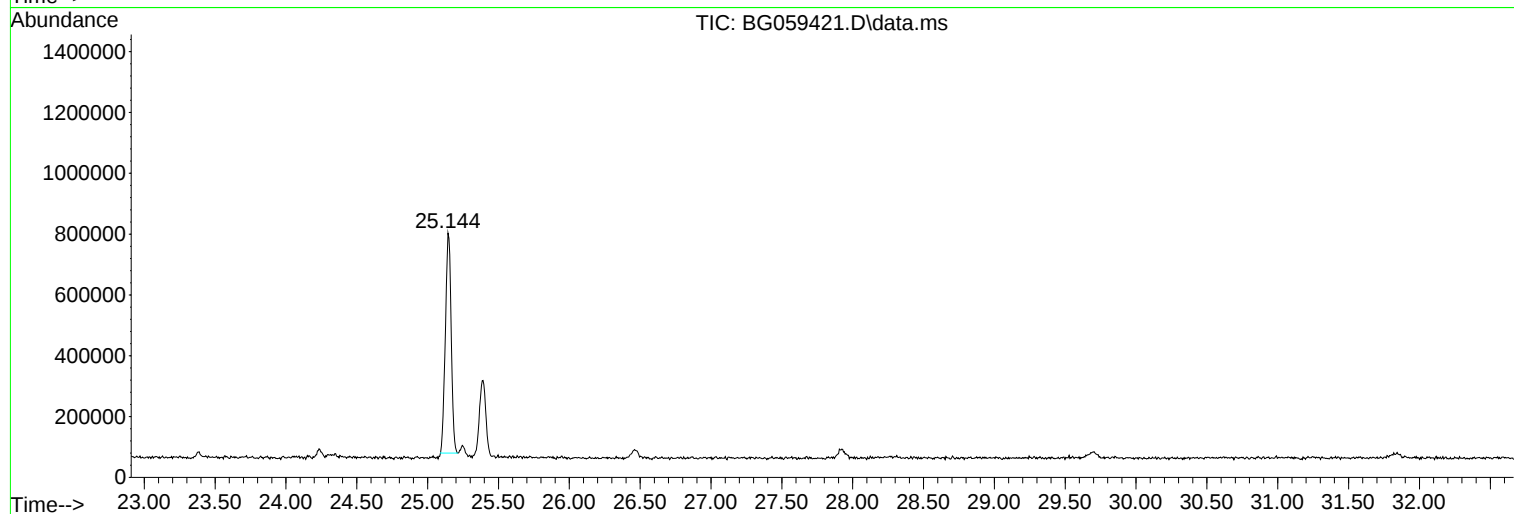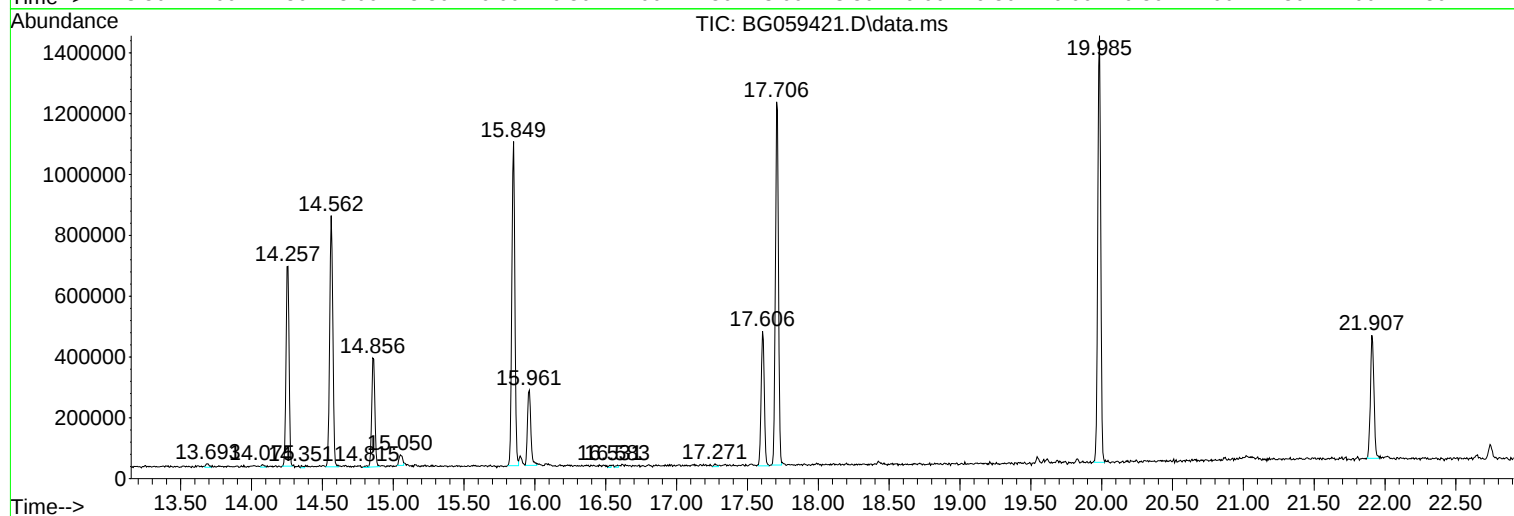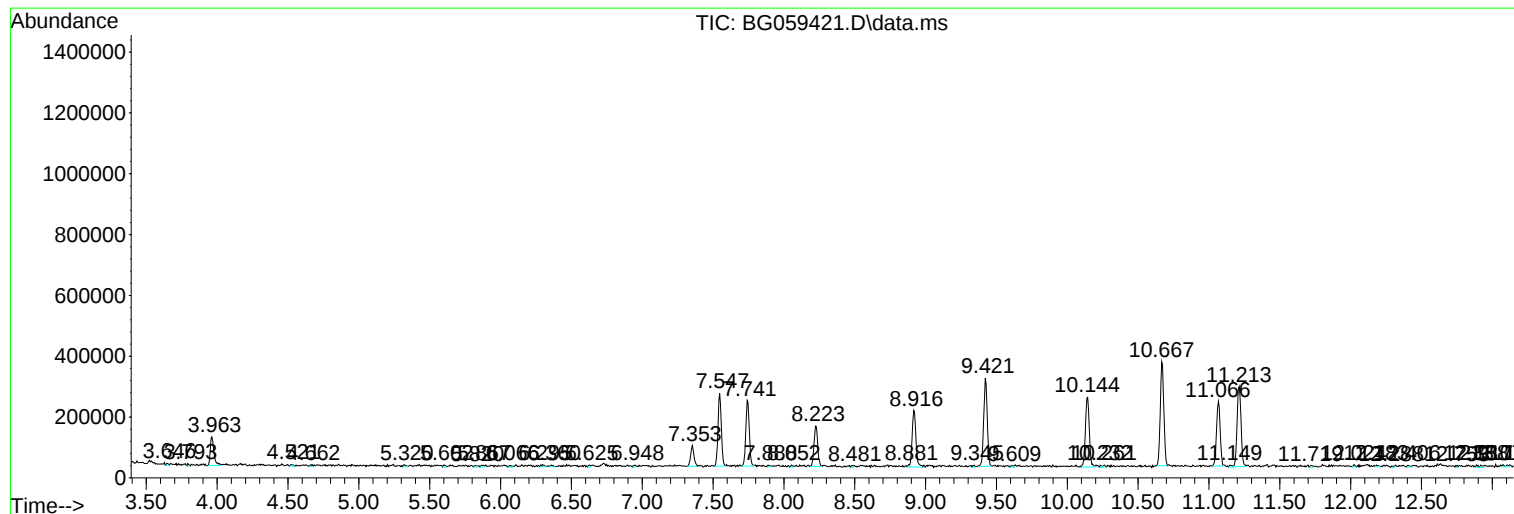

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059421.D
Acq On : 10 Oct 2023 8:51
Operator : MA/JU
Sample : 04654-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBK63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100923\
Data File : BG059421.D
Acq On : 10 Oct 2023 8:51
Operator : MA/JU
Sample : 04654-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBK63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc