

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101023\
 Data File : BG059425.D
 Acq On : 10 Oct 2023 15:00
 Operator : MA/JU
 Sample : PB156059BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK059

Quant Time: Oct 10 22:51:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 07 22:45:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.223	152	41789	20.000	ng/ul	0.00
20) Naphthalene-d8	11.061	136	197419	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.857	164	136627	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.607	188	301002	20.000	ng/ul	0.00
79) Chrysene-d12	21.902	240	273285	20.000	ng/ul	-0.01
88) Perylene-d12	25.380	264	325860	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.517	96	8683	7.408	ng/uL	0.00
4) Pyridine-d5	3.958	84	125997	37.349	ng/ul	0.00
7) Phenol-d5	7.348	99	169768	36.792	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.542	67	97072	37.220	ng/ul	0.00
11) 2-Chlorophenol-d4	7.742	132	123686	38.327	ng/ul	0.00
15) 4-Methylphenol-d8	8.917	113	128597	35.770	ng/ul	0.00
21) Nitrobenzene-d5	9.422	128	63409	37.731	ng/ul	0.00
24) 2-Nitrophenol-d4	10.139	143	67631	37.181	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.668	165	133844	40.767	ng/ul	0.00
31) 4-Chloroaniline-d4	11.208	131	197481	37.868	ng/ul	0.00
46) Dimethylphthalate-d6	14.252	166	456350	40.770	ng/ul	0.00
49) Acenaphthylene-d8	14.563	160	525810	39.474	ng/ul	0.00
54) 4-Nitrophenol-d4	15.051	143	67728	32.289	ng/ul	0.00
60) Fluorene-d10	15.844	176	415226	38.863	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.956	200	55930	28.143	ng/ul	0.00
73) Anthracene-d10	17.706	188	636207	43.087	ng/ul	0.00
81) Pyrene-d10	19.980	212	739900	44.692	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.139	264	763726	44.539	ng/ul	-0.01


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.917	70	2765	1.016 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101023\
Data File : BG059425.D
Acq On : 10 Oct 2023 15:00
Operator : MA/JU
Sample : PB156059BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK059


Quant Time: Oct 10 22:51:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 07 22:45:22 2023
Response via : Initial Calibration

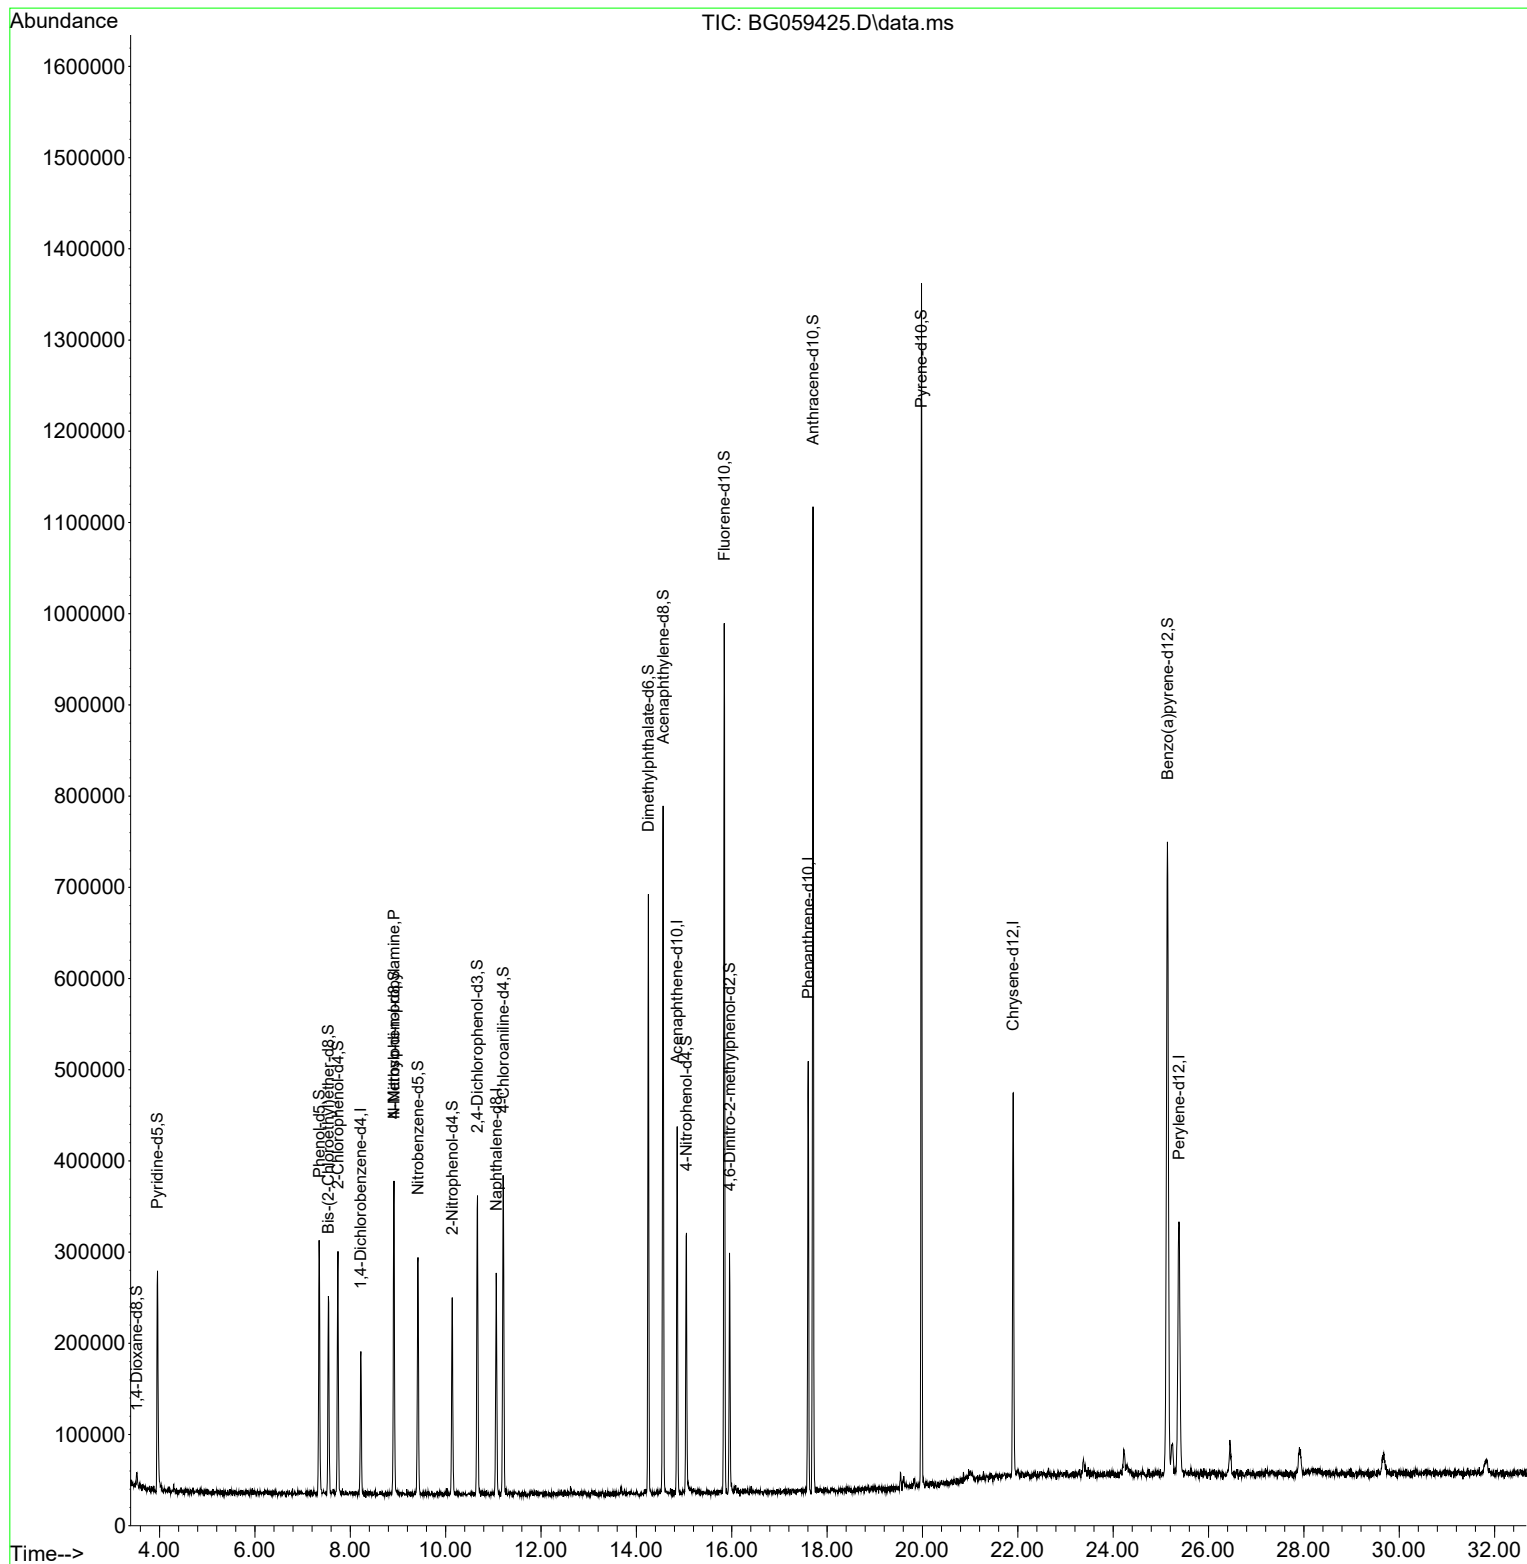

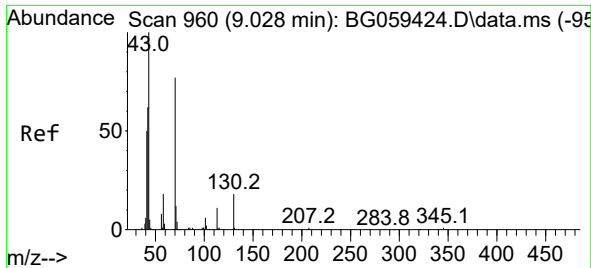

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.016 ng/ul
 RT: 8.917 min Scan# 941
 Delta R.T. -0.120 min
 Lab File: BG059425.D
 Acq: 10 Oct 2023 15:00

Instrument :
 BNA_G
 ClientSampleId :
 SBLK059

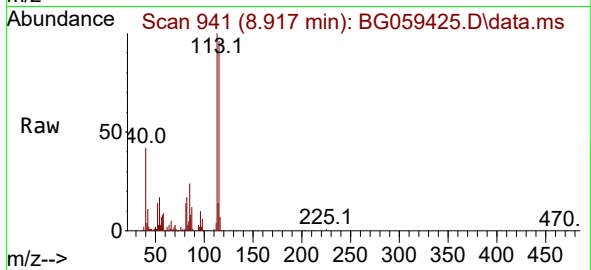

Tgt Ion:	70	Resp:	2765
Ion	Ratio	Lower	Upper
70	100		
42	430.4	58.2	87.4#
101	0.0	6.4	9.6#
130	0.0	15.4	23.0#

