

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101023\
 Data File : BG059425.D
 Acq On : 10 Oct 2023 15:00
 Operator : MA/JU
 Sample : PB156059BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.958	92	97	107	rBV	242595	428338	22.31%	2.481%
2	4.299	153	155	156	rBV	7941	6268	0.33%	0.036%
3	4.945	263	265	267	rBV	6491	6463	0.34%	0.037%
4	4.974	267	270	273	rVV2	5623	6542	0.34%	0.038%
5	5.515	361	362	365	rVB	6480	5384	0.28%	0.031%
6	5.709	393	395	398	rBV	6550	6946	0.36%	0.040%
7	5.903	425	428	431	rBV	6300	8959	0.47%	0.052%
8	6.055	451	454	457	rBV	6454	8875	0.46%	0.051%
9	7.178	642	645	648	rBV	7190	9613	0.50%	0.056%
10	7.236	651	655	656	rBV	6765	6514	0.34%	0.038%
11	7.348	667	674	682	rBV	279594	480516	25.03%	2.784%
12	7.542	701	707	714	rBV	218827	374104	19.49%	2.167%
13	7.742	734	741	747	rBV	263669	424839	22.13%	2.461%
14	7.836	754	757	760	rBV	7612	6734	0.35%	0.039%
15	8.165	811	813	816	rBV	5425	6583	0.34%	0.038%
16	8.223	816	823	830	rVV	157582	273712	14.26%	1.586%
17	8.341	841	843	845	rBV	6444	7093	0.37%	0.041%
18	8.917	933	941	949	rBV	343860	585689	30.51%	3.393%
19	9.046	960	963	967	rBV	4657	7623	0.40%	0.044%
20	9.216	990	992	995	rBV	5954	7249	0.38%	0.042%
21	9.422	1020	1027	1035	rVB	260634	461209	24.02%	2.672%
22	10.027	1129	1130	1134	rVB	8233	5698	0.30%	0.033%
23	10.139	1143	1149	1157	rVB	216687	372258	19.39%	2.156%
24	10.368	1184	1188	1190	rBV	4583	5987	0.31%	0.035%
25	10.580	1221	1224	1226	rVB	4569	5327	0.28%	0.031%
26	10.668	1232	1239	1246	rBV	327851	586210	30.54%	3.396%
27	10.768	1254	1256	1259	rVB	5654	5583	0.29%	0.032%
28	11.061	1299	1306	1314	rBV	243470	416105	21.67%	2.410%
29	11.208	1322	1331	1338	rBV	352271	651734	33.95%	3.775%
30	11.361	1354	1357	1359	rBV2	5064	6088	0.32%	0.035%
31	11.408	1363	1365	1368	rBV	5536	6668	0.35%	0.039%
32	12.225	1503	1504	1506	rBV	6056	5060	0.26%	0.029%
33	12.483	1545	1548	1550	rBV	5772	7685	0.40%	0.045%
34	13.065	1643	1647	1649	rBV	6168	7503	0.39%	0.043%
35	13.682	1749	1752	1756	rVB3	6867	10190	0.53%	0.059%
36	14.005	1805	1807	1812	rVB	5339	6828	0.36%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101023\
 Data File : BG059425.D
 Acq On : 10 Oct 2023 15:00
 Operator : MA/JU
 Sample : PB156059BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK059

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
 Title : SVOA CALIBRATION

37	14.252	1843	1849	1856	rBV	656002	927613	48.32%	5.373%
38	14.563	1894	1902	1909	rVB	752864	1170798	60.99%	6.782%
39	14.716	1926	1928	1931	rVB	7555	6510	0.34%	0.038%
40	14.792	1937	1941	1942	rBV	6574	5316	0.28%	0.031%
41	14.857	1946	1952	1961	rVB	404605	607758	31.66%	3.521%
42	14.974	1969	1972	1974	rBV	5945	6126	0.32%	0.035%
43	15.051	1977	1985	1990	rBV	285625	462132	24.07%	2.677%
44	15.685	2092	2093	2098	rVB	5658	6505	0.34%	0.038%
45	15.844	2114	2120	2127	rBV	954535	1457660	75.93%	8.444%
46	15.956	2133	2139	2145	rBV	262843	387767	20.20%	2.246%
47	16.085	2155	2161	2165	rVB4	8351	13631	0.71%	0.079%
48	16.185	2176	2178	2183	rBV	8266	12515	0.65%	0.072%
49	16.243	2187	2188	2193	rBV	6122	6391	0.33%	0.037%
50	16.337	2202	2204	2209	rVB	7248	7914	0.41%	0.046%
51	16.379	2209	2211	2214	rBV	6041	6572	0.34%	0.038%
52	16.696	2260	2265	2268	rBV	4977	10539	0.55%	0.061%
53	17.266	2360	2362	2363	rBV	5954	5340	0.28%	0.031%
54	17.607	2413	2420	2426	rBV	471492	723090	37.67%	4.189%
55	17.706	2430	2437	2445	rBV2	1082842	1623550	84.57%	9.405%
56	18.788	2619	2621	2625	rBV	7009	10327	0.54%	0.060%
57	18.899	2638	2640	2643	rBV2	5312	6660	0.35%	0.039%
58	19.540	2745	2749	2754	rVB4	19828	32474	1.69%	0.188%
59	19.980	2818	2824	2830	rBV2	1316219	1863190	97.05%	10.793%
60	21.907	3146	3152	3163	rVB2	418607	754608	39.31%	4.371%
61	25.139	3693	3702	3713	rVB2	682711	1919771	100.00%	11.121%




Sum of corrected areas: 17262934

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101023\
Data File : BG059425.D
Acq On : 10 Oct 2023 15:00
Operator : MA/JU
Sample : PB156059BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

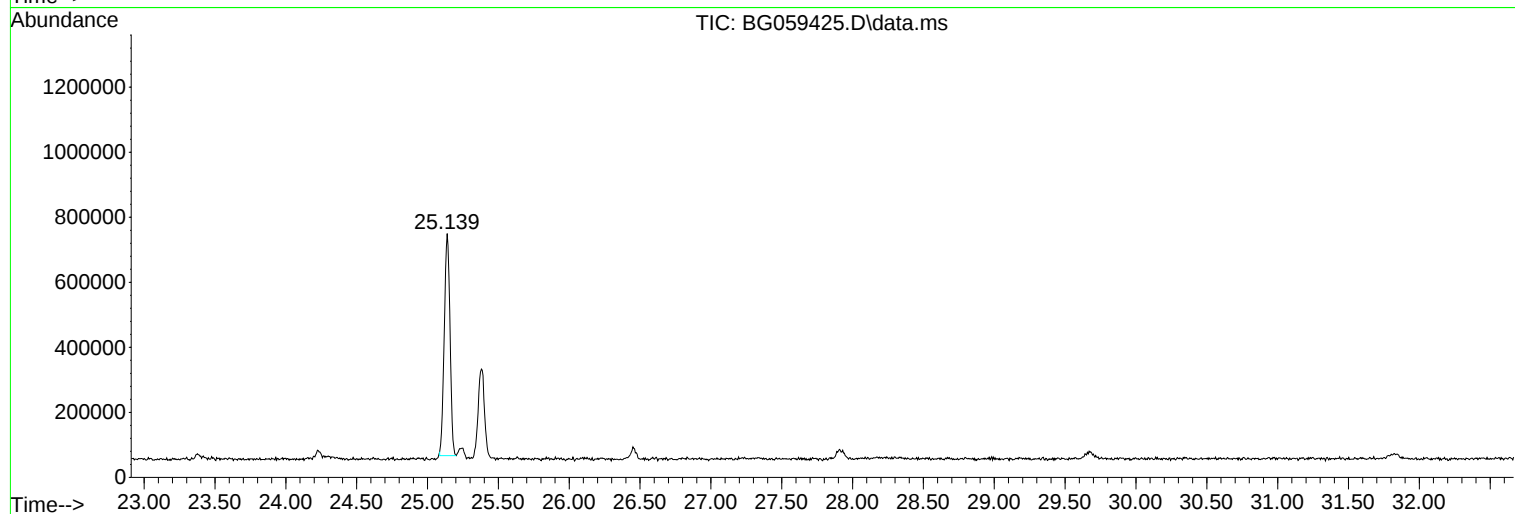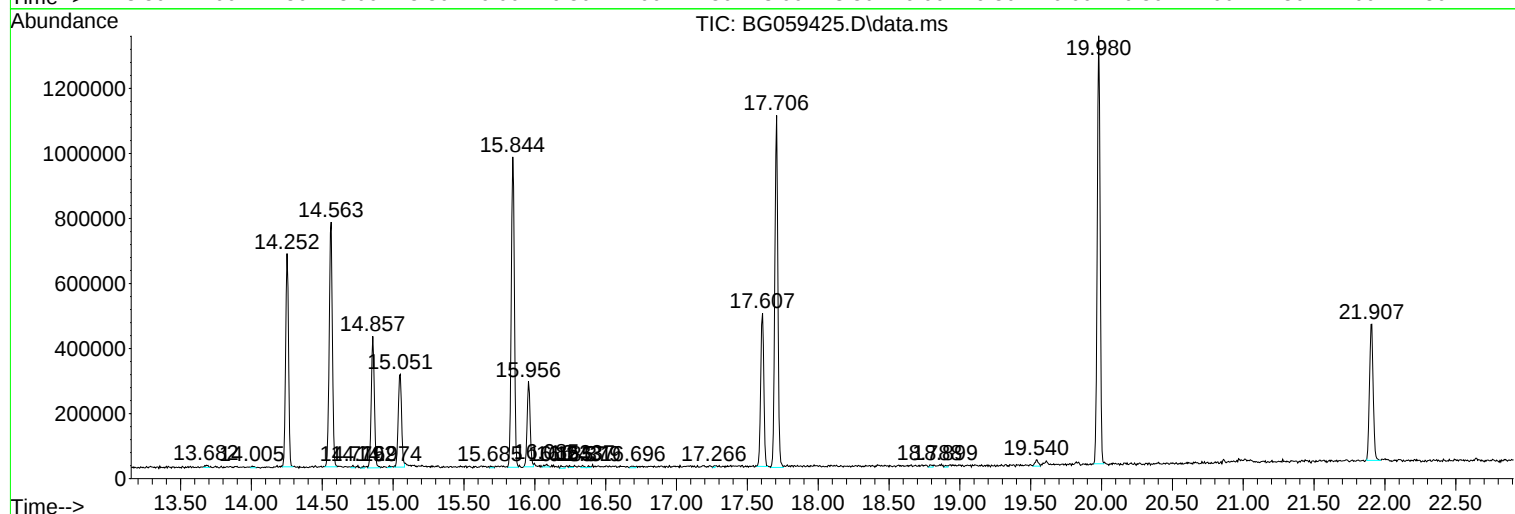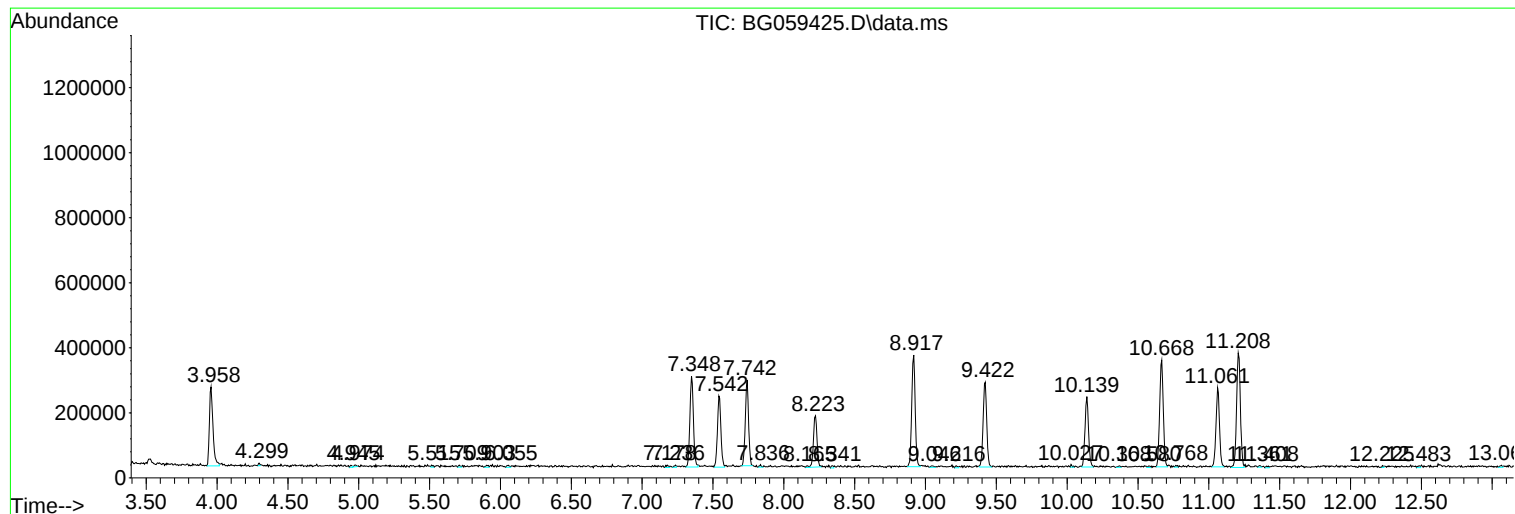

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101023\
Data File : BG059425.D
Acq On : 10 Oct 2023 15:00
Operator : MA/JU
Sample : PB156059BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101023\
Data File : BG059425.D
Acq On : 10 Oct 2023 15:00
Operator : MA/JU
Sample : PB156059BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK059

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG100723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------