
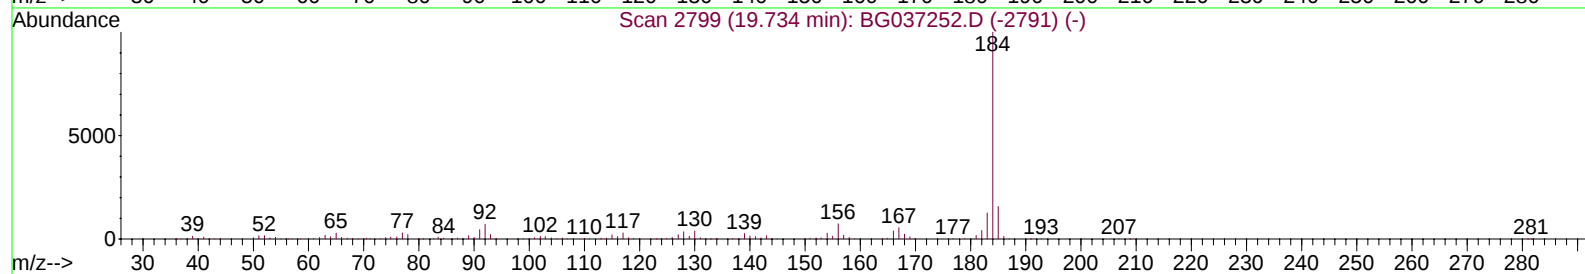
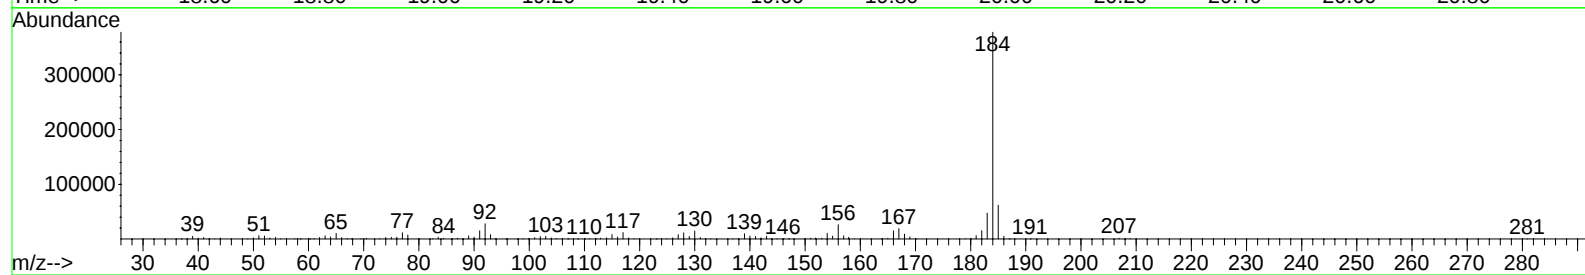


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101218\
Data File : BG037291.D
Acq On : 12 Oct 2018 15:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 16:33:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

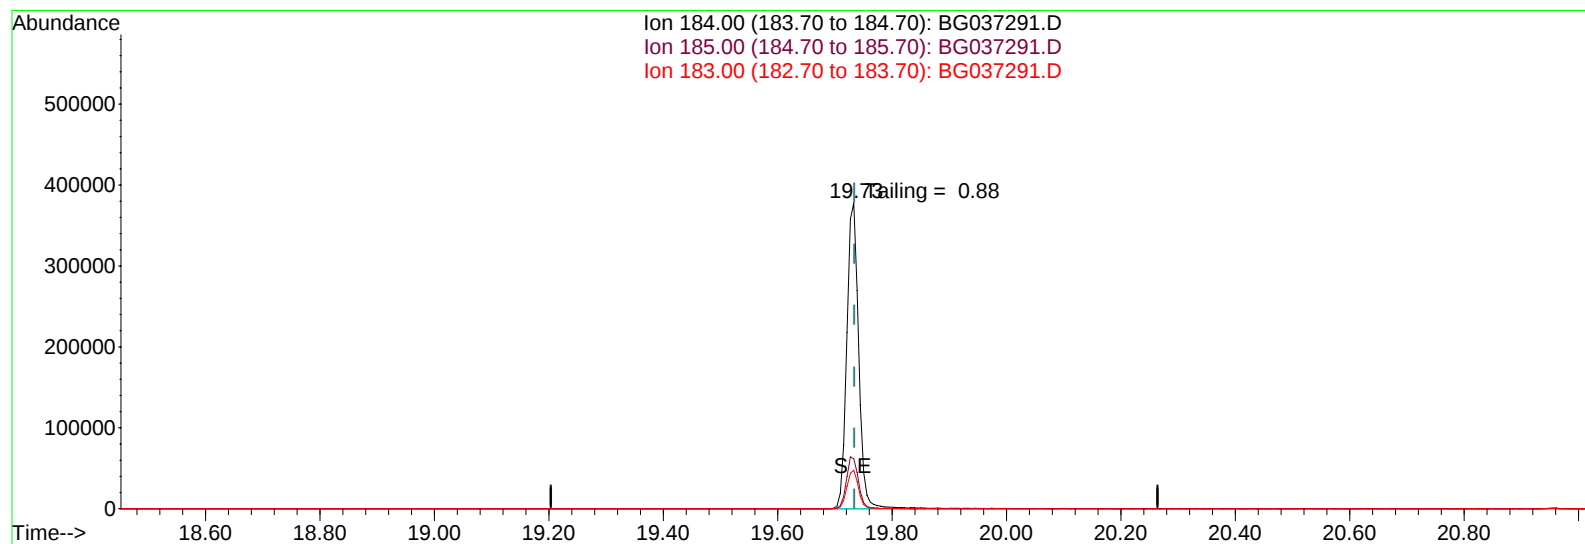

TIC: BG037291.D

(77) Benzidine




19.733min (-0.001) 0.00ng

response 546094

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.37
183.00	12.70	12.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101218\
Data File : BG037291.D
Acq On : 12 Oct 2018 15:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 16:33:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

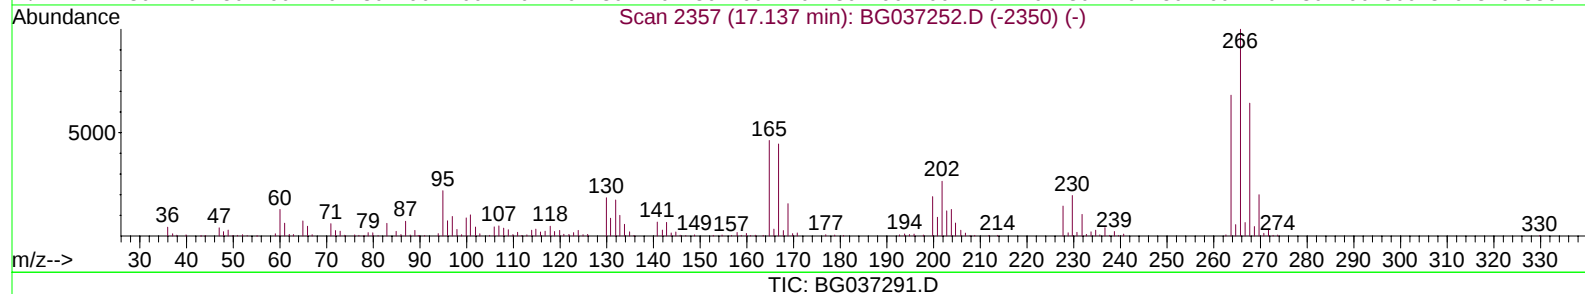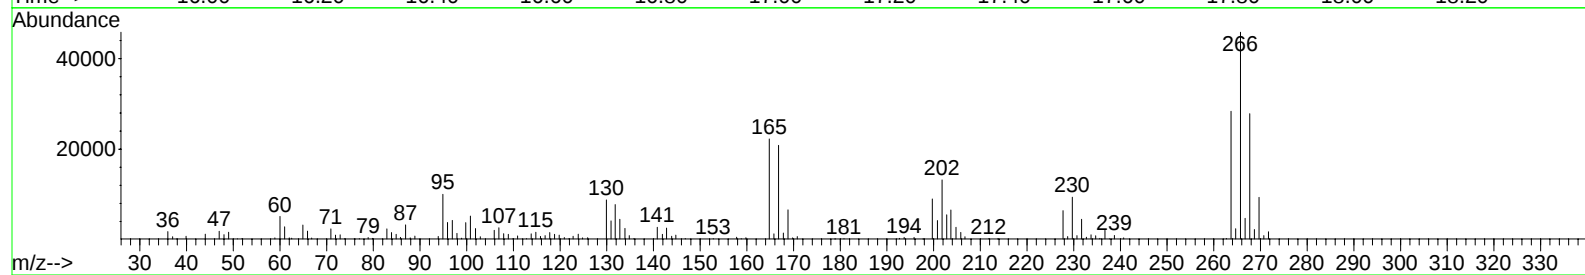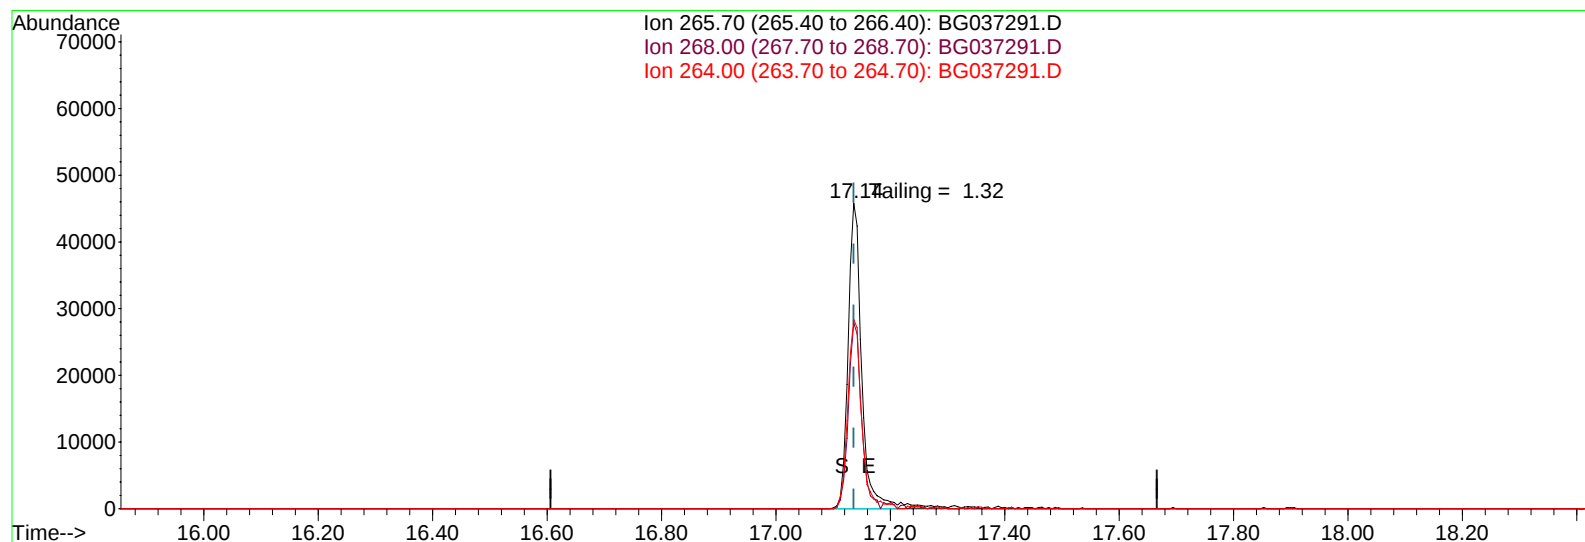

(70) Pentachlorophenol (C)

17.136min (-0.000) 24624.24ng

response 74843

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	65.66
264.00	73.60	67.18
0.00	0.00	0.00