
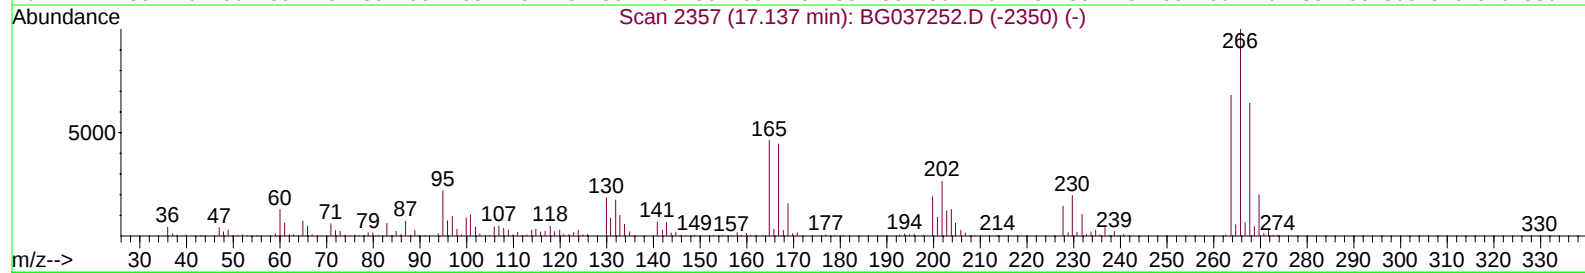
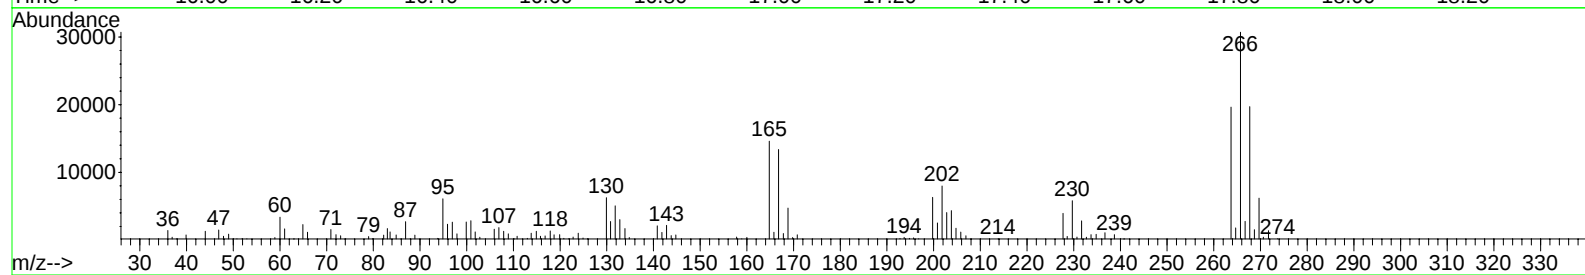


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101218\
Data File : BG037310.D
Acq On : 13 Oct 2018 4:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 03:56:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

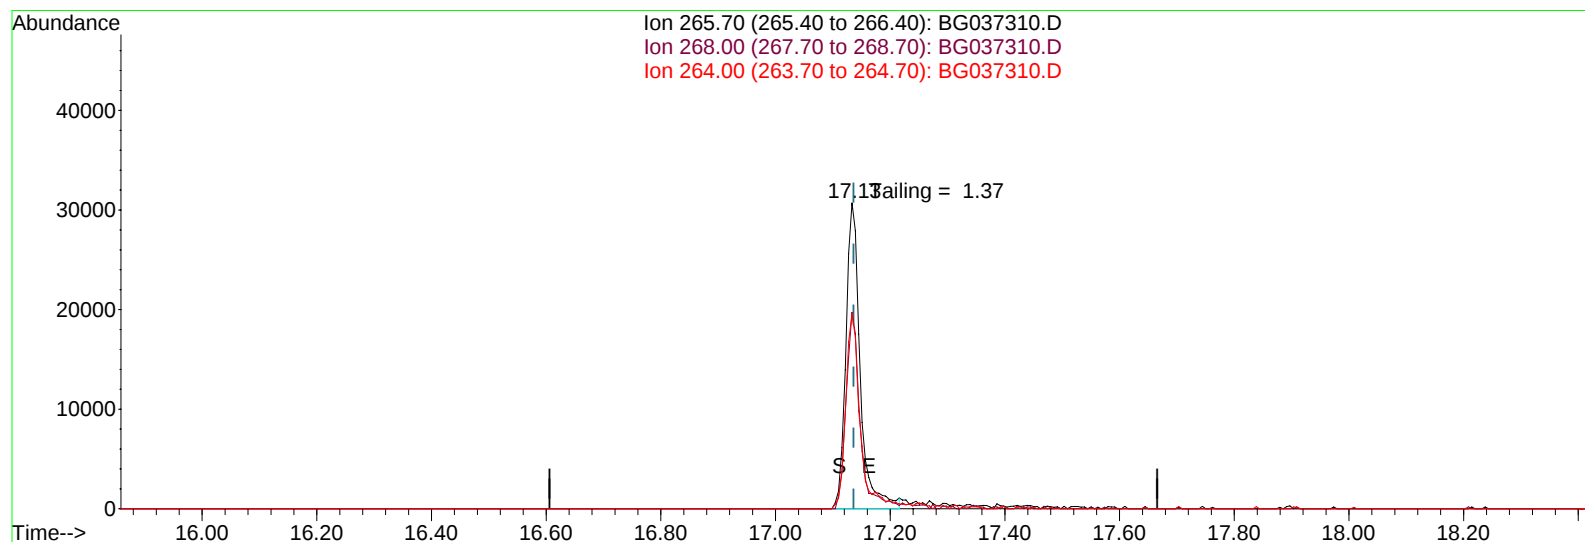

TIC: BG037310.D

(70) Pentachlorophenol (C)




17.133min (-0.003) 102635.03ng

response 53350

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	69.17
264.00	73.60	69.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101218\
Data File : BG037310.D
Acq On : 13 Oct 2018 4:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 03:56:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

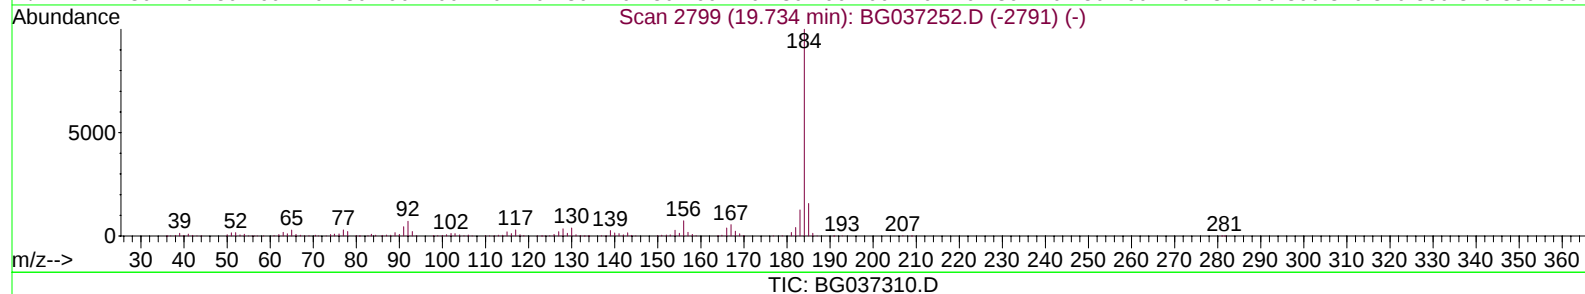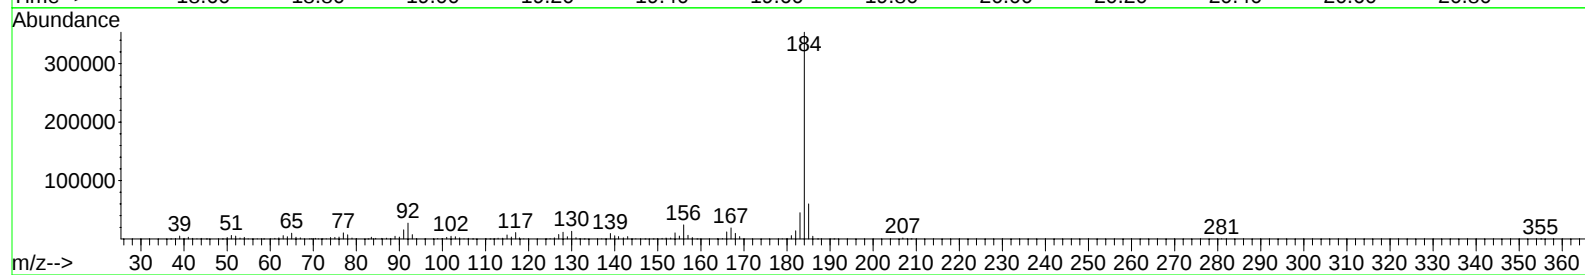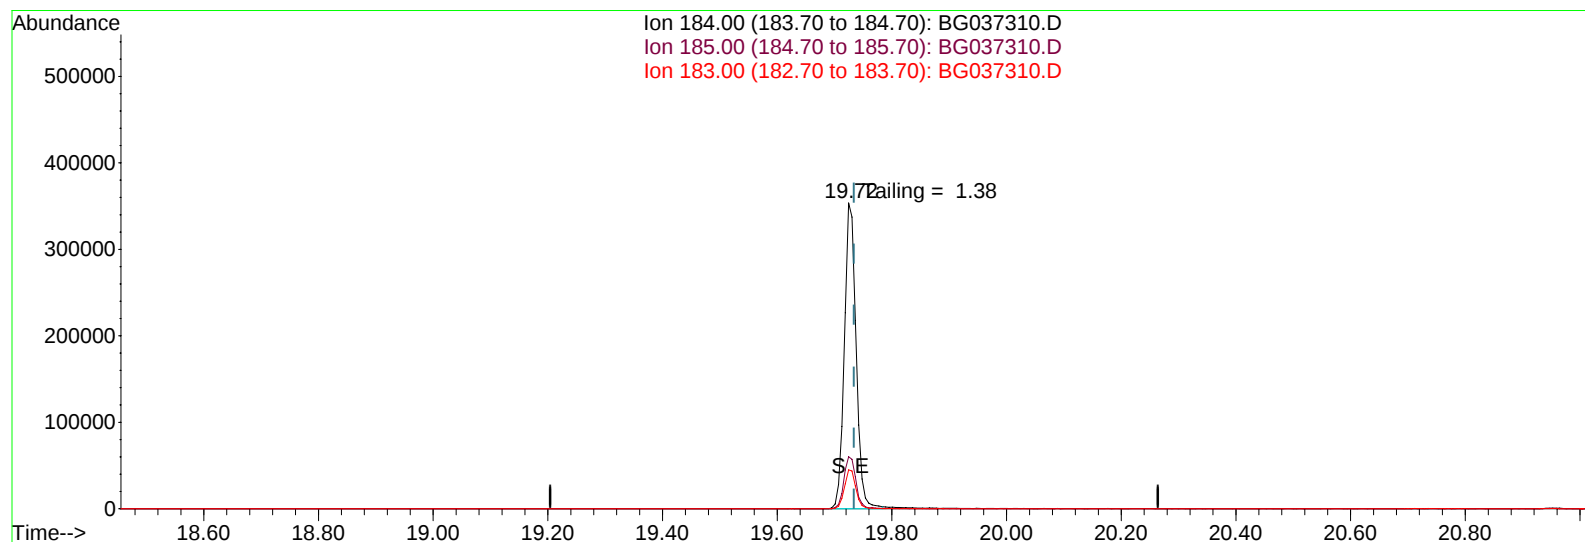

TIC: BG037310.D

(77) Benzidine

19.724min (-0.009) 0.00ng

response 509631

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.02
183.00	12.70	12.73
0.00	0.00	0.00