

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101218\
 Data File : BG037296.D
 Acq On : 12 Oct 2018 18:19
 Operator : JU/SJ
 Sample : J5450-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 VNJ218-210-282

Quant Time: Oct 13 00:27:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 13:59:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	59543	20.00	ng	0.00
21) Naphthalene-d8	10.94	136	243753	20.00	ng	0.00
39) Acenaphthene-d10	14.75	164	160901	20.00	ng	0.00
64) Phenanthrene-d10	17.50	188	421524	20.00	ng	-0.01
76) Chrysene-d12	21.78	240	413653	20.00	ng	-0.01
87) Perylene-d12	25.13	264	423426	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	372712	110.16	ng	0.00
7) Phenol-d6	7.25	99	464907	90.53	ng	0.00
23) Nitrobenzene-d5	9.29	82	338245	91.23	ng	0.00
42) 2,4,6-Tribromophenol	16.24	330	216649	137.29	ng	0.00
45) 2-Fluorobiphenyl	13.38	172	783726	73.15	ng	0.00
79) Terphenyl-d14	20.10	244	1495884	75.93	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101218\
Data File : BG037296.D
Acq On : 12 Oct 2018 18:19
Operator : JU/SJ
Sample : J5450-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
VNJ218-210-282

Quant Time: Oct 13 00:27:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

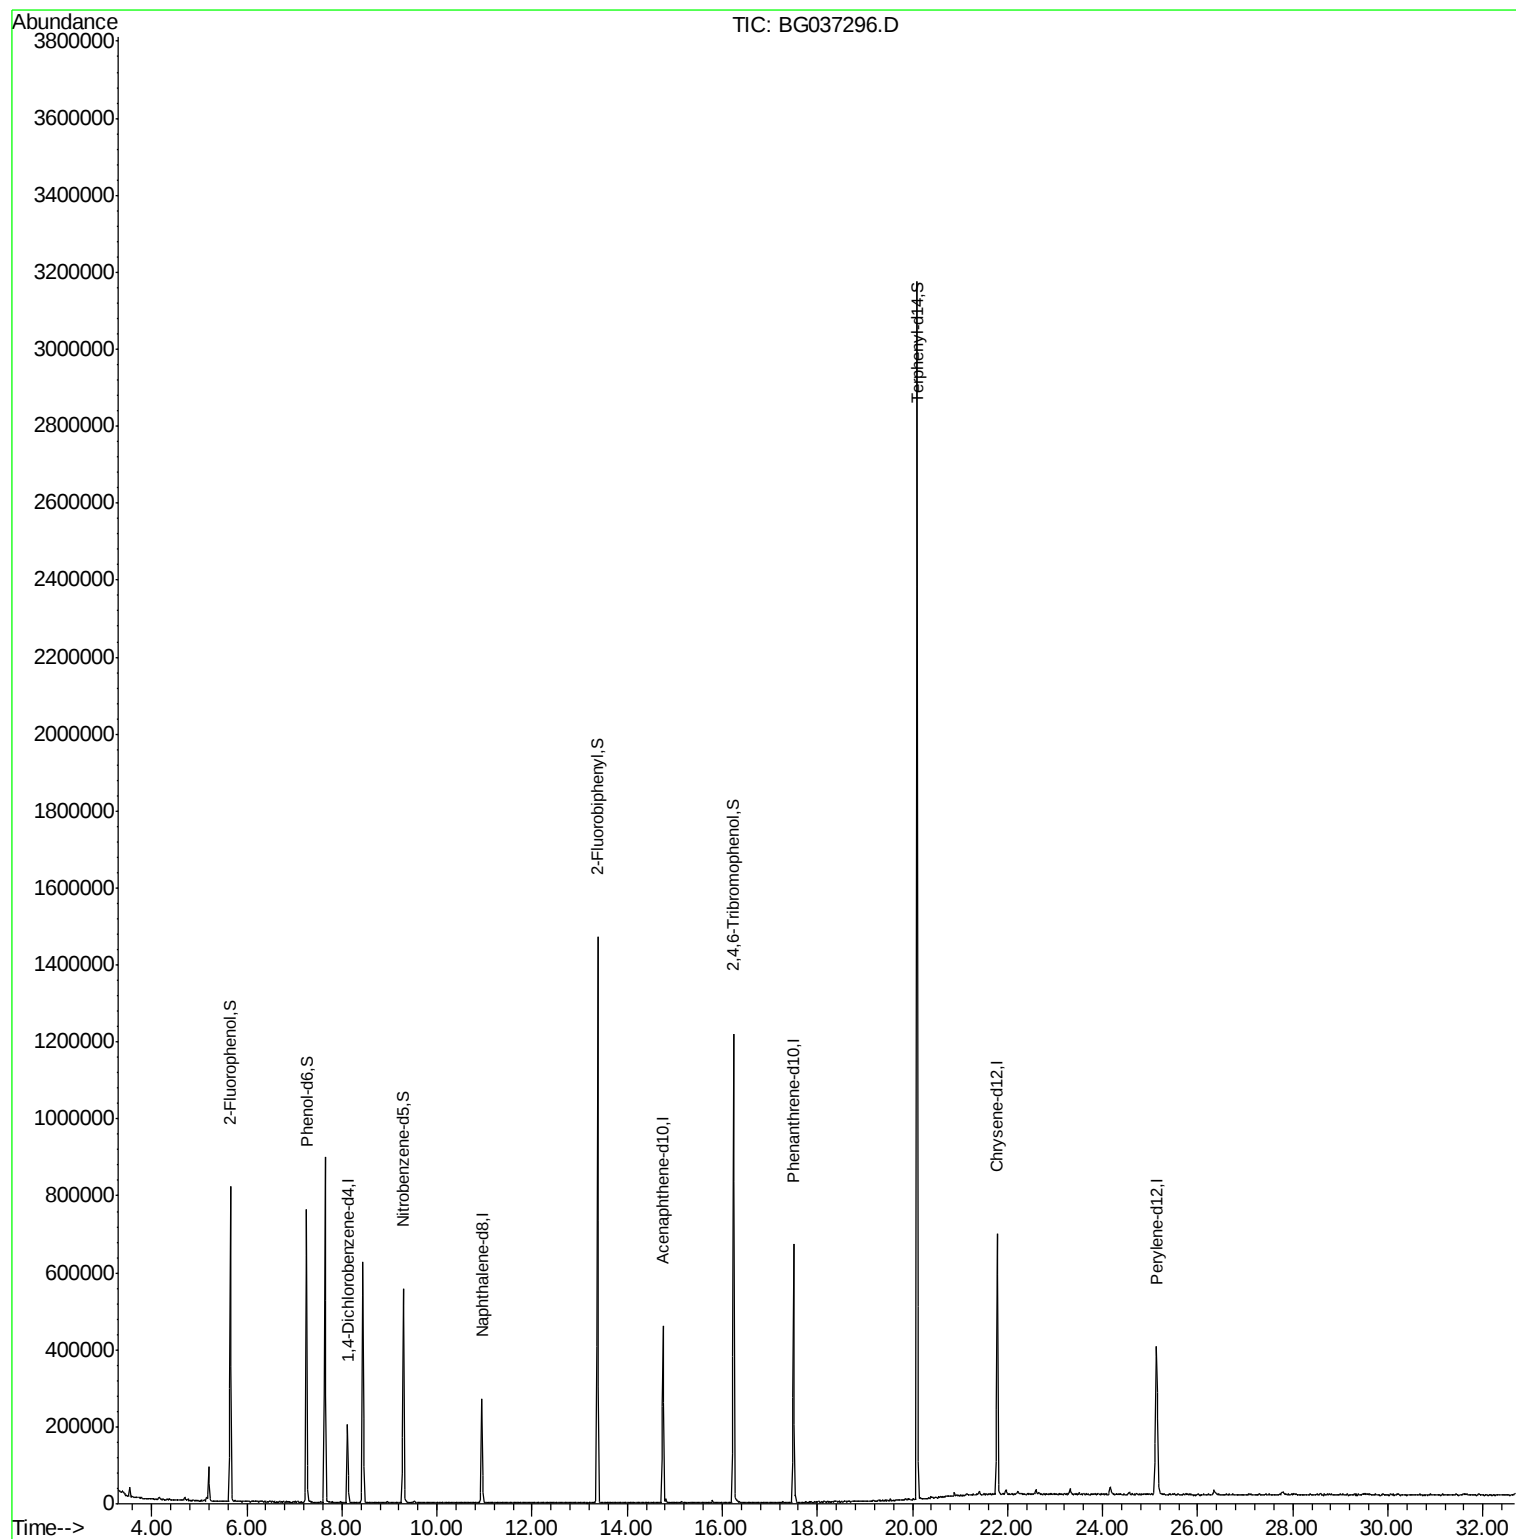

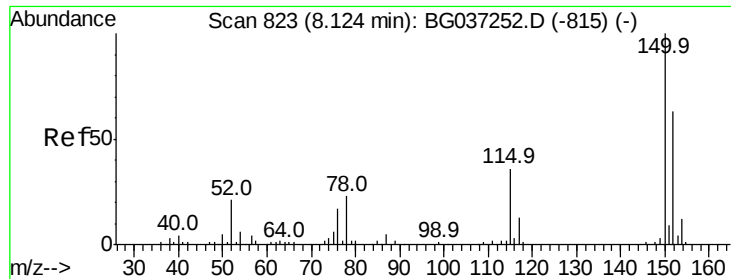


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 822
Delta R.T. -0.01 min
Lab File: BG037296.D
Acq: 12 Oct 2018 18:19

Instrument :
BNA_G
ClientSampleId :
VNJ218-210-282

Tot Ion:152 Resp: 59543
Ion Ratio Lower Upper
152 100
150 162.9 126.0 189.0
115 58.0 45.5 68.3

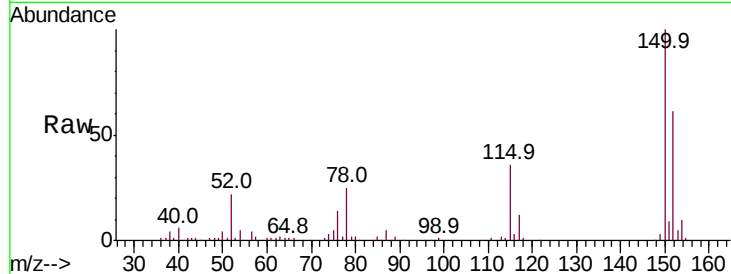


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

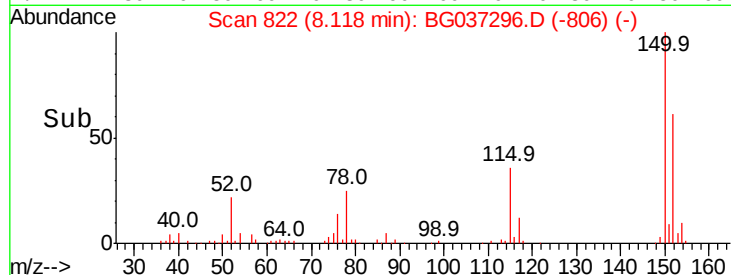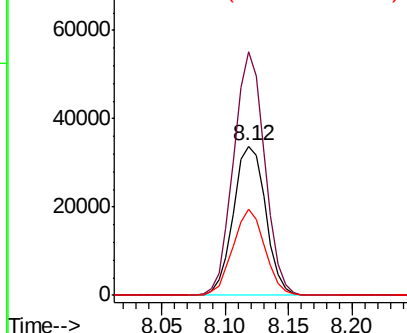



#5


2-Fluorophenol
Concen: 110.162 ng
RT: 5.66 min Scan# 403
Delta R.T. 0.01 min
Lab File: BG037296.D
Acq: 12 Oct 2018 18:19

Tgt Ion:112 Resp: 372712
Ion Ratio Lower Upper
112 100
64 65.7 53.1 79.7
63 33.6 27.3 40.9

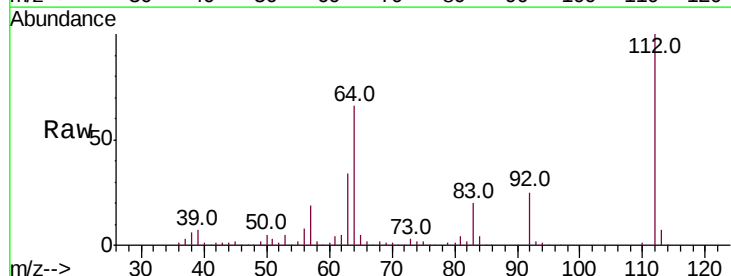

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

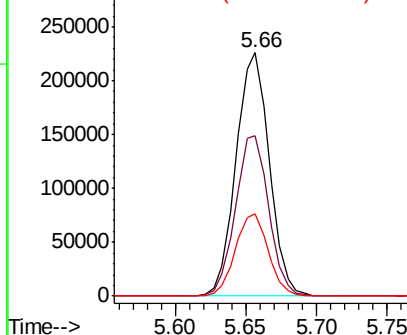

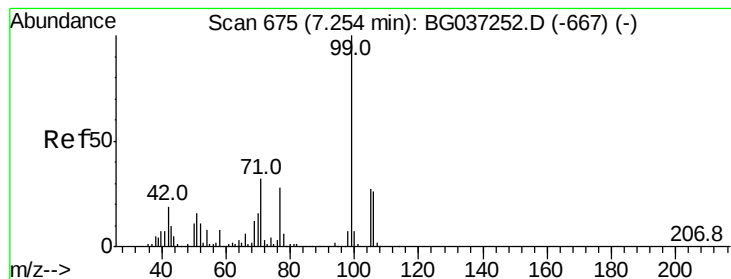

#7

Phenol-d6

Concen: 90.531 ng

RT: 7.25 min Scan# 675

Delta R.T. 0.00 min

Lab File: BG037296.D

Acq: 12 Oct 2018 18:19

Instrument :

BNA_G

ClientSampleId :

VNJ218-210-282


Tot Ion: 99 Resp: 464907

Ion Ratio Lower Upper




99 100

42 17.8 15.0 22.4

71 31.5 25.5 38.3



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

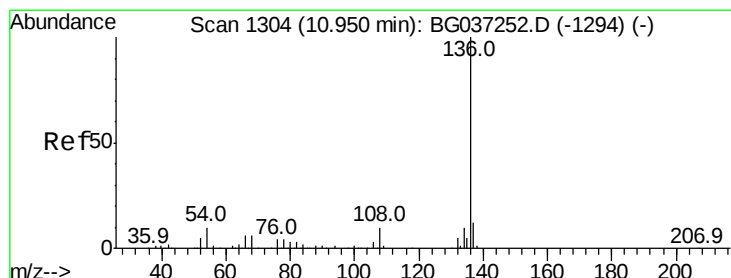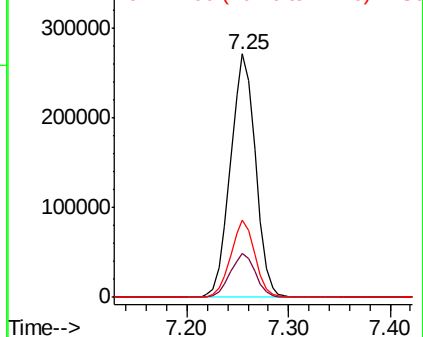

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.94 min Scan# 1303

Delta R.T. -0.01 min

Lab File: BG037296.D

Acq: 12 Oct 2018 18:19

Tgt Ion: 136 Resp: 243753


Ion Ratio Lower Upper

136 100



137 11.5 9.6 14.4


54 9.6 7.9 11.9

68 6.2 4.8 7.2



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




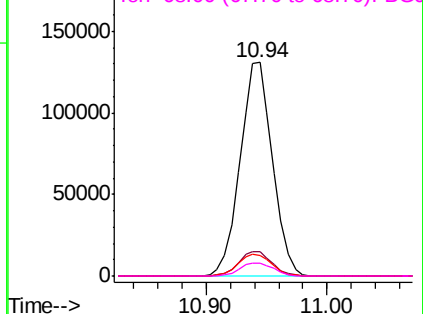




#23
Nitrobenzene-d5
Concen: 91.231 ng
RT: 9.29 min Scan# 1022
Delta R.T. -0.01 min
Lab File: BG037296.D
Acq: 12 Oct 2018 18:19




Instrument :
BNA_G
ClientSampleId :
VNJ218-210-282


Tot Ion	82	Resp	338245
Ion Ratio	Lower	Upper	
82	100		
128	42.4	34.6	51.8
54	52.3	45.3	67.9

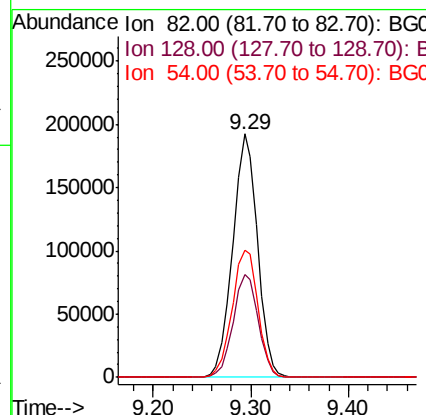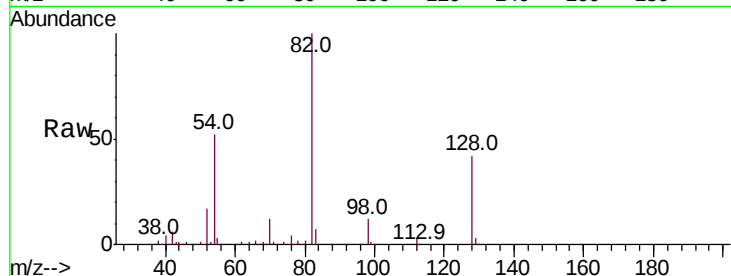

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.75 min Scan# 1951
Delta R.T. -0.01 min
Lab File: BG037296.D
Acq: 12 Oct 2018 18:19

Tgt Ion	164	Resp	160901
Ion Ratio	Lower	Upper	
164	100		
162	100.8	81.3	121.9
160	42.8	36.3	54.5

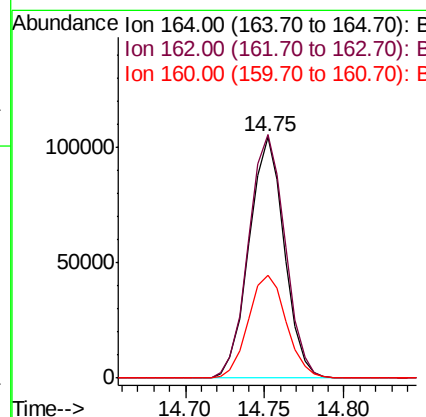




#42
 2,4,6-Tribromophenol
 Concen: 137.294 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. -0.01 min
 Lab File: BG037296.D
 Acq: 12 Oct 2018 18:19

Instrument :
 BNA_G
 ClientSampleId :
 VNJ218-210-282

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	78.4	117.6
141	39.4	32.2	48.2



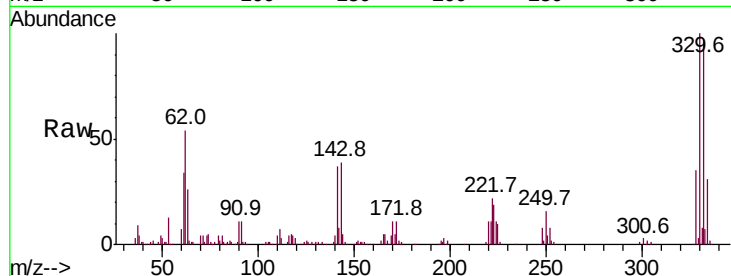


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

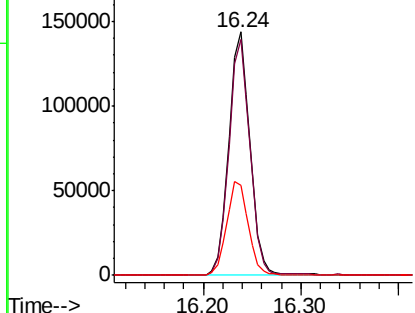

#45
 2-Fluorobiphenyl
 Concen: 73.149 ng
 RT: 13.38 min Scan# 1717
 Delta R.T. -0.01 min
 Lab File: BG037296.D
 Acq: 12 Oct 2018 18:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	31.0	46.4
170	25.5	20.2	30.2






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

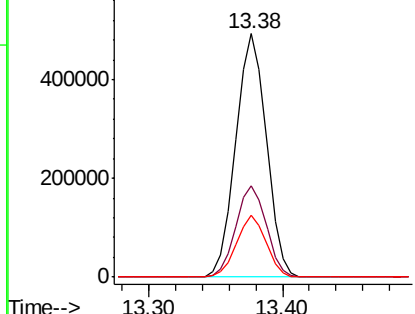



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.50 min Scan# 2418

Delta R.T. -0.01 min

Lab File: BG037296.D

Acq: 12 Oct 2018 18:19

Instrument :

BNA_G

ClientSampleId :

VNJ218-210-282


Tot Ion:188 Resp: 421524

Ion Ratio Lower Upper

188 100

94 9.2 7.2 10.8




80 10.2 7.7 11.5



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

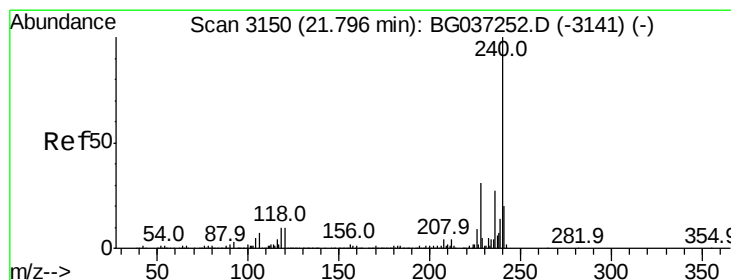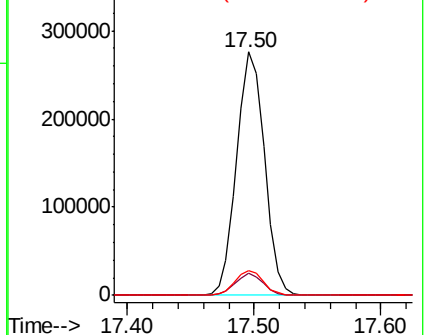

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.78 min Scan# 3148

Delta R.T. -0.01 min

Lab File: BG037296.D

Acq: 12 Oct 2018 18:19


Tgt Ion:240 Resp: 413653

Ion Ratio Lower Upper

240 100

120 10.8 8.1 12.1



236 27.8 21.4 32.0




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

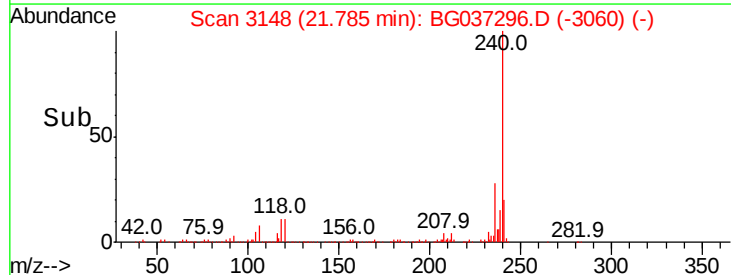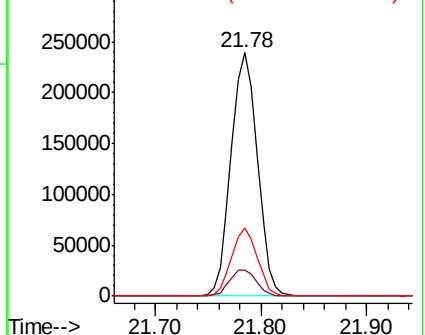

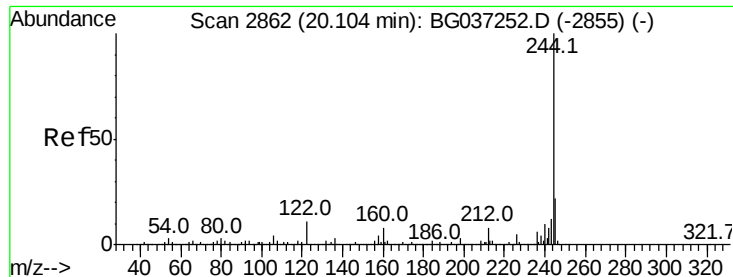

#79

Terphenyl-d14

Concen: 75.933 ng

RT: 20.10 min Scan# 2861

Delta R.T. -0.01 min

Lab File: BG037296.D

Acq: 12 Oct 2018 18:19

Instrument :

BNA_G

ClientSampleId :

VNJ218-210-282


Tot Ion:244 Resp: 1495884

Ion Ratio Lower Upper

244 100

212 8.6 6.5 9.7




122 11.5 9.0 13.4

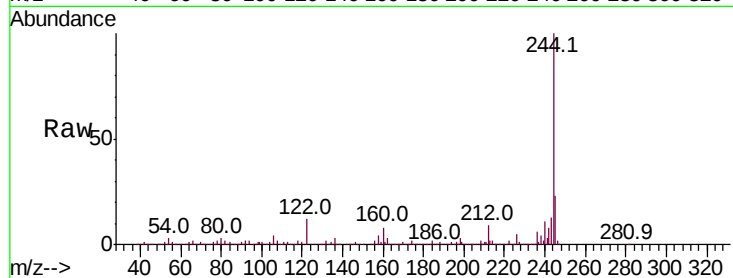

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

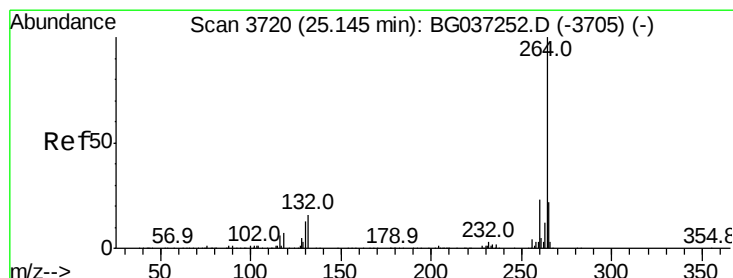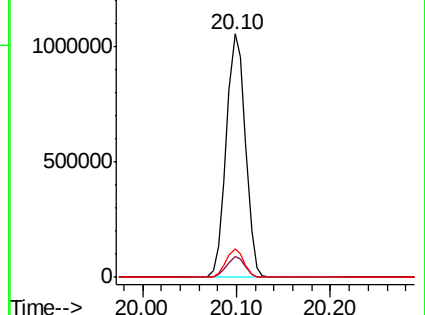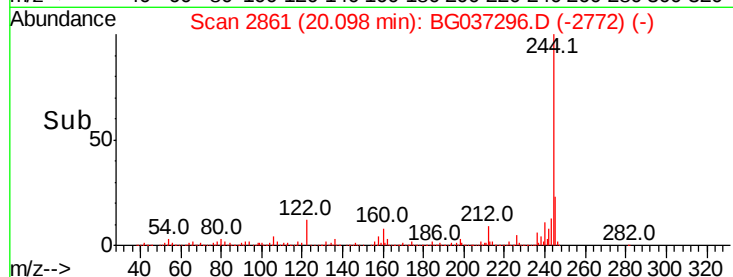

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.13 min Scan# 3718

Delta R.T. -0.01 min

Lab File: BG037296.D

Acq: 12 Oct 2018 18:19


Tgt Ion:264 Resp: 423426

Ion Ratio Lower Upper

264 100

260 23.7 18.2 27.4

265 21.2 17.9 26.9

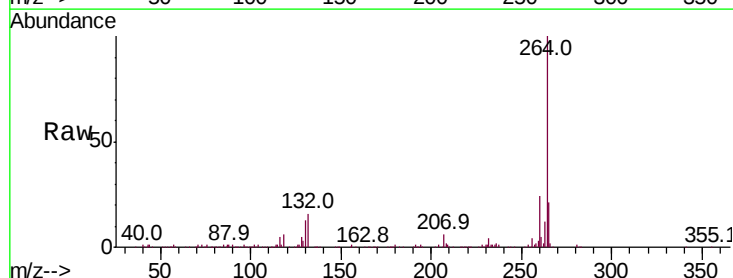

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

