

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101218\
 Data File : BG037303.D
 Acq On : 12 Oct 2018 22:55
 Operator : JU/SJ
 Sample : J5197-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 HD-01-101118

Quant Time: Oct 13 00:47:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 13:59:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	53070	20.00	ng	0.00
21) Naphthalene-d8	10.94	136	221861	20.00	ng	-0.01
39) Acenaphthene-d10	14.75	164	147483	20.00	ng	0.00
64) Phenanthrene-d10	17.50	188	397103	20.00	ng	-0.01
76) Chrysene-d12	21.78	240	382471	20.00	ng	-0.01
87) Perylene-d12	25.13	264	394146	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	364874	121.00	ng	0.00
7) Phenol-d6	7.25	99	471749	103.07	ng	0.00
23) Nitrobenzene-d5	9.29	82	323683	95.92	ng	0.00
42) 2,4,6-Tribromophenol	16.24	330	234286	161.98	ng	0.00
45) 2-Fluorobiphenyl	13.38	172	750750	76.45	ng	0.00
79) Terphenyl-d14	20.10	244	1434711	78.77	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101218\
Data File : BG037303.D
Acq On : 12 Oct 2018 22:55
Operator : JU/SJ
Sample : J5197-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
HD-01-101118

Quant Time: Oct 13 00:47:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

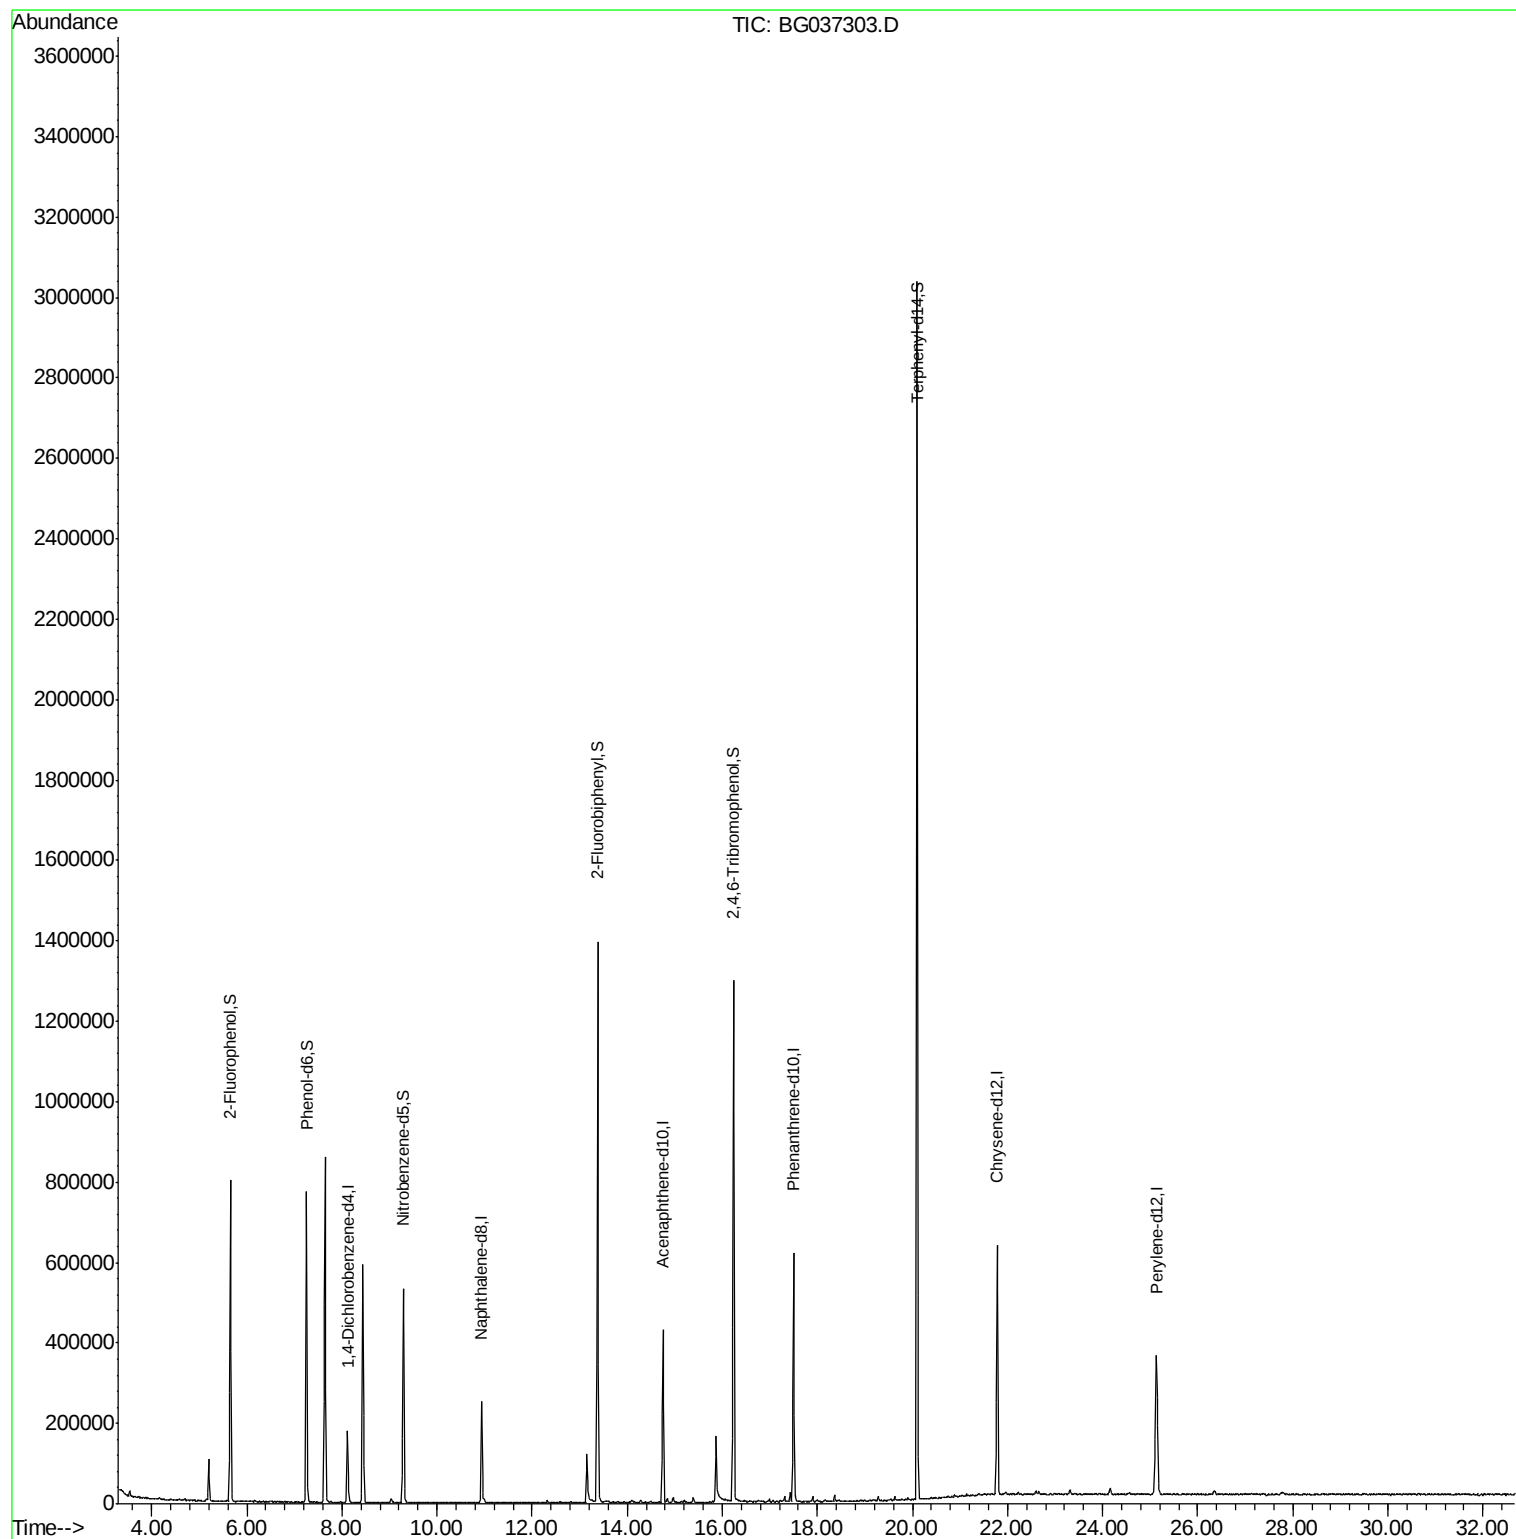

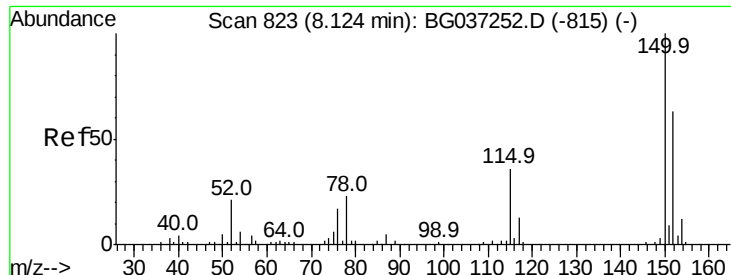


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 822
Delta R.T. -0.01 min
Lab File: BG037303.D
Acq: 12 Oct 2018 22:55

Instrument :
BNA_G
ClientSampleId :
HD-01-101118

Tot Ion:152 Resp: 53070
Ion Ratio Lower Upper
152 100
150 149.6 126.0 189.0
115 54.2 45.5 68.3

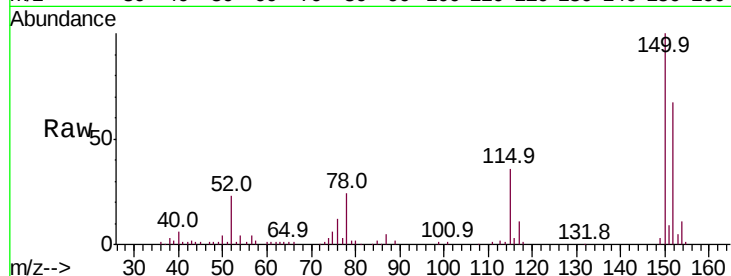


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

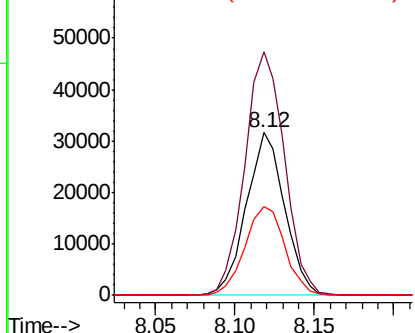



#5


2-Fluorophenol
Concen: 120.999 ng
RT: 5.66 min Scan# 403
Delta R.T. 0.01 min
Lab File: BG037303.D
Acq: 12 Oct 2018 22:55

Tgt Ion:112 Resp: 364874
Ion Ratio Lower Upper
112 100
64 65.0 53.1 79.7
63 33.6 27.3 40.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

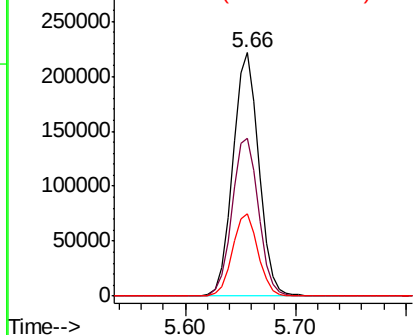



#7

Phenol-d6

Concen: 103.069 ng

RT: 7.25 min Scan# 675

Delta R.T. -0.00 min

Lab File: BG037303.D

Acq: 12 Oct 2018 22:55

Instrument :

BNA_G

ClientSampleId :

HD-01-101118


Tot Ion: 99 Resp: 471749

Ion Ratio Lower Upper




99 100

42 19.3 15.0 22.4

71 31.0 25.5 38.3

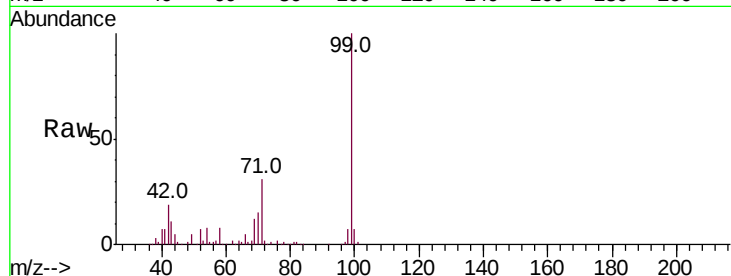

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

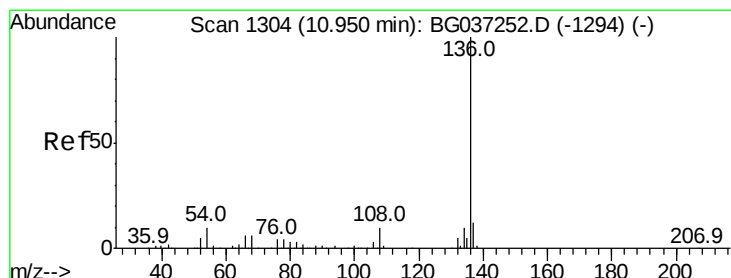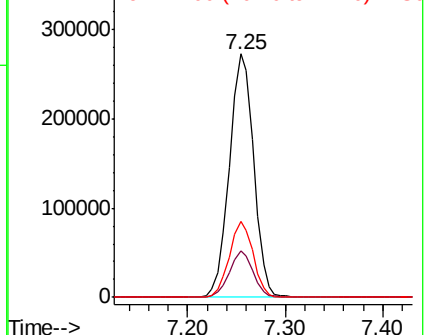

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.94 min Scan# 1302

Delta R.T. -0.01 min

Lab File: BG037303.D

Acq: 12 Oct 2018 22:55

Tgt Ion: 136 Resp: 221861


Ion Ratio Lower Upper

136 100



137 11.4 9.6 14.4


54 10.4 7.9 11.9

68 6.6 4.8 7.2



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

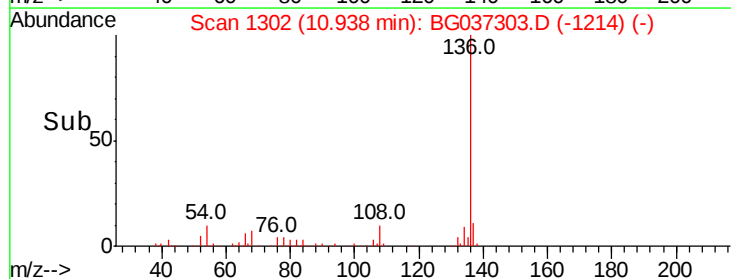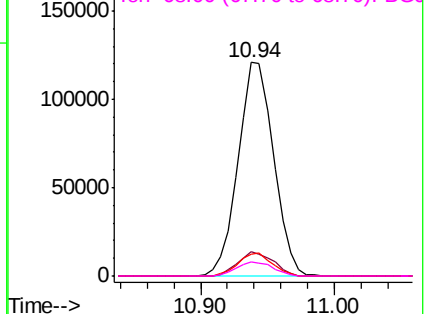




#23
Nitrobenzene-d5
Concen: 95.918 ng
RT: 9.29 min Scan# 1022
Delta R.T. -0.01 min
Lab File: BG037303.D
Acq: 12 Oct 2018 22:55

Instrument :
BNA_G
ClientSampleId :
HD-01-101118

Tot Ion	Ratio	Lower	Upper
82	100		
128	43.1	34.6	51.8
54	54.4	45.3	67.9



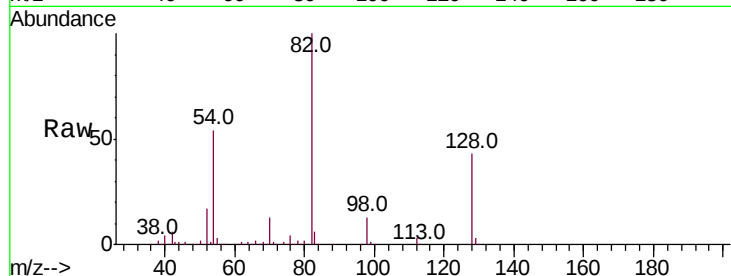


Abundance

Ion 82.00 (81.70 to 82.70): BGC


Ion 128.00 (127.70 to 128.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

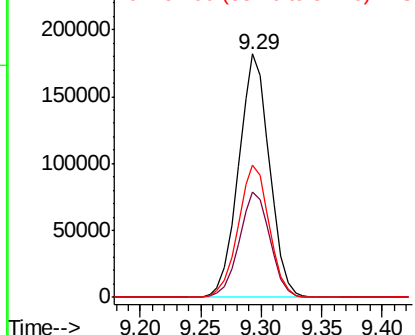

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.75 min Scan# 1951
Delta R.T. -0.01 min
Lab File: BG037303.D
Acq: 12 Oct 2018 22:55

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.2	81.3	121.9
160	43.4	36.3	54.5






Abundance

Ion 164.00 (163.70 to 164.70): BGC

Ion 162.00 (161.70 to 162.70): BGC

Ion 160.00 (159.70 to 160.70): BGC

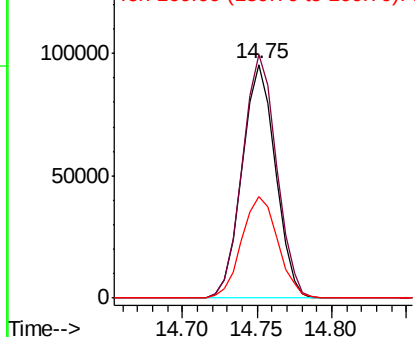


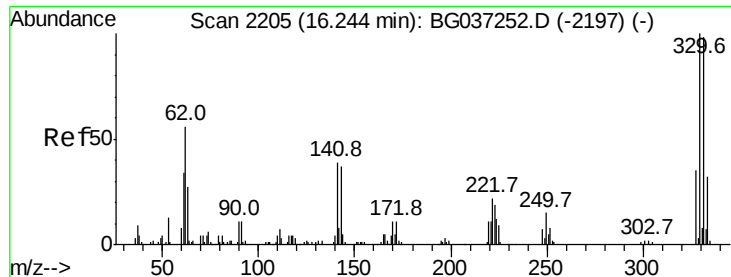

#42
 2,4,6-Tribromophenol
 Concen: 161.979 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. -0.01 min
 Lab File: BG037303.D
 Acq: 12 Oct 2018 22:55

Instrument :
 BNA_G
 ClientSampleId :
 HD-01-101118

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.1	78.4	117.6
141	39.8	32.2	48.2



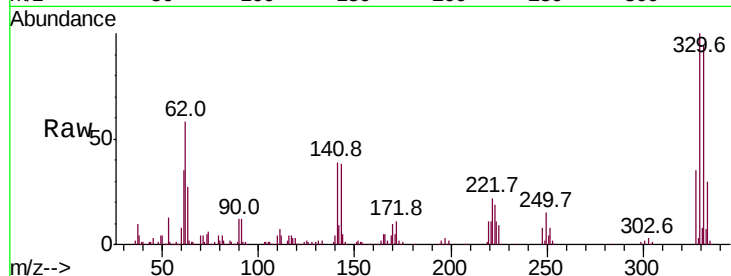


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

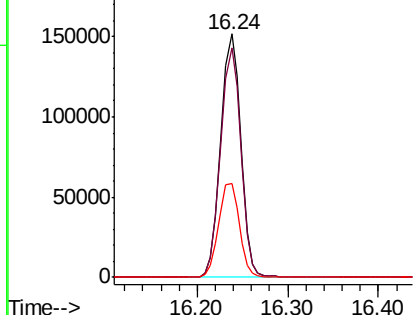

#45
 2-Fluorobiphenyl
 Concen: 76.446 ng
 RT: 13.38 min Scan# 1717
 Delta R.T. -0.01 min
 Lab File: BG037303.D
 Acq: 12 Oct 2018 22:55

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.9	31.0	46.4
170	25.5	20.2	30.2






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

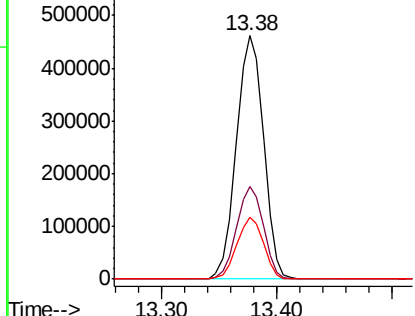

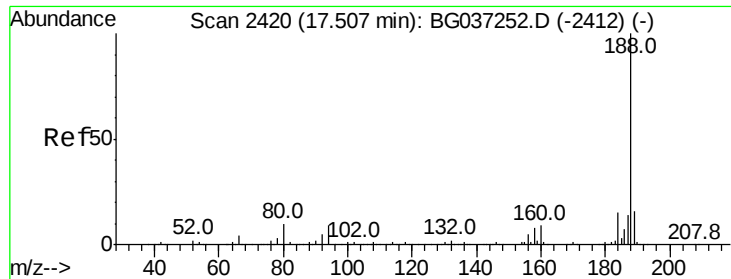

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.50 min Scan# 2418

Delta R.T. -0.01 min

Lab File: BG037303.D

Acq: 12 Oct 2018 22:55

Instrument :

BNA_G

ClientSampleId :

HD-01-101118


Tot Ion:188 Resp: 397103

Ion Ratio Lower Upper

188 100

94 9.5 7.2 10.8




80 10.3 7.7 11.5



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

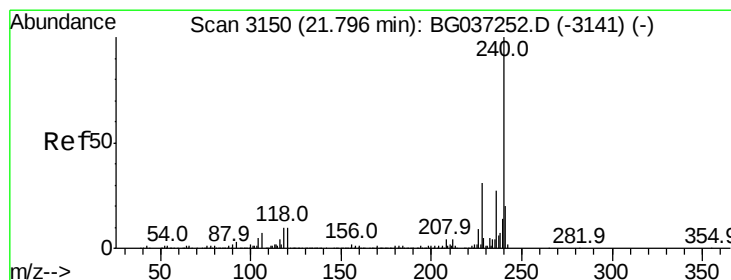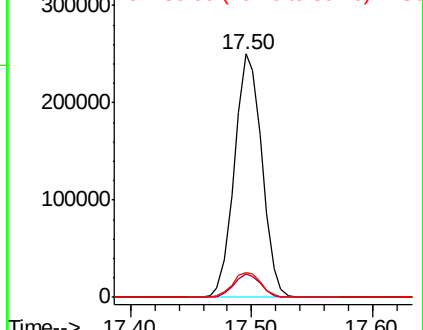

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.78 min Scan# 3148

Delta R.T. -0.01 min

Lab File: BG037303.D

Acq: 12 Oct 2018 22:55


Tgt Ion:240 Resp: 382471

Ion Ratio Lower Upper

240 100

120 10.7 8.1 12.1



236 27.5 21.4 32.0




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

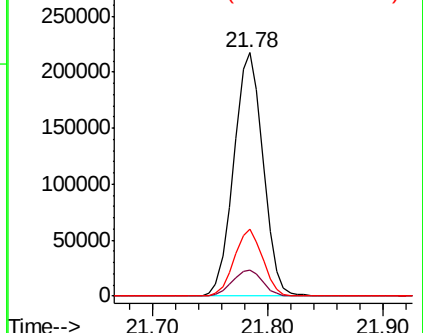

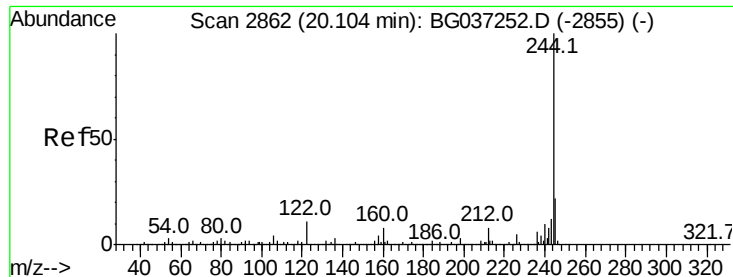

#79

Terphenyl-d14

Concen: 78.765 ng

RT: 20.10 min Scan# 2861

Delta R.T. -0.01 min

Lab File: BG037303.D

Acq: 12 Oct 2018 22:55

Instrument :

BNA_G

ClientSampleId :

HD-01-101118


Tot Ion:244 Resp: 1434711

Ion Ratio Lower Upper

244 100

212 8.5 6.5 9.7




122 11.7 9.0 13.4

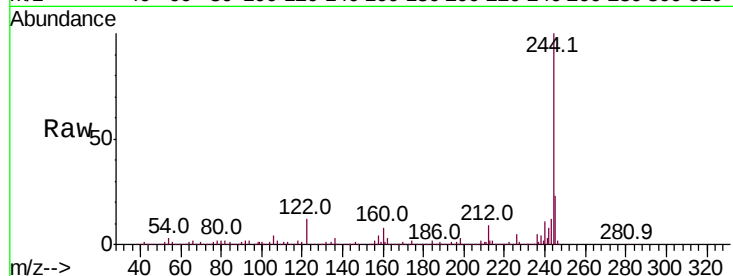

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

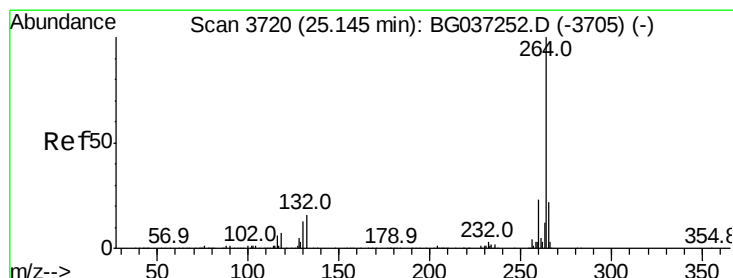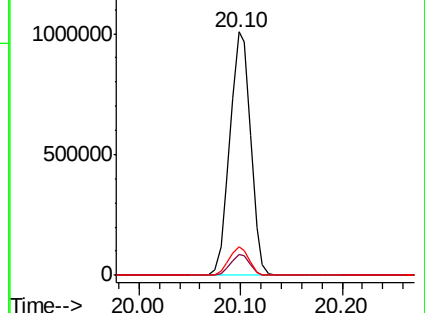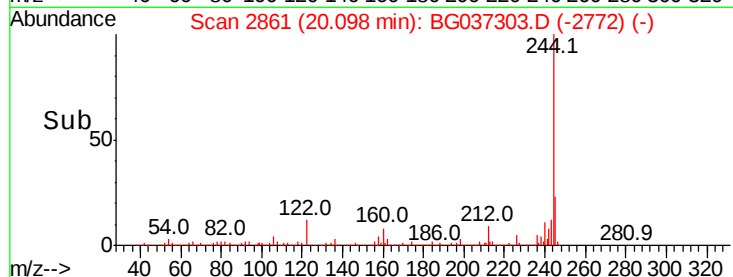

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.13 min Scan# 3718

Delta R.T. -0.01 min

Lab File: BG037303.D

Acq: 12 Oct 2018 22:55


Tgt Ion:264 Resp: 394146

Ion Ratio Lower Upper

264 100

260 23.3 18.2 27.4

265 22.2 17.9 26.9

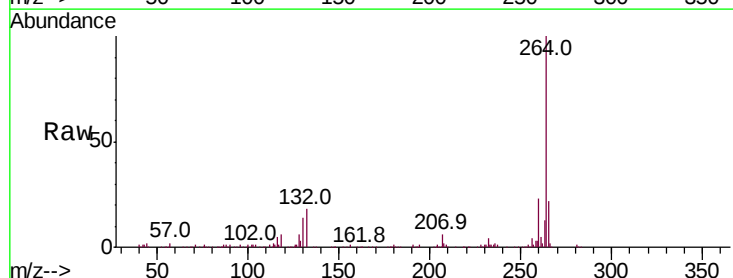

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

