

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101218\
 Data File : BG037325.D
 Acq On : 13 Oct 2018 13:56
 Operator : JU/SJ
 Sample : J5383-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 100918-DBRI-F-U-S

Quant Time: Oct 15 02:46:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 13:59:58 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	57746	20.00	ng	0.00
21) Naphthalene-d8	10.94	136	241009	20.00	ng	-0.01
39) Acenaphthene-d10	14.75	164	163440	20.00	ng	0.00
64) Phenanthrene-d10	17.49	188	418681	20.00	ng	-0.01
76) Chrysene-d12	21.78	240	406576	20.00	ng	-0.02
87) Perylene-d12	25.13	264	410349	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	158829	48.41	ng	0.00
7) Phenol-d6	7.25	99	143408	28.79	ng	0.00
23) Nitrobenzene-d5	9.29	82	434313	118.48	ng	0.00
42) 2,4,6-Tribromophenol	16.24	330	191078	119.21	ng	0.00
45) 2-Fluorobiphenyl	13.38	172	1061306	97.52	ng	0.00
79) Terphenyl-d14	20.10	244	1723745	89.02	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.19	163	37378	2.910	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101218\
Data File : BG037325.D
Acq On : 13 Oct 2018 13:56
Operator : JU/SJ
Sample : J5383-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
100918-DBRI-F-U-S

Quant Time: Oct 15 02:46:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

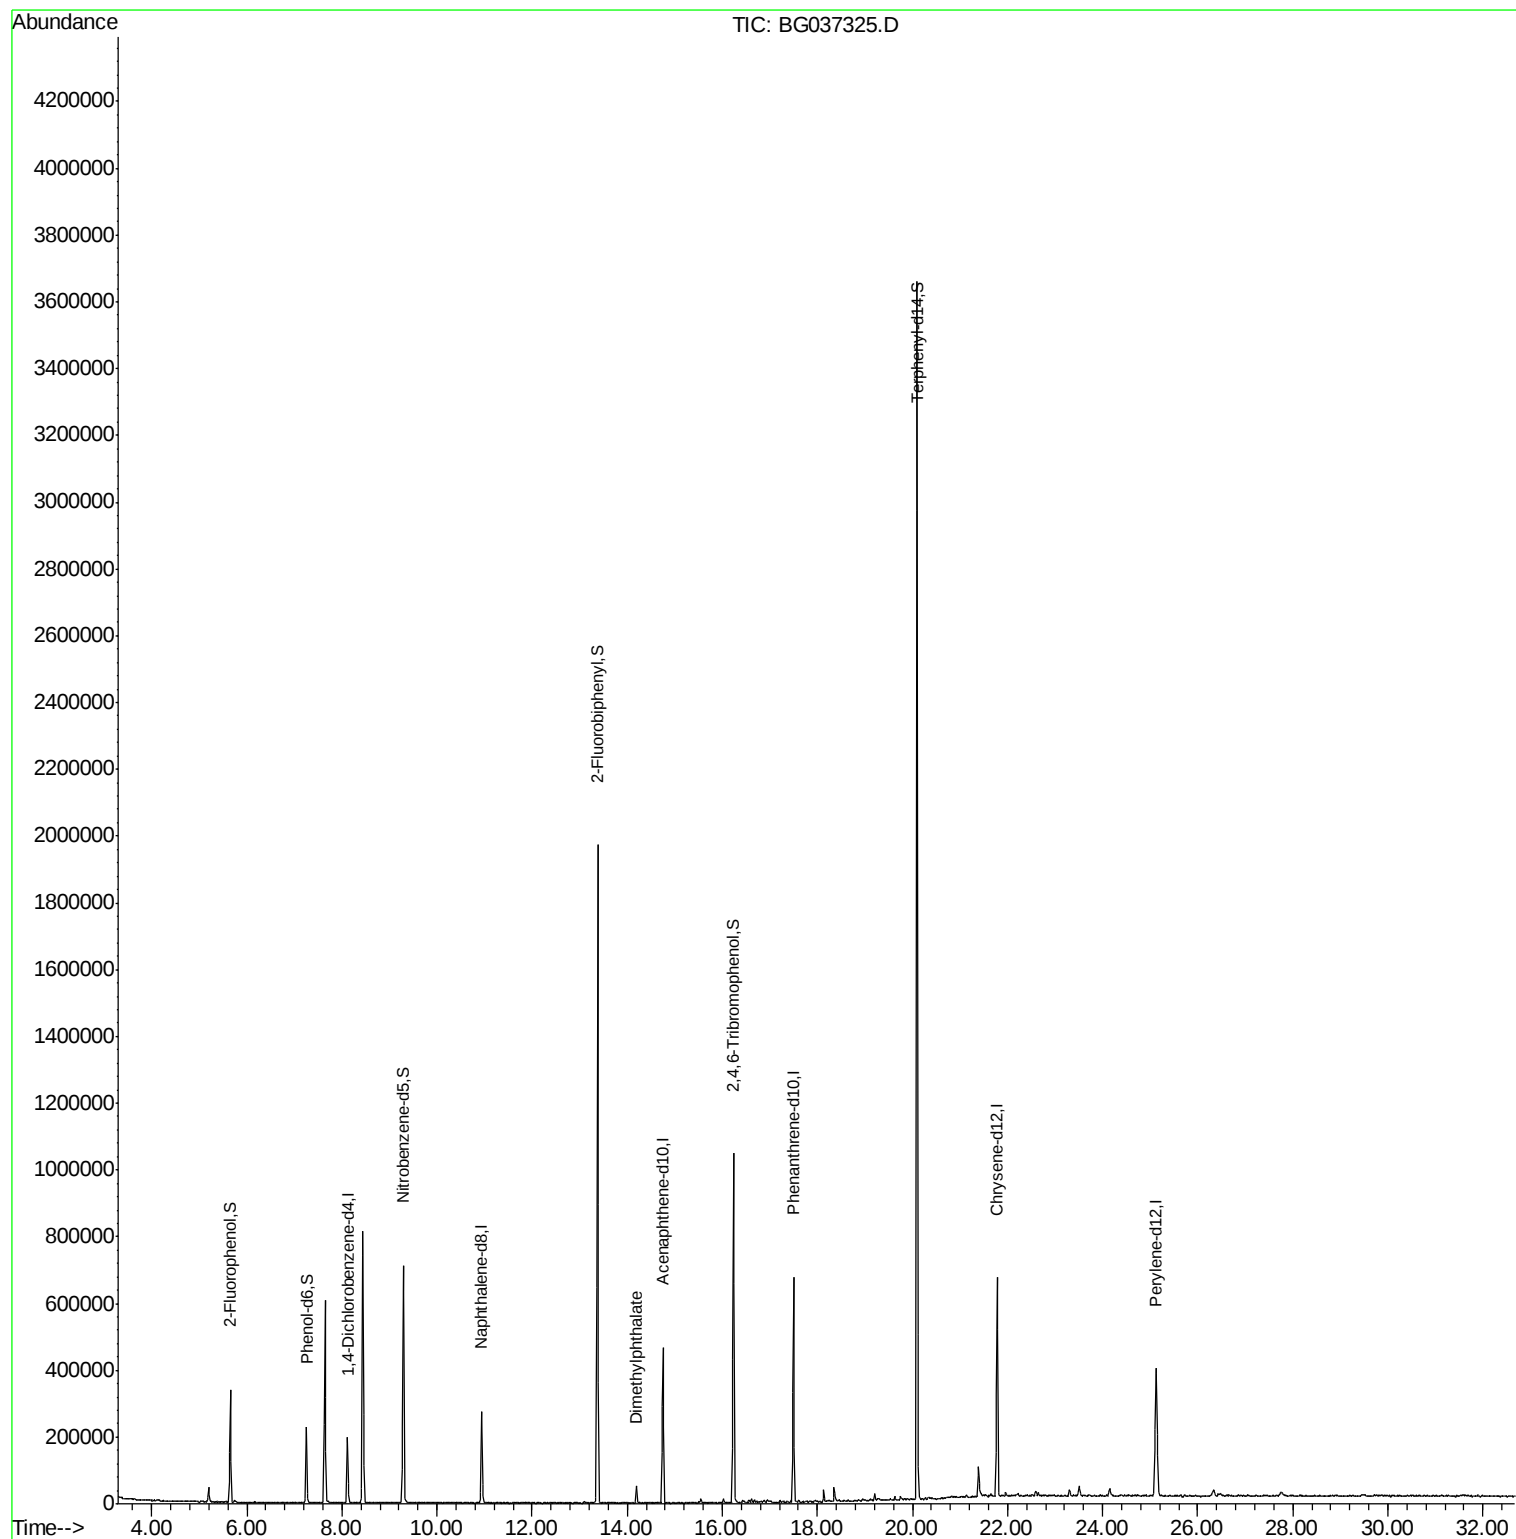

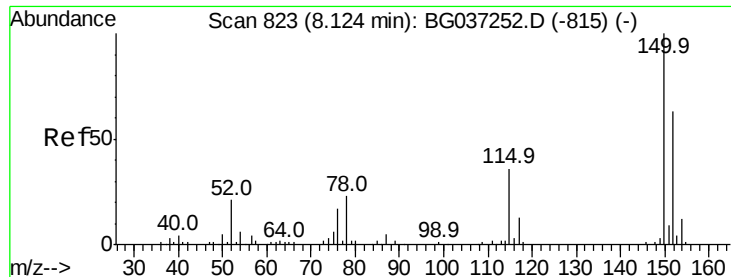


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 822
Delta R.T. -0.01 min
Lab File: BG037325.D
Acq: 13 Oct 2018 13:56

Instrument :
BNA_G
ClientSampleId :
100918-DBRI-F-U-S

Tot Ion:152 Resp: 57746
Ion Ratio Lower Upper
152 100
150 156.1 126.0 189.0
115 53.9 45.5 68.3

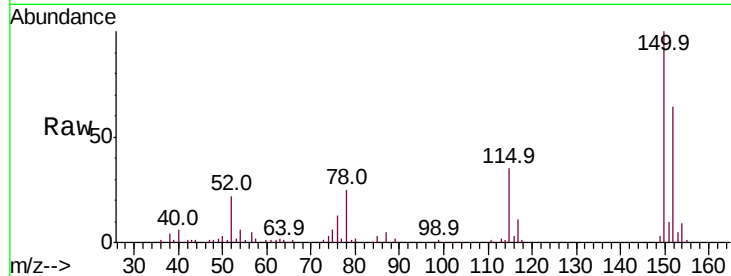


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

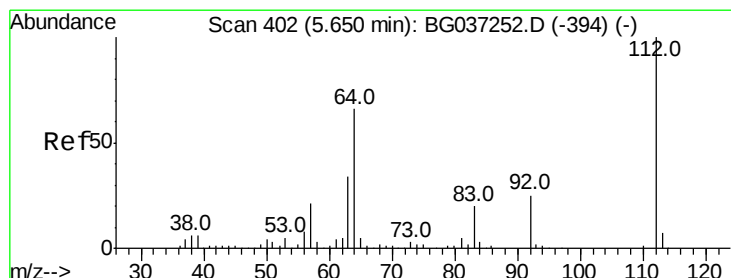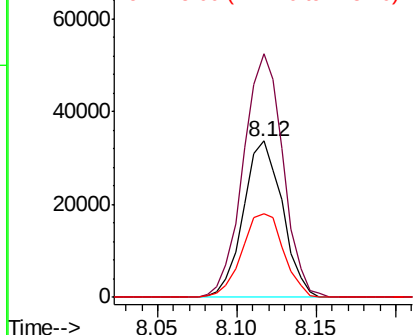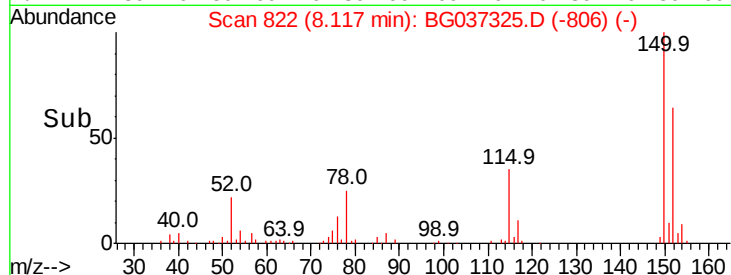



#5


2-Fluorophenol
Concen: 48.406 ng
RT: 5.65 min Scan# 402
Delta R.T. -0.00 min
Lab File: BG037325.D
Acq: 13 Oct 2018 13:56

Tgt Ion:112 Resp: 158829
Ion Ratio Lower Upper
112 100
64 66.7 53.1 79.7
63 33.5 27.3 40.9

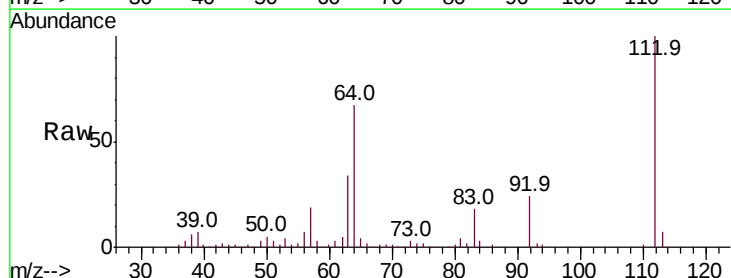

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

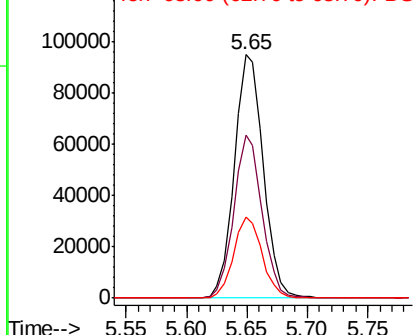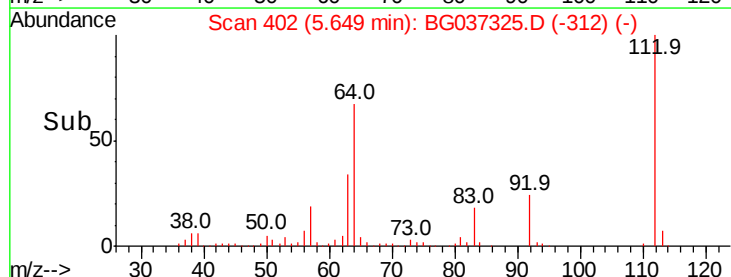

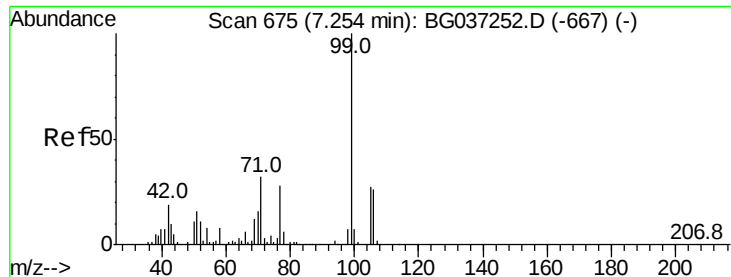

#7

Phenol-d6

Concen: 28.795 ng

RT: 7.25 min Scan# 675

Delta R.T. -0.00 min

Lab File: BG037325.D

Acq: 13 Oct 2018 13:56

Instrument :

BNA_G

ClientSampleId :

100918-DBRI-F-U-S


Tot Ion: 99 Resp: 143408

Ion Ratio Lower Upper




99 100

42 17.3 15.0 22.4

71 27.6 25.5 38.3

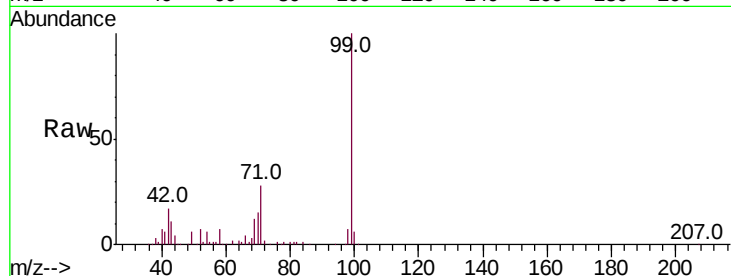

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

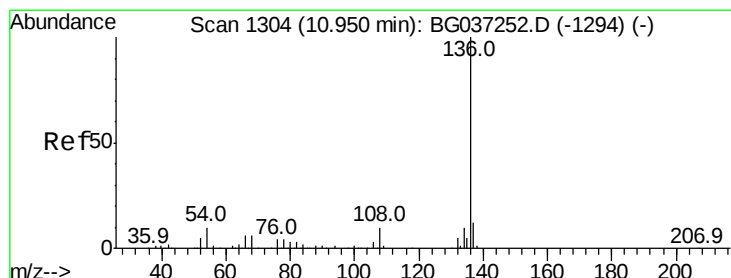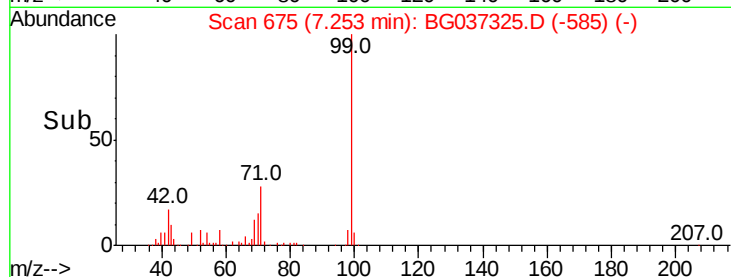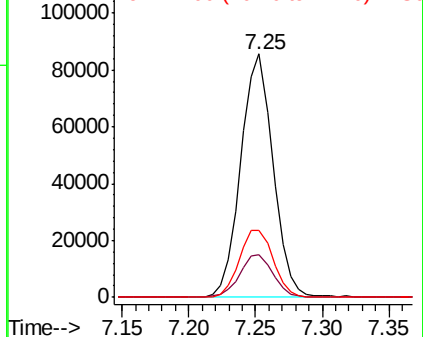

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.94 min Scan# 1302

Delta R.T. -0.01 min

Lab File: BG037325.D

Acq: 13 Oct 2018 13:56

Tgt Ion: 136 Resp: 241009


Ion Ratio Lower Upper

136 100



137 12.4 9.6 14.4


54 11.2 7.9 11.9

68 7.0 4.8 7.2

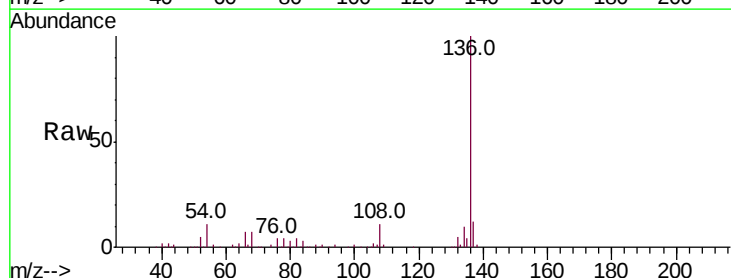

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

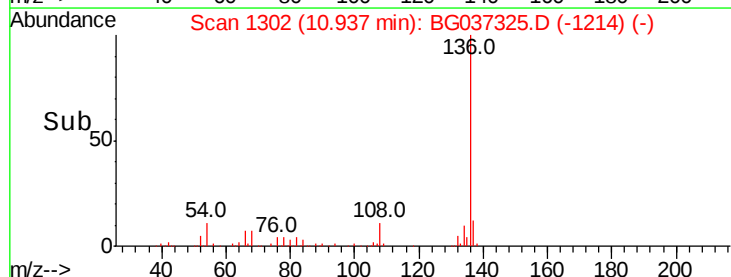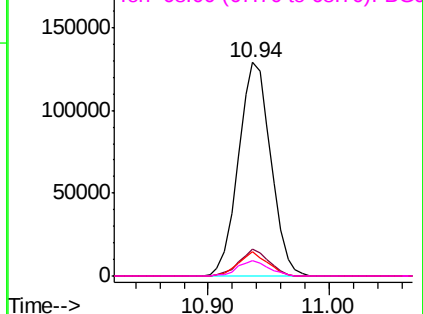


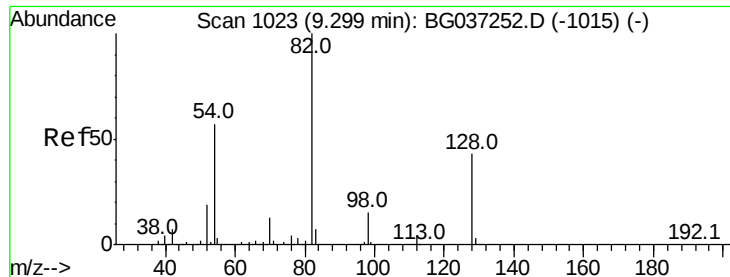

#23
 Nitrobenzene-d5
 Concen: 118.476 ng
 RT: 9.29 min Scan# 1022
 Delta R.T. -0.01 min
 Lab File: BG037325.D
 Acq: 13 Oct 2018 13:56

Instrument :
 BNA_G
 ClientSampleId :
 100918-DBRI-F-U-S

Tot Ion	82	Resp	434313
Ion Ratio	Lower	Upper	
82	100		
128	43.7	34.6	51.8
54	55.2	45.3	67.9



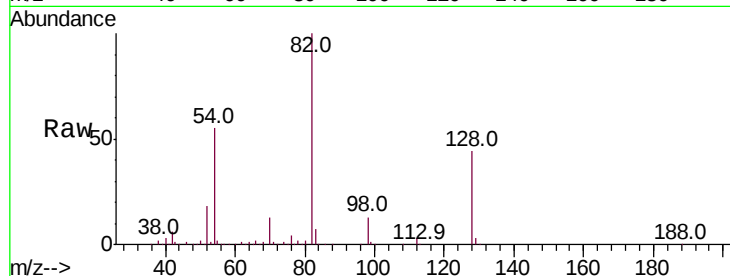


Abundance

Ion 82.00 (81.70 to 82.70): BGC


Ion 128.00 (127.70 to 128.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

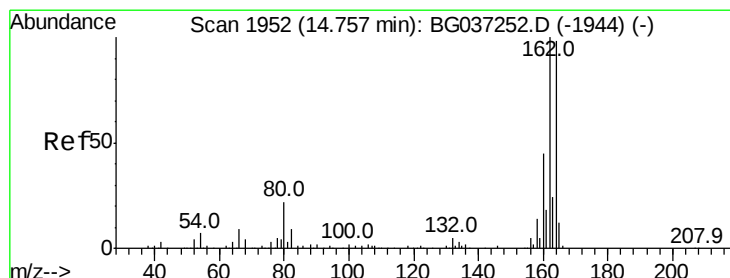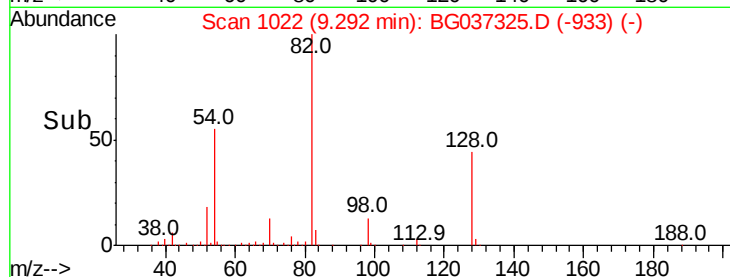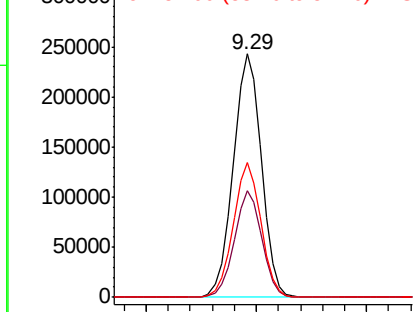

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.75 min Scan# 1951
 Delta R.T. -0.01 min
 Lab File: BG037325.D
 Acq: 13 Oct 2018 13:56

Tgt Ion	164	Resp	163440
Ion Ratio	Lower	Upper	
164	100		
162	107.7	81.3	121.9
160	47.9	36.3	54.5


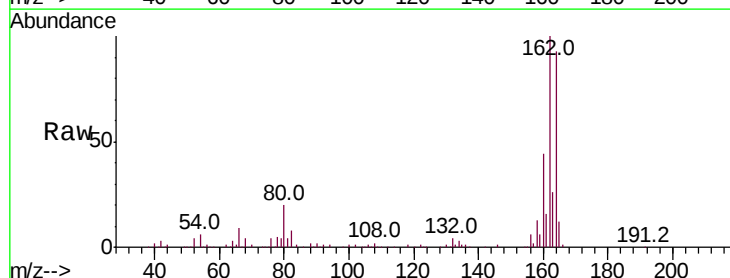



Abundance

Ion 164.00 (163.70 to 164.70): BGC

Ion 162.00 (161.70 to 162.70): BGC

Ion 160.00 (159.70 to 160.70): BGC

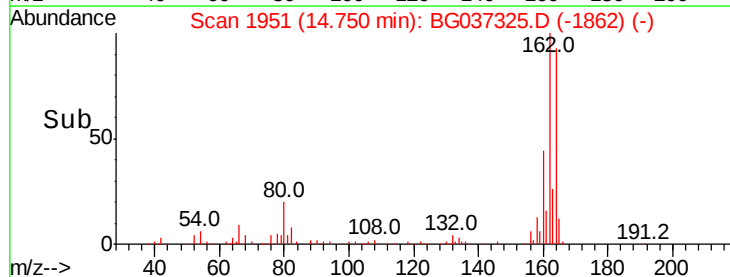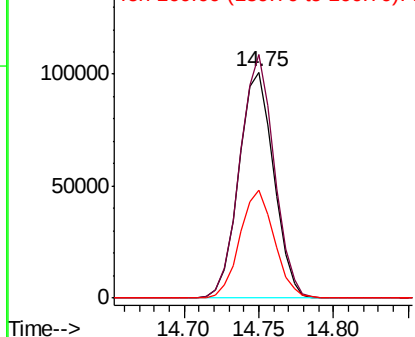

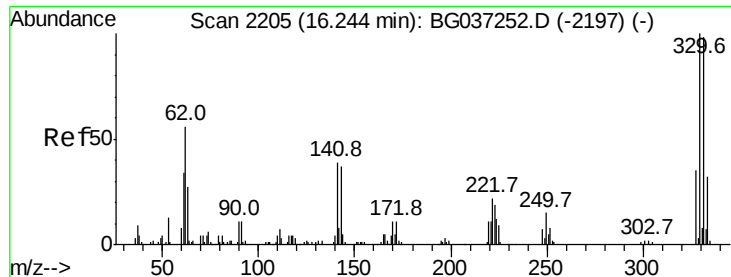

#42

2,4,6-Tribromophenol

Concen: 119.208 ng

RT: 16.24 min Scan# 2204

Delta R.T. -0.01 min

Lab File: BG037325.D

Acq: 13 Oct 2018 13:56

Instrument :

BNA_G

ClientSampleId :

100918-DBRI-F-U-S


Tot Ion:330 Resp: 191078

Ion Ratio Lower Upper




330 100

332 94.2 78.4 117.6

141 39.1 32.2 48.2

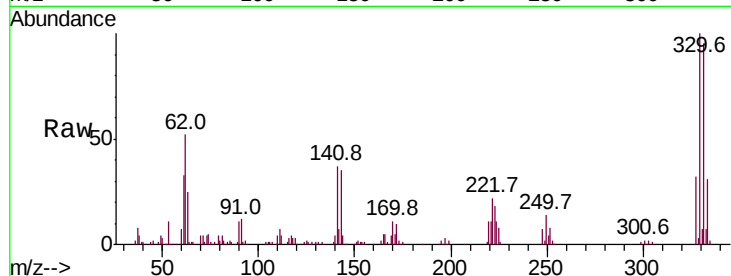

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

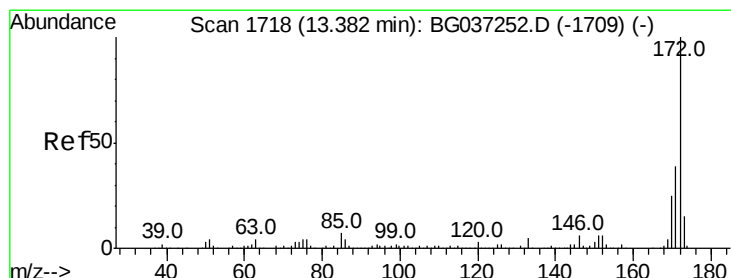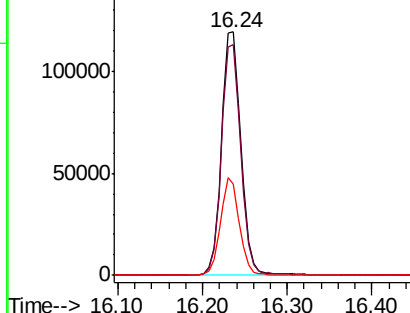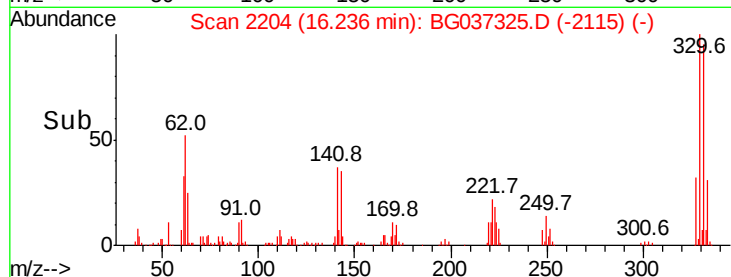

#45

2-Fluorobiphenyl

Concen: 97.518 ng

RT: 13.38 min Scan# 1717

Delta R.T. -0.01 min

Lab File: BG037325.D

Acq: 13 Oct 2018 13:56


Tgt Ion:172 Resp: 1061306

Ion Ratio Lower Upper



172 100


171 38.9 31.0 46.4

170 25.4 20.2 30.2

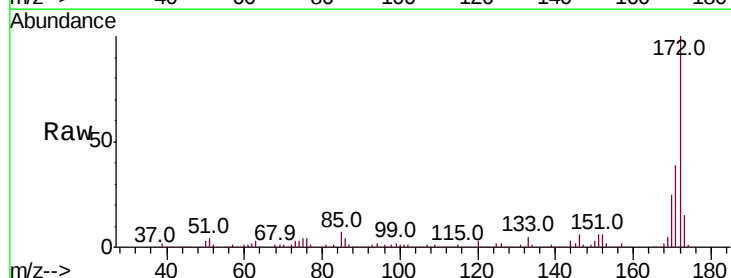

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

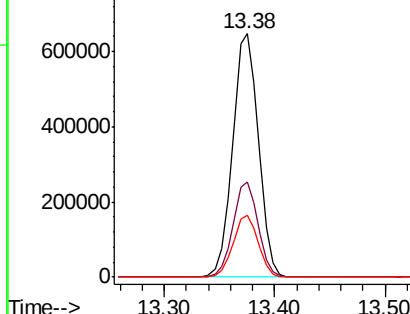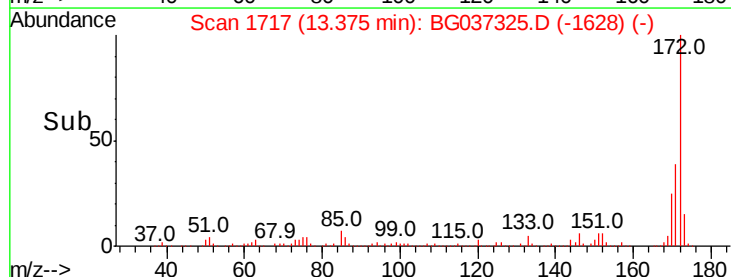

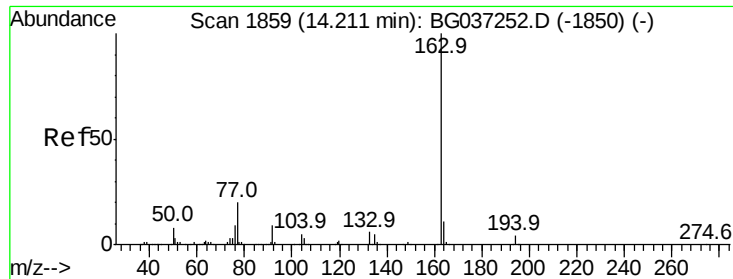

#50

Dimethylphthalate

Concen: 2.910 ng

RT: 14.19 min Scan# 1856

Delta R.T. -0.02 min

Lab File: BG037325.D

Acq: 13 Oct 2018 13:56

Instrument :

BNA_G

ClientSampleId :

100918-DBRI-F-U-S


Tot Ion:163 Resp: 37378

Ion Ratio Lower Upper

163 100

194 5.3 3.5 5.3#




164 10.3 8.5 12.7

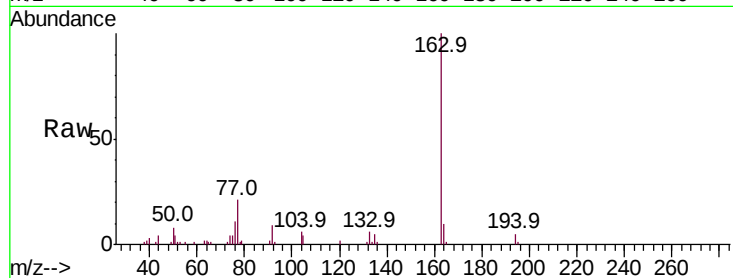

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

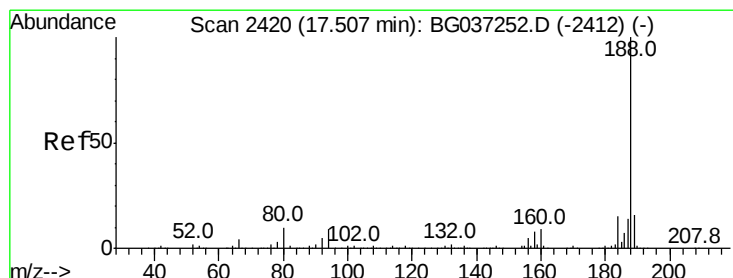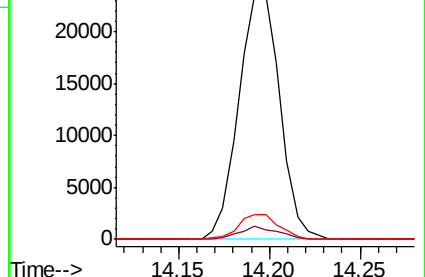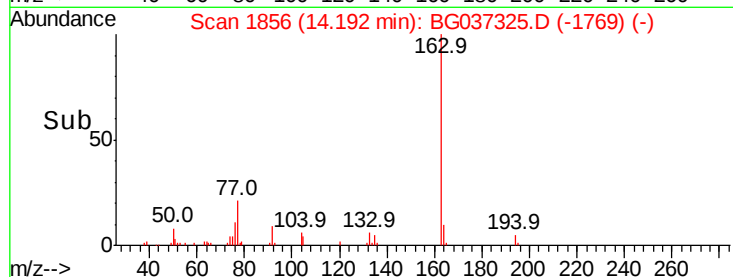

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.49 min Scan# 2418

Delta R.T. -0.01 min

Lab File: BG037325.D

Acq: 13 Oct 2018 13:56


Tgt Ion:188 Resp: 418681

Ion Ratio Lower Upper

188 100

94 8.9 7.2 10.8



80 10.3 7.7 11.5

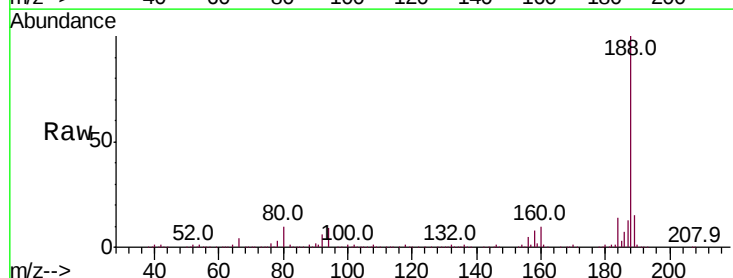


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

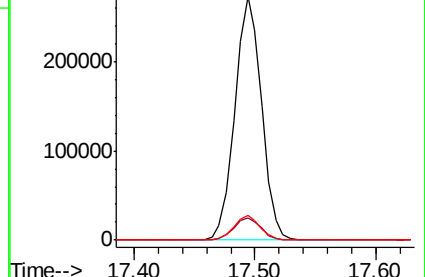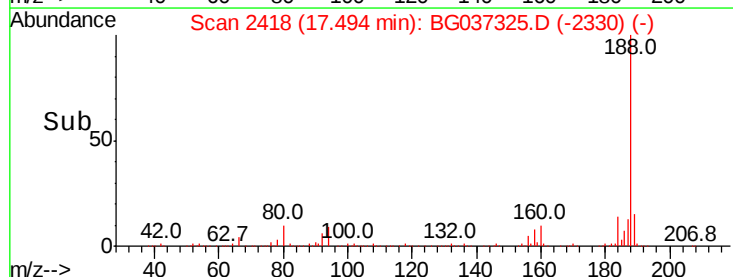

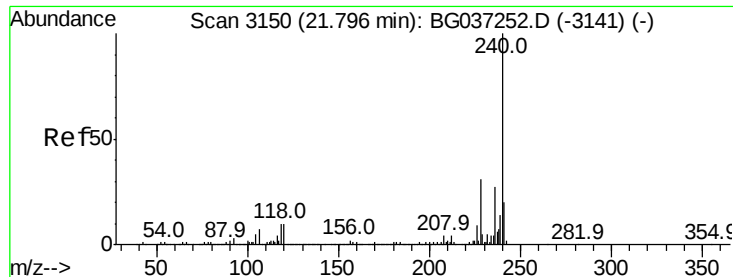

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.78 min Scan# 3147

Delta R.T. -0.02 min

Lab File: BG037325.D

Acq: 13 Oct 2018 13:56

Instrument :

BNA_G

ClientSampleId :

100918-DBRI-F-U-S


Tot Ion:240 Resp: 406576

Ion Ratio Lower Upper

240 100

120 11.4 8.1 12.1




236 25.5 21.4 32.0

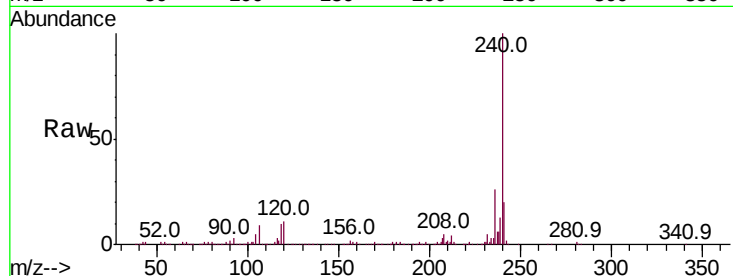

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

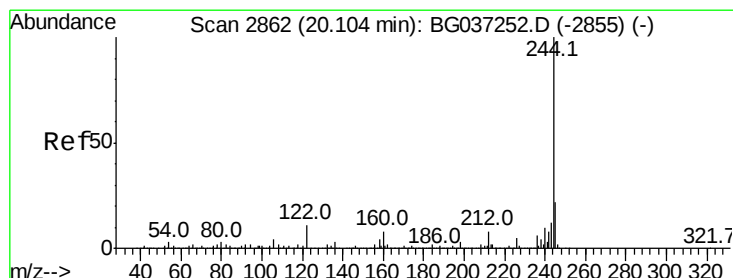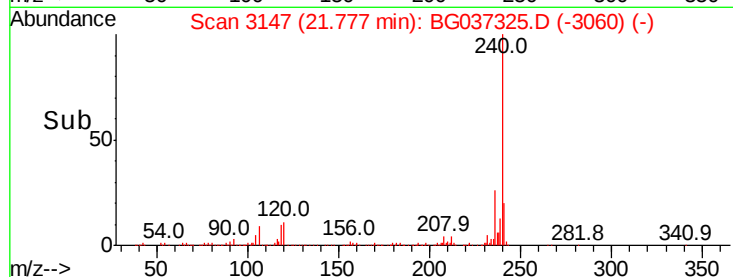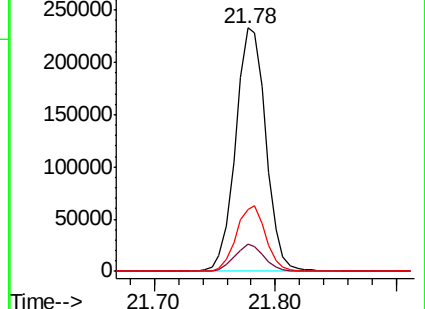

#79

Terphenyl-d14

Concen: 89.022 ng

RT: 20.10 min Scan# 2861

Delta R.T. -0.01 min

Lab File: BG037325.D

Acq: 13 Oct 2018 13:56


Tgt Ion:244 Resp: 1723745

Ion Ratio Lower Upper

244 100

212 9.1 6.5 9.7



122 12.0 9.0 13.4

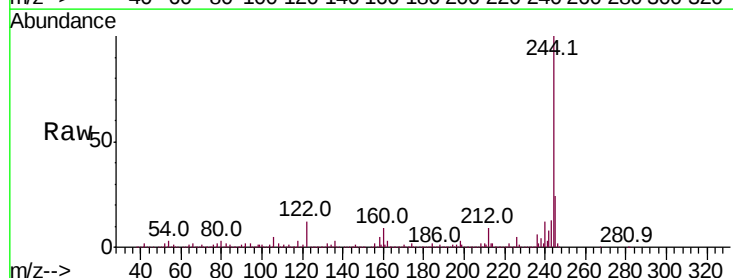


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

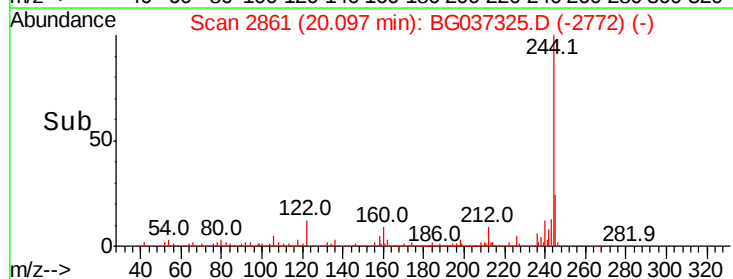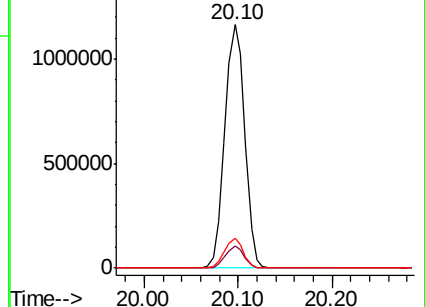

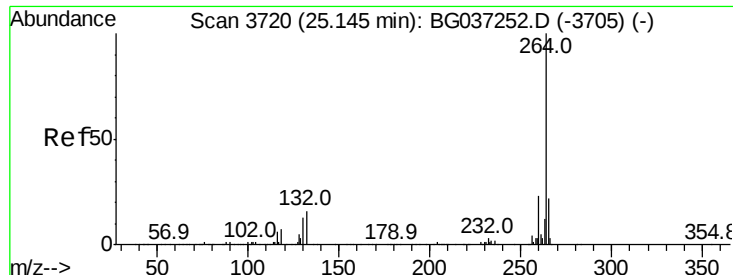

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.13 min Scan# 3717
Delta R.T. -0.02 min
Lab File: BG037325.D
Acq: 13 Oct 2018 13:56

Instrument :
BNA_G
ClientSampleId :
100918-DBRI-F-U-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.4	18.2	27.4
265	20.6	17.9	26.9

