


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101218\
 Data File : BG037291.D
 Acq On : 12 Oct 2018 15:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 11 13:59:58 2018

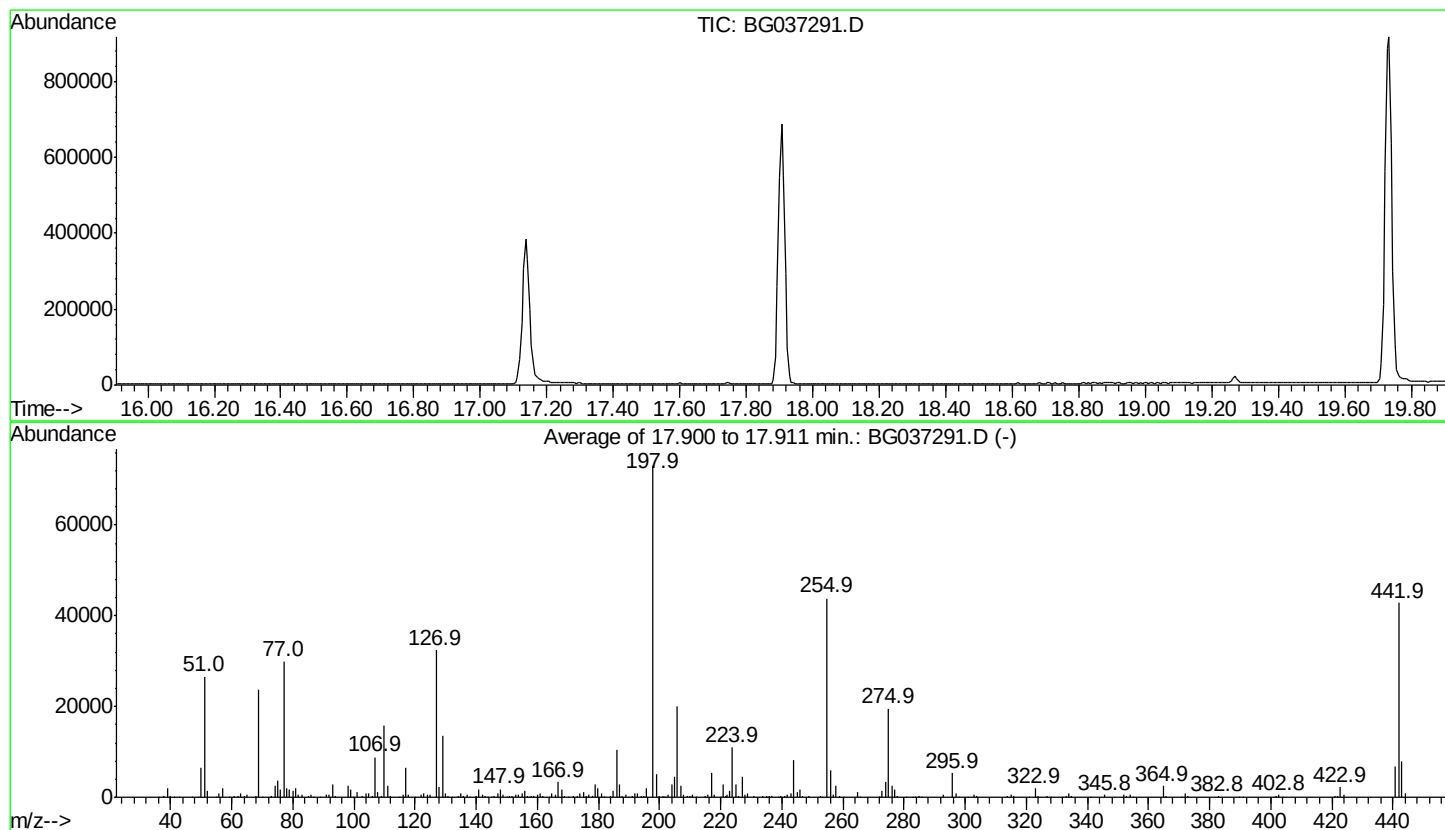

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	26532	PASS
68	69	0.00	2	1.5	344	PASS
69	198	0.00	100	32.4	23658	PASS
70	69	0.00	2	0.6	138	PASS
127	198	10	80	44.2	32333	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73112	PASS
199	198	5	9	6.8	4977	PASS
275	198	10	60	26.7	19490	PASS
365	198	1	100	3.3	2449	PASS
441	198	0.01	100	9.4	6905	PASS
442	198	50	100	58.6	42837	PASS
443	442	15	24	18.5	7908	PASS