


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101218\
 Data File : BG037310.D
 Acq On : 13 Oct 2018 4:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 11 13:59:58 2018

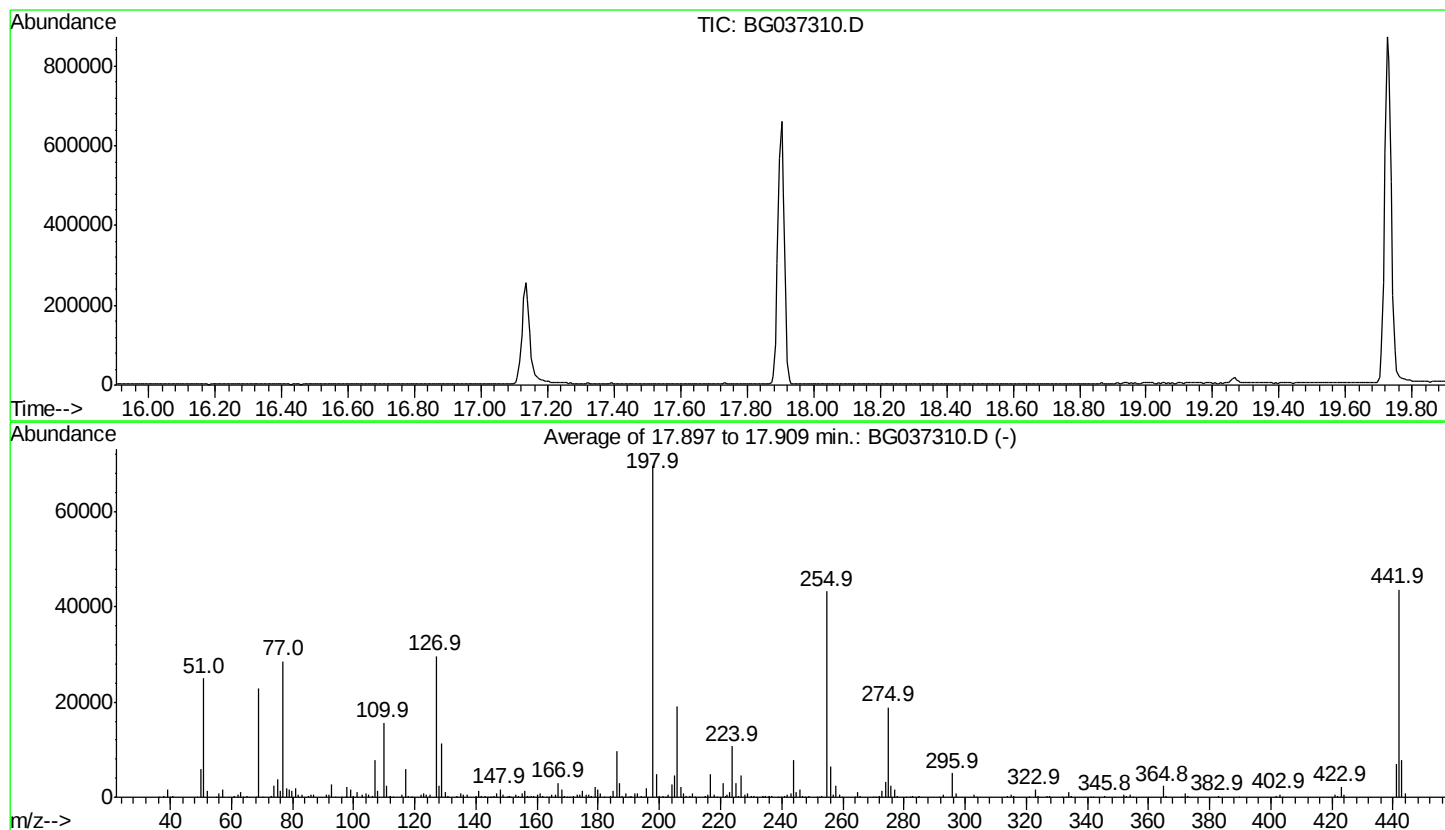

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	24941	PASS
68	69	0.00	2	0.3	68	PASS
69	198	0.00	100	33.0	23005	PASS
70	69	0.00	2	0.5	117	PASS
127	198	10	80	42.6	29685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69698	PASS
199	198	5	9	6.8	4765	PASS
275	198	10	60	27.1	18909	PASS
365	198	1	100	3.4	2389	PASS
441	198	0.01	100	10.0	7000	PASS
442	198	50	100	62.6	43664	PASS
443	442	15	24	18.1	7925	PASS