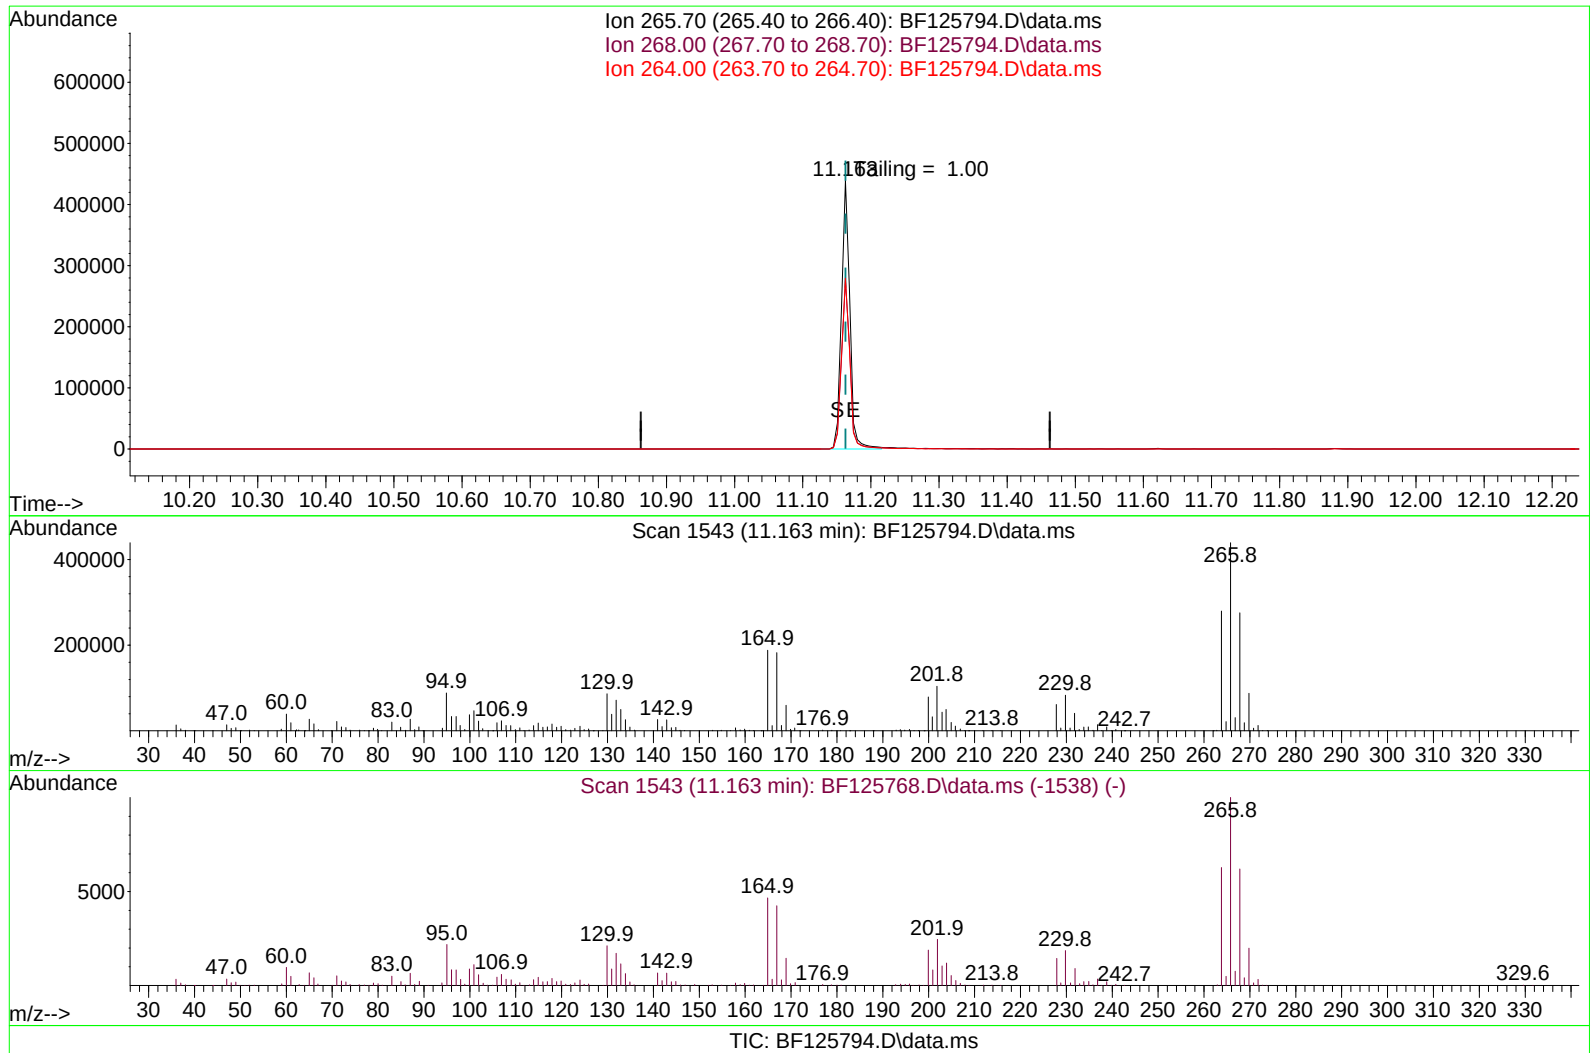


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101221\
Data File : BF125794.D
Acq On : 12 Oct 2021 10:29
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 18:13:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 17:16:23 2021
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****11.163min (0.000) 458254.10 ng****response 378157**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.79
264.00	69.90	63.65
0.00	0.00	0.00