
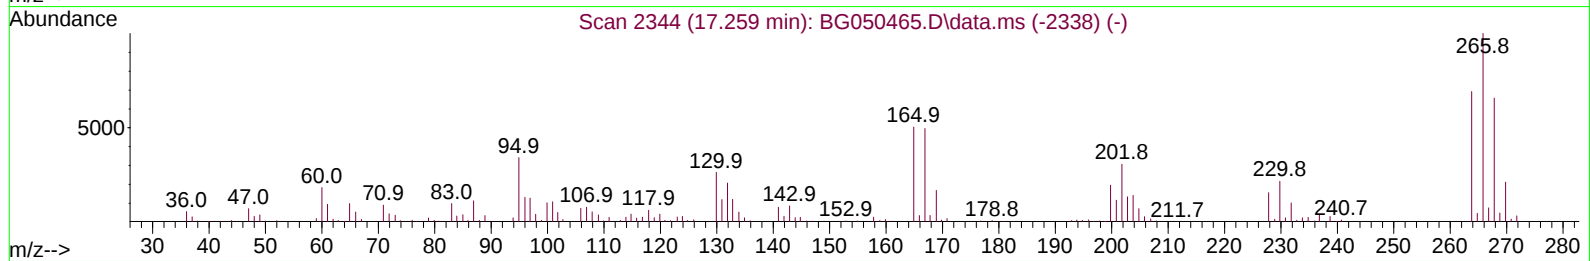
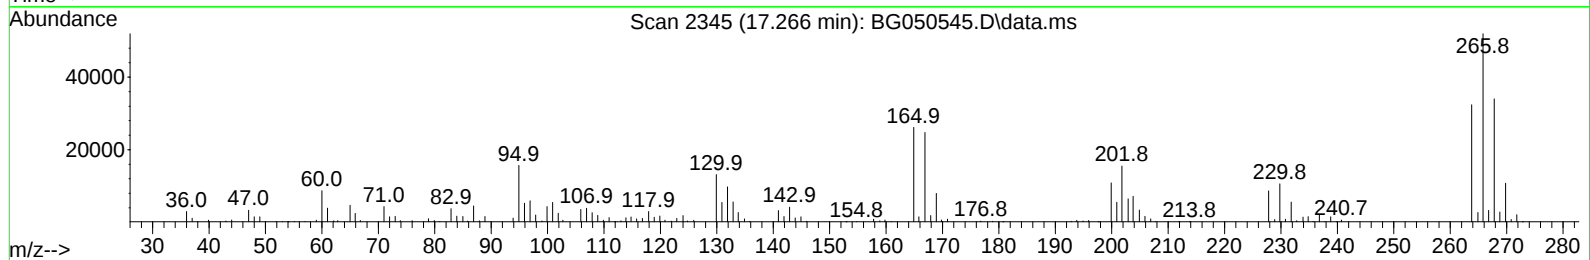


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101221\
 Data File : BG050545.D
 Acq On : 12 Oct 2021 9:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 18:20:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 06 15:51:01 2021
 Response via : Initial Calibration

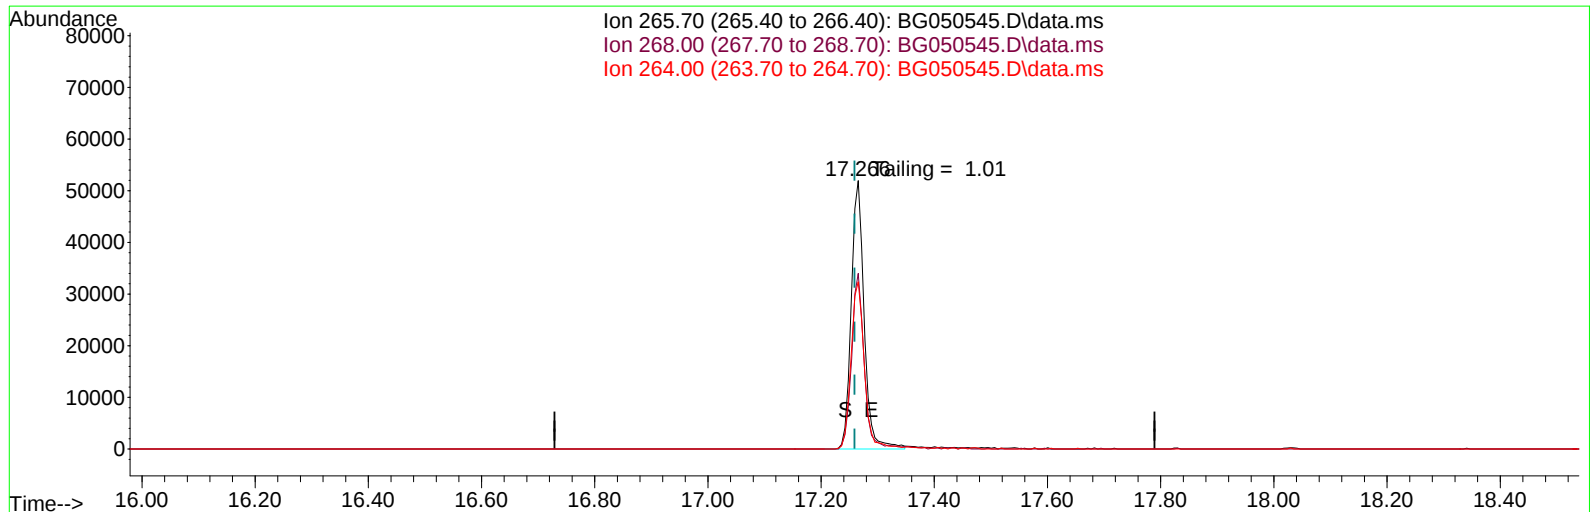

TIC: BG050545.D\data.ms

(70) Pentachlorophenol (C)

17.266min (+ 0.007) 19738.19 ng

response 83569

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.43
264.00	61.30	62.32
0.00	0.00	0.00