
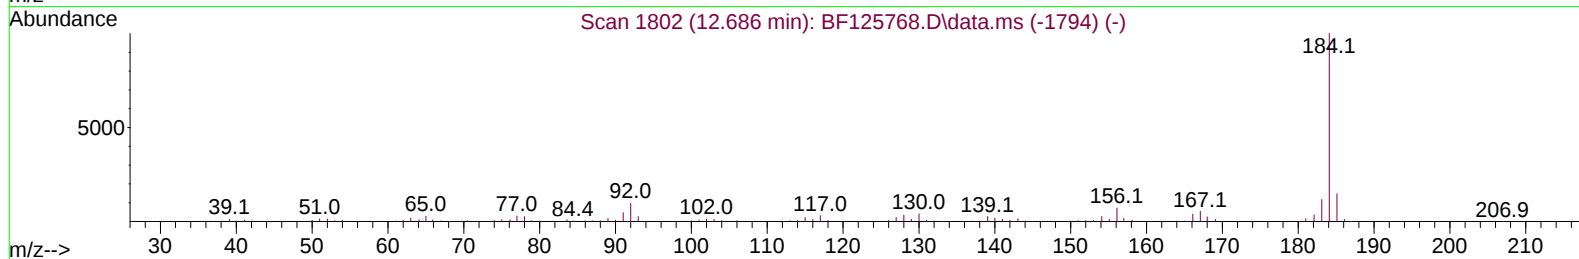
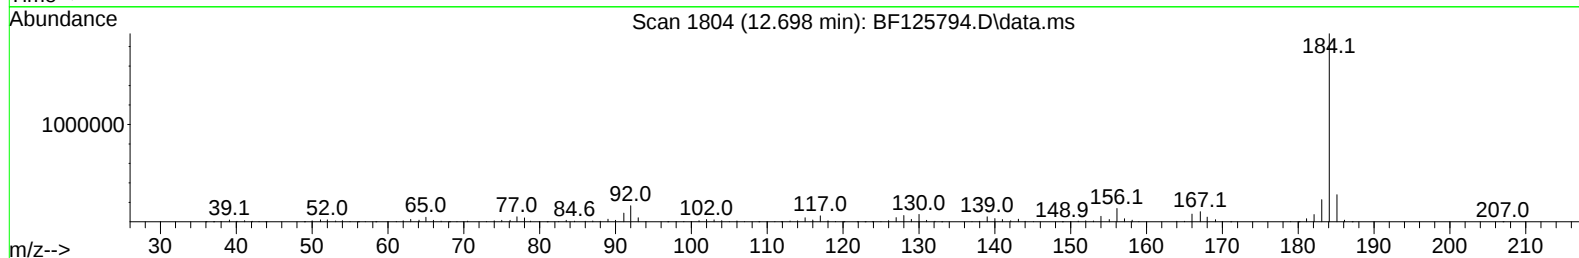


Quant Time: Oct 12 18:13:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 07 17:16:23 2021
Response via : Initial Calibration

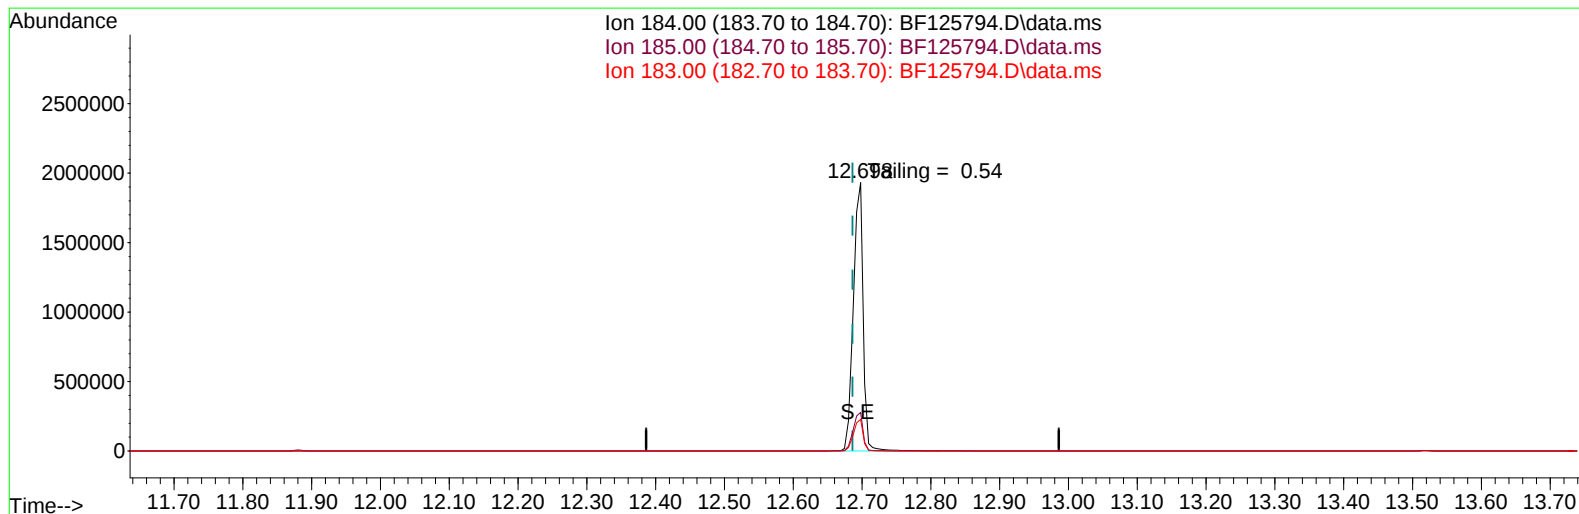

TIC: BF125794.D\data.ms

(77) Benzidine

12.698min (+ 0.012) 4896.67 ng m

response **1900688**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.38
183.00	10.10	11.80
0.00	0.00	0.00