
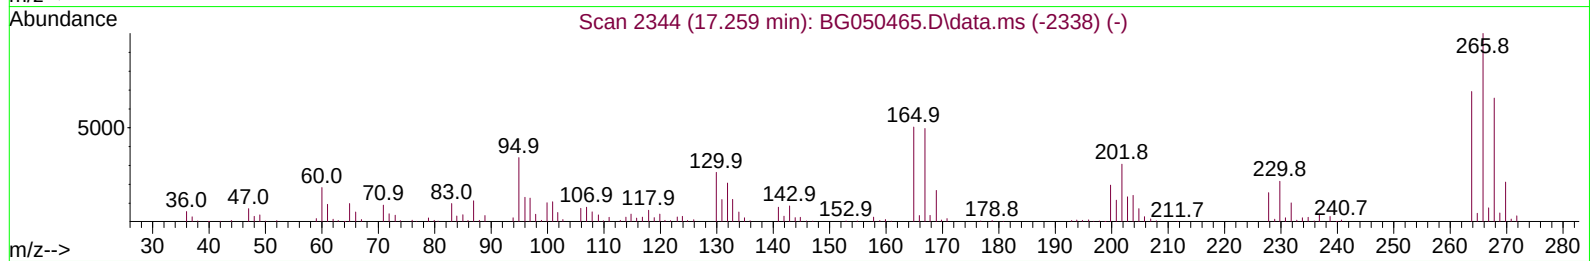
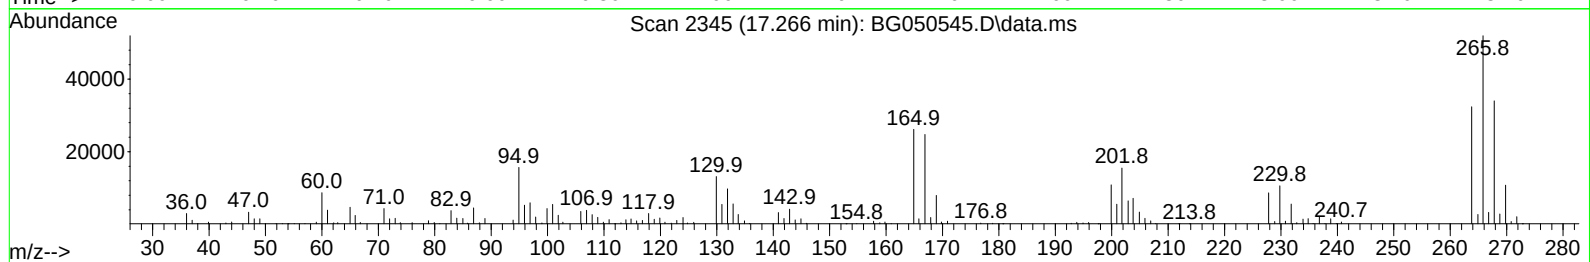


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101221\
Data File : BG050545.D
Acq On : 12 Oct 2021 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 18:20:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

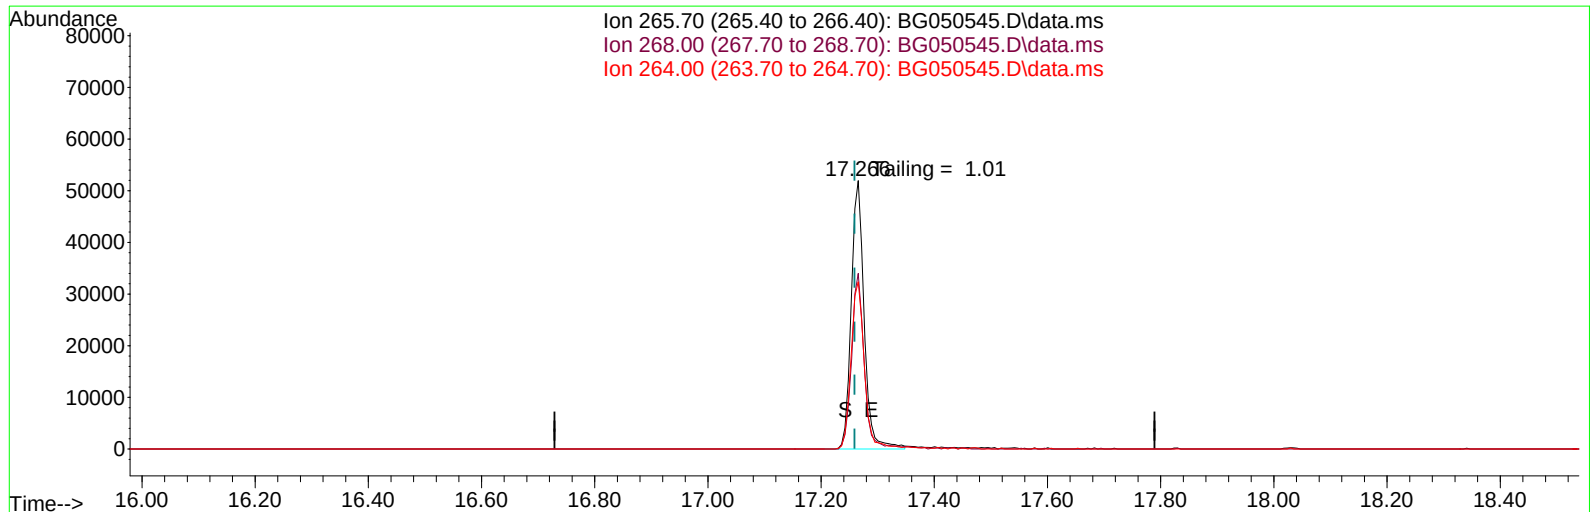

TIC: BG050545.D\data.ms

(70) Pentachlorophenol (C)




17.266min (+ 0.007) 19738.19 ng

response 83569

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.43
264.00	61.30	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101221\
Data File : BG050545.D
Acq On : 12 Oct 2021 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 18:20:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

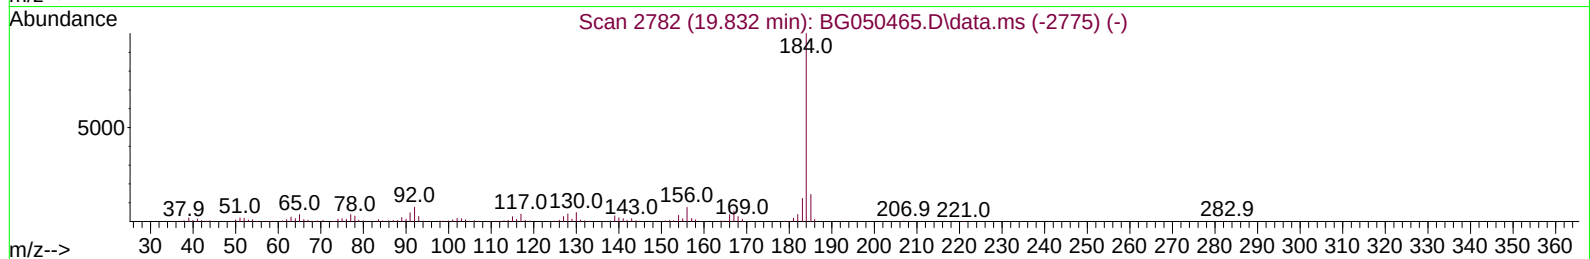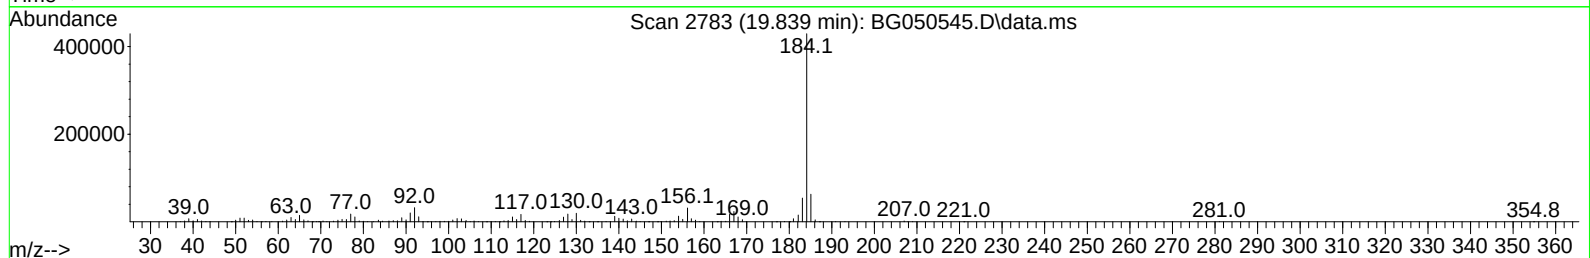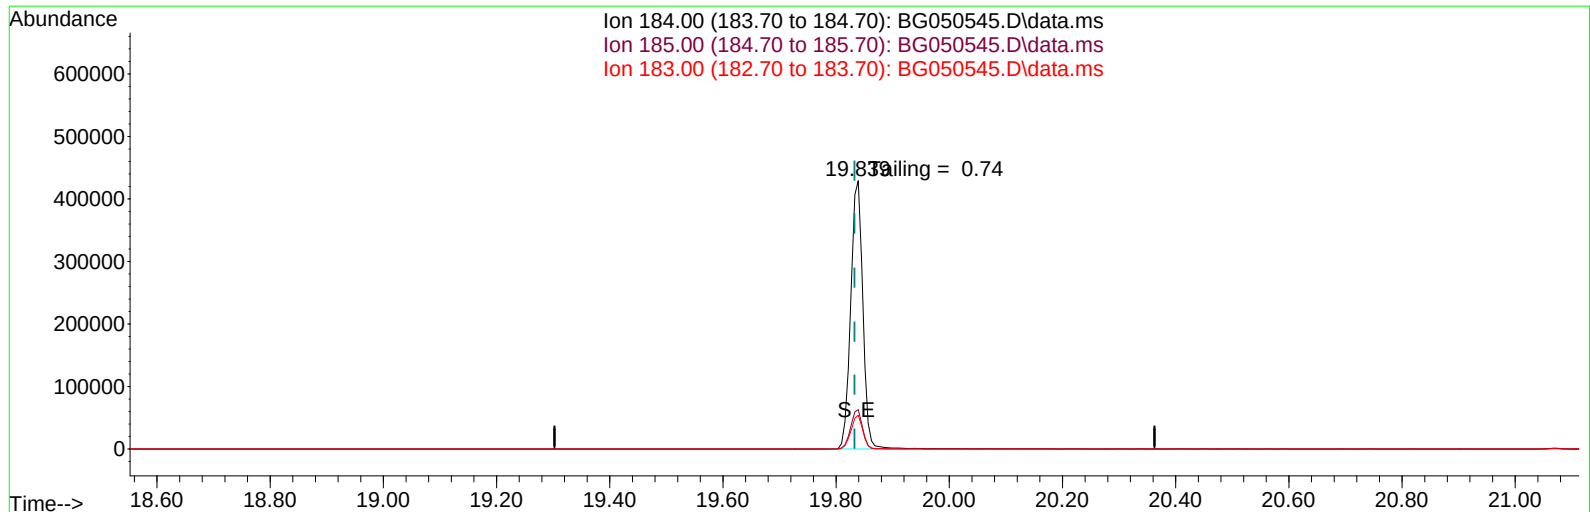

TIC: BG050545.D\data.ms

(77) Benzidine**19.839min (+ 0.007) 298071.51 ng****response 637616**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.70
183.00	11.70	12.61
0.00	0.00	0.00