


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101221\
 Data File : BG050545.D
 Acq On : 12 Oct 2021 9:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 06 15:51:01 2021

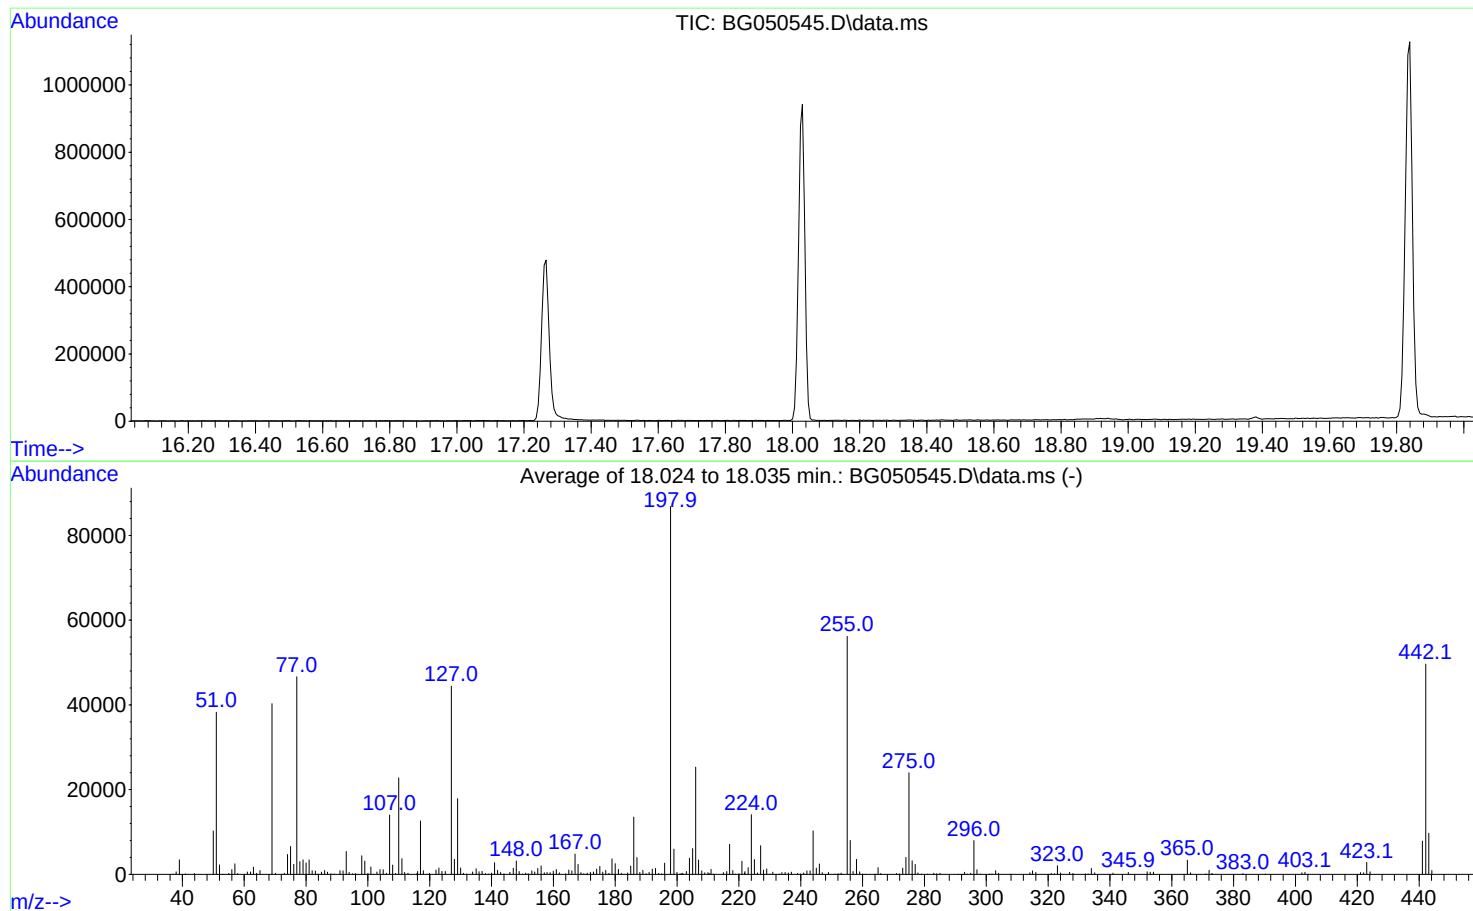




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	38256	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.4	40291	PASS
70	69	0.00	2	0.7	272	PASS
127	198	10	80	51.1	44411	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86829	PASS
199	198	5	9	6.9	5962	PASS
275	198	10	60	27.6	23989	PASS
365	198	1	100	3.9	3354	PASS
441	198	0.01	100	9.1	7875	PASS
442	442	50	100	100.0	49635	PASS
443	442	15	24	19.5	9700	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101221\
 Data File : BG050545.D
 Acq On : 12 Oct 2021 9:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 12 18:20:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 06 15:51:01 2021
 Response via : Initial Calibration

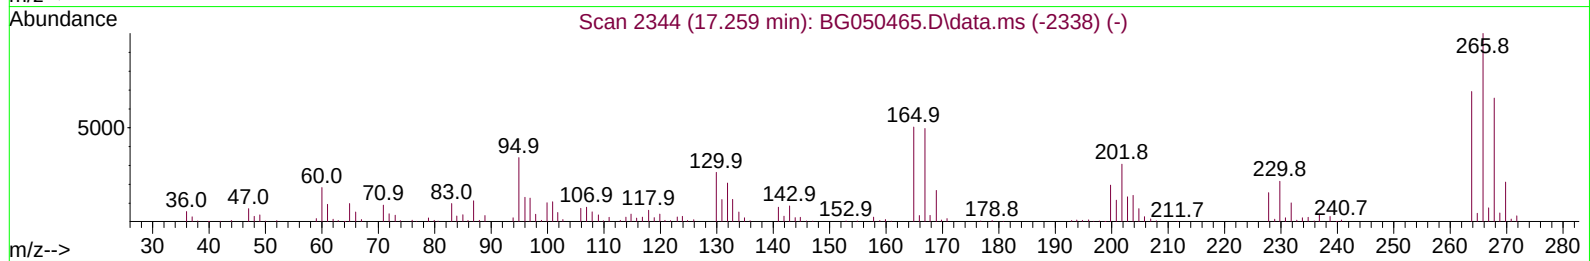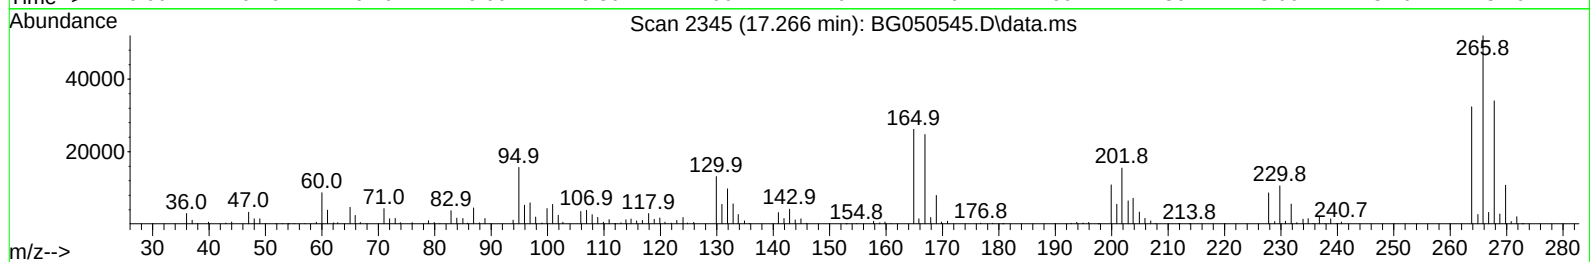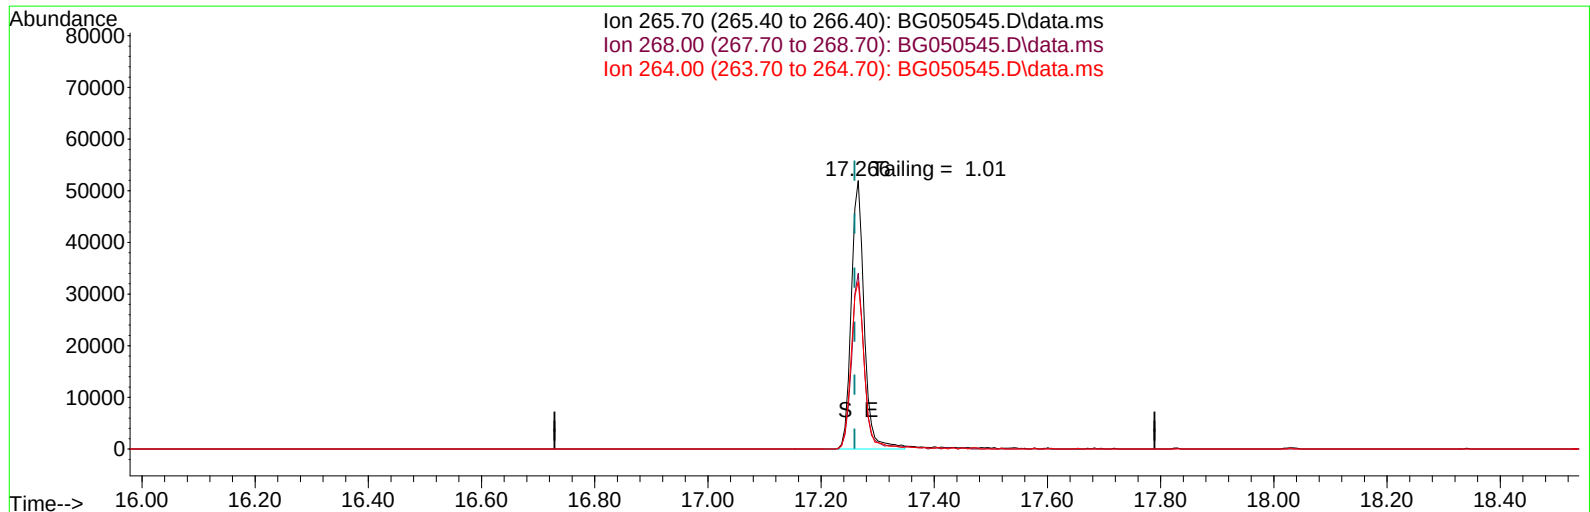

TIC: BG050545.D\data.ms

(70) Pentachlorophenol (C)

17.266min (+ 0.007) 19738.19 ng




response 83569

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.43
264.00	61.30	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101221\
Data File : BG050545.D
Acq On : 12 Oct 2021 9:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 12 18:20:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

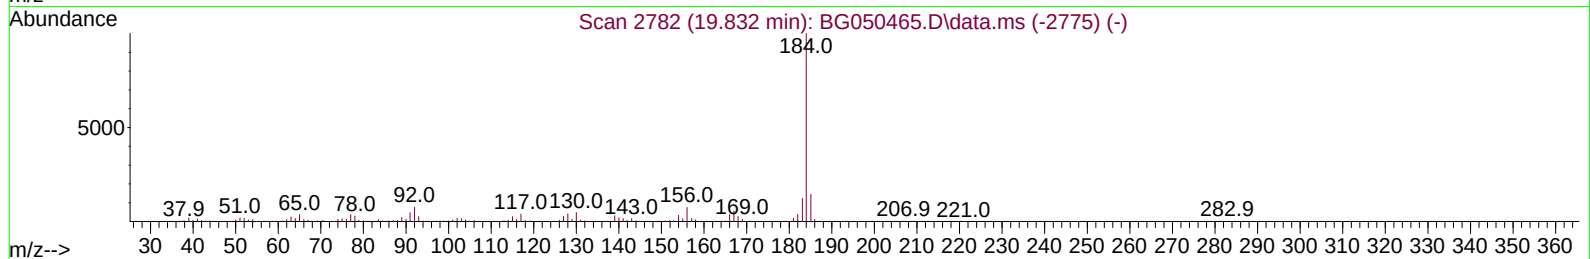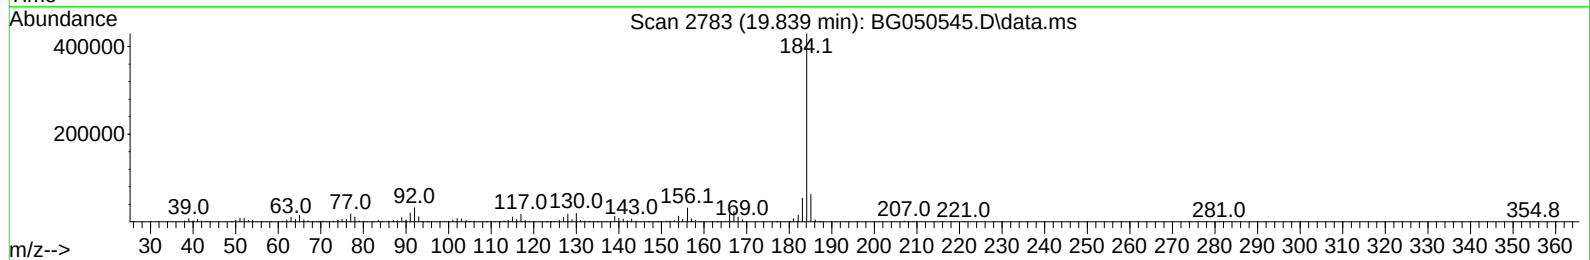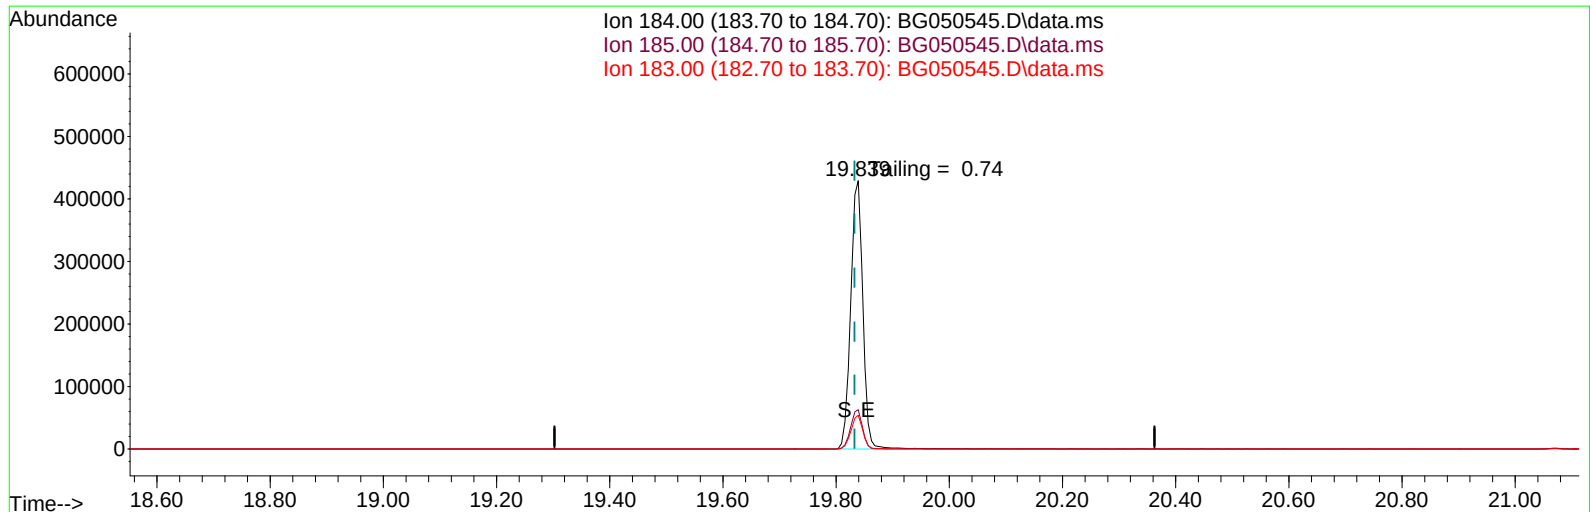

TIC: BG050545.D\data.ms

(77) Benzidine

19.839min (+ 0.007) 298071.51 ng

response 637616

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.70
183.00	11.70	12.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/12/2021	BNA_G	BG050545.D
Compound Name	Response	Retention Time
DDT	286719	21.07
DDD	991	20.62
DDE	134	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1125	287844	0.39

Instrument :
BNA_G
ClientSampleId :
DFTPP