

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
 Data File : BG059441.D
 Acq On : 13 Oct 2023 11:53
 Operator : MA/JU
 Sample : PB156220BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.508	16	20	27	rVB2	13509	20206	1.46%	0.160%
2	3.825	73	74	77	rBV3	3390	3315	0.24%	0.026%
3	3.942	89	94	108	rBV	173713	296312	21.42%	2.342%
4	4.295	152	154	156	rVB2	4129	3265	0.24%	0.026%
5	4.442	177	179	181	rVB2	3209	2691	0.19%	0.021%
6	4.659	213	216	219	rBV3	2803	4060	0.29%	0.032%
7	4.806	238	241	243	rBV	2214	2571	0.19%	0.020%
8	5.329	326	330	333	rVB3	2139	3101	0.22%	0.025%
9	5.482	354	356	358	rBV2	2534	2579	0.19%	0.020%
10	5.740	397	400	403	rVB2	2841	2773	0.20%	0.022%
11	6.645	550	554	557	rVB2	2102	2570	0.19%	0.020%
12	7.344	664	673	682	rBV	174604	306599	22.16%	2.423%
13	7.538	698	706	714	rBV	154501	253727	18.34%	2.006%
14	7.732	732	739	748	rBV	185233	305983	22.12%	2.419%
15	7.820	751	754	757	rBV	1363	2504	0.18%	0.020%
16	8.220	815	822	830	rVB	134872	229470	16.59%	1.814%
17	8.466	859	864	867	rBV	2771	4192	0.30%	0.033%
18	8.907	932	939	948	rBV	211310	373685	27.01%	2.954%
19	9.078	966	968	972	rVB	2716	2735	0.20%	0.022%
20	9.418	1016	1026	1035	rVB	169994	304127	21.98%	2.404%
21	9.741	1079	1081	1084	rBV	2297	2836	0.21%	0.022%
22	9.959	1115	1118	1120	rBV2	2236	2676	0.19%	0.021%
23	10.135	1141	1148	1157	rVV	131795	231202	16.71%	1.827%
24	10.476	1203	1206	1209	rVB	2324	3016	0.22%	0.024%
25	10.664	1231	1238	1247	rBV	195646	351727	25.43%	2.780%
26	11.058	1299	1305	1313	rVV	198067	345979	25.01%	2.735%
27	11.210	1323	1331	1341	rBV	214583	396834	28.69%	3.137%
28	12.374	1527	1529	1534	rVV	1615	2798	0.20%	0.022%
29	12.497	1547	1550	1552	rVB	2809	2790	0.20%	0.022%
30	12.620	1568	1571	1573	rBV	2716	3467	0.25%	0.027%
31	13.672	1747	1750	1753	rBV2	4676	6299	0.46%	0.050%
32	13.989	1798	1804	1806	rBV	2065	2516	0.18%	0.020%
33	14.254	1842	1849	1856	rBV	415203	596987	43.15%	4.719%
34	14.559	1894	1901	1907	rBV2	470431	715678	51.73%	5.657%
35	14.771	1934	1937	1938	rVB	3255	2708	0.20%	0.021%
36	14.859	1945	1952	1959	rVV2	292094	466686	33.74%	3.689%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
 Data File : BG059441.D
 Acq On : 13 Oct 2023 11:53
 Operator : MA/JU
 Sample : PB156220BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

37	15.047	1976	1984	1993	rBV	168163	276108	19.96%	2.182%
38	15.670	2086	2090	2093	rVB	2168	2646	0.19%	0.021%
39	15.846	2113	2120	2128	rBV	592420	883769	63.89%	6.986%
40	15.958	2131	2139	2147	rBV2	176837	274844	19.87%	2.172%
41	16.075	2158	2159	2168	rBV3	3783	5734	0.41%	0.045%
42	16.422	2216	2218	2221	rVB	2452	2728	0.20%	0.022%
43	16.616	2249	2251	2256	rBV	2035	3442	0.25%	0.027%
44	17.256	2355	2360	2362	rBV2	2012	3337	0.24%	0.026%
45	17.397	2382	2384	2387	rVV	2932	2976	0.22%	0.024%
46	17.609	2409	2420	2429	rBV	368445	581502	42.04%	4.596%
47	17.709	2429	2437	2444	rBV	658524	1020928	73.80%	8.070%
48	18.226	2522	2525	2526	rBV	2198	2643	0.19%	0.021%
49	18.396	2551	2554	2556	rBV2	2701	2777	0.20%	0.022%
50	18.890	2637	2638	2642	rBV2	3075	3829	0.28%	0.030%
51	18.948	2645	2648	2652	rVB2	3168	4350	0.31%	0.034%
52	19.007	2655	2658	2661	rVB2	2838	2673	0.19%	0.021%
53	19.066	2666	2668	2671	rVB3	3094	2741	0.20%	0.022%
54	19.195	2688	2690	2694	rBV2	2829	3879	0.28%	0.031%
55	19.542	2744	2749	2755	rBV4	10509	14307	1.03%	0.113%
56	19.612	2755	2761	2766	rVB3	9045	15084	1.09%	0.119%
57	19.753	2783	2785	2787	rBV2	3008	2849	0.21%	0.023%
58	19.830	2795	2798	2806	rBV3	6955	6991	0.51%	0.055%
59	19.900	2808	2810	2812	rBV	3230	3961	0.29%	0.031%
60	19.982	2818	2824	2832	rBV	907927	1248811	90.27%	9.871%
61	20.159	2852	2854	2857	rVB2	4464	3198	0.23%	0.025%
62	20.200	2857	2861	2862	rBV2	4005	4469	0.32%	0.035%
63	20.511	2911	2914	2915	rBV2	4306	3604	0.26%	0.028%
64	20.617	2930	2932	2934	rVB3	4548	2874	0.21%	0.023%
65	20.635	2934	2935	2937	rBV2	3587	3141	0.23%	0.025%
66	20.658	2937	2939	2940	rVB2	4164	2795	0.20%	0.022%
67	20.864	2972	2974	2976	rBV3	4820	3411	0.25%	0.027%
68	21.011	2998	2999	3001	rBV2	4068	3082	0.22%	0.024%
69	21.052	3005	3006	3009	rVV2	4070	2736	0.20%	0.022%
70	21.451	3072	3074	3076	rBV3	6443	5105	0.37%	0.040%
71	21.545	3088	3090	3091	rBV2	4223	2756	0.20%	0.022%
72	21.857	3141	3143	3144	rBV2	4222	3666	0.27%	0.029%
73	21.910	3145	3152	3160	rVV	396588	687726	49.71%	5.436%
74	22.098	3182	3184	3185	rBV	3686	2496	0.18%	0.020%
75	22.626	3272	3274	3275	rBV2	5138	3461	0.25%	0.027%
76	23.913	3492	3493	3495	rBV2	5059	3476	0.25%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
 Data File : BG059441.D
 Acq On : 13 Oct 2023 11:53
 Operator : MA/JU
 Sample : PB156220BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

77	24.236	3543	3548	3554	rBV4	16757	36178	2.62%	0.286%
78	24.330	3562	3564	3565	rBV2	5905	3143	0.23%	0.025%
79	24.583	3605	3607	3609	rVB2	4549	3238	0.23%	0.026%
80	25.018	3679	3681	3686	rBV4	5930	6800	0.49%	0.054%
81	25.147	3692	3703	3715	rBV2	469208	1383361	100.00%	10.935%
82	25.388	3734	3744	3758	rVB	256373	773459	55.91%	6.114%
83	26.786	3980	3982	3984	rBV3	5797	5417	0.39%	0.043%
84	27.362	4078	4080	4081	rBV	4674	2739	0.20%	0.022%
85	27.526	4107	4108	4110	rBV2	6853	3059	0.22%	0.024%
86	27.550	4110	4112	4114	rBV3	4685	3309	0.24%	0.026%
87	28.232	4227	4228	4230	rBV	5970	3333	0.24%	0.026%
88	28.531	4277	4279	4280	rBV2	5196	2950	0.21%	0.023%
89	28.931	4345	4347	4348	rBV2	5515	2975	0.22%	0.024%
90	29.859	4503	4505	4507	rVB2	6047	4687	0.34%	0.037%
91	29.994	4526	4528	4530	rBV3	6000	5405	0.39%	0.043%
92	30.012	4530	4531	4534	rVV3	4582	3234	0.23%	0.026%
93	30.100	4544	4546	4547	rVB2	5186	3115	0.23%	0.025%
94	30.118	4547	4549	4552	rVB4	5449	4798	0.35%	0.038%
95	30.411	4597	4599	4600	rBV2	4134	3003	0.22%	0.024%
96	30.541	4620	4621	4623	rVB2	6102	3083	0.22%	0.024%
97	31.152	4723	4725	4727	rBV2	6113	5089	0.37%	0.040%
98	31.222	4735	4737	4742	rBV4	3959	6078	0.44%	0.048%
99	31.657	4810	4811	4813	rBV2	3769	3240	0.23%	0.026%
100	31.751	4823	4827	4829	rBV5	6016	8017	0.58%	0.063%




Sum of corrected areas: 12651279

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
Data File : BG059441.D
Acq On : 13 Oct 2023 11:53
Operator : MA/JU
Sample : PB156220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

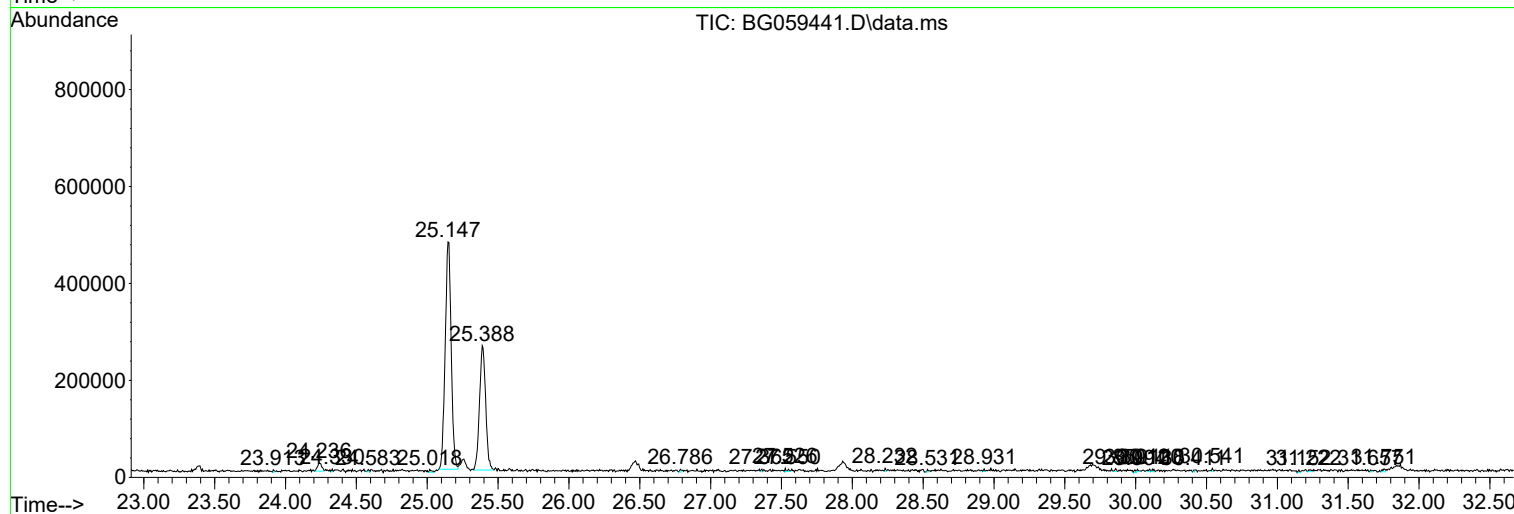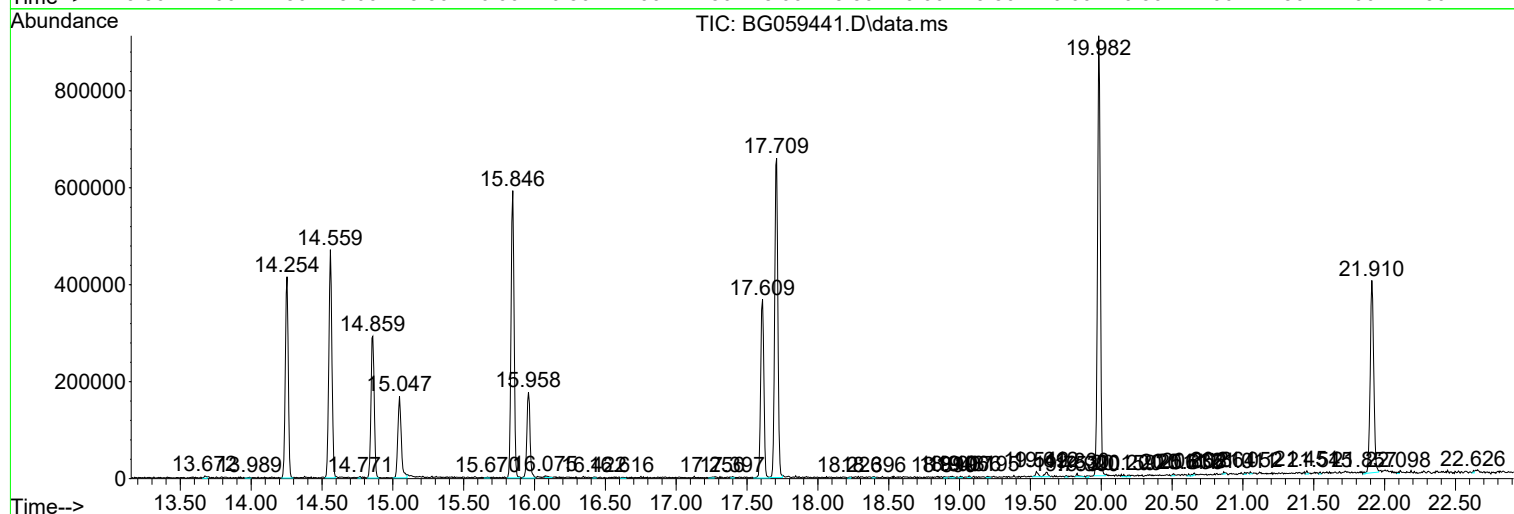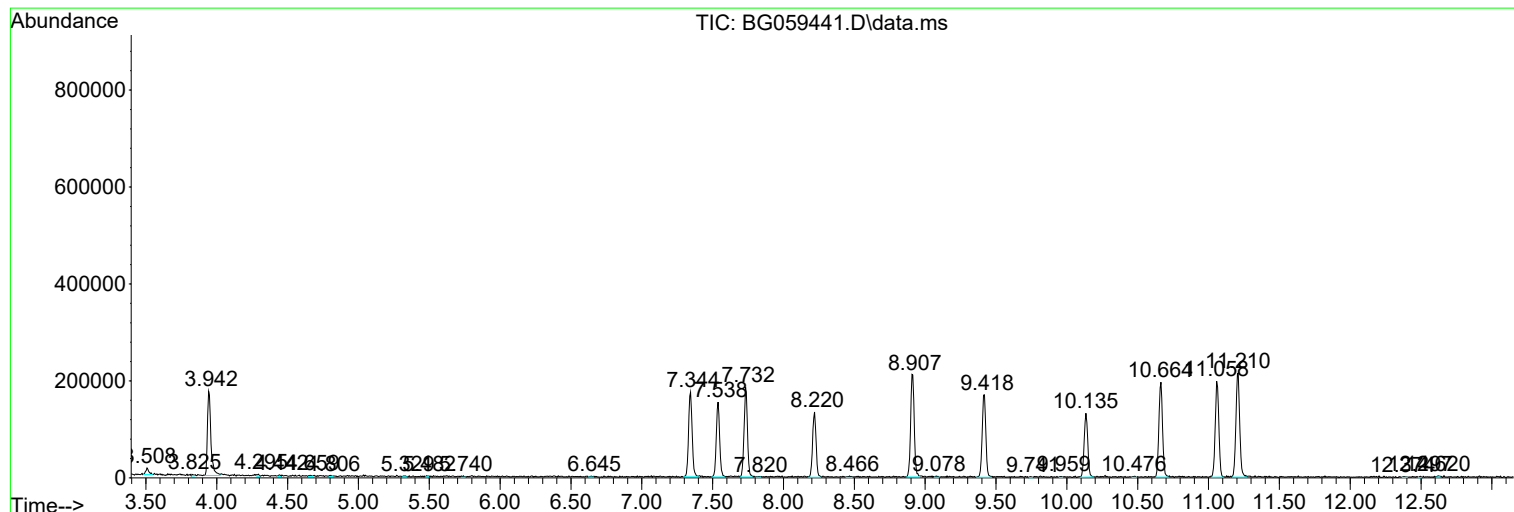

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
Data File : BG059441.D
Acq On : 13 Oct 2023 11:53
Operator : MA/JU
Sample : PB156220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
Data File : BG059441.D
Acq On : 13 Oct 2023 11:53
Operator : MA/JU
Sample : PB156220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------