

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
 Data File : BG059445.D
 Acq On : 13 Oct 2023 16:36
 Operator : MA/JU
 Sample : PB156222BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.511	18	21	27	rVB3	17325	23737	1.80%	0.184%
2	3.946	90	95	104	rBV	180391	300393	22.78%	2.330%
3	4.204	137	139	144	rVB3	3356	3094	0.23%	0.024%
4	4.251	144	147	149	rVV3	3800	3497	0.27%	0.027%
5	4.281	149	152	157	rVB4	5875	9623	0.73%	0.075%
6	5.168	301	303	306	rBV3	2807	2793	0.21%	0.022%
7	5.332	328	331	332	rBV2	3302	3147	0.24%	0.024%
8	5.973	438	440	443	rBV2	2529	3183	0.24%	0.025%
9	7.342	665	673	686	rBV	192062	330938	25.10%	2.567%
10	7.536	699	706	714	rBV	151546	249821	18.95%	1.938%
11	7.735	733	740	747	rVB2	170992	292458	22.18%	2.269%
12	7.923	767	772	775	rVB	2440	3813	0.29%	0.030%
13	8.217	813	822	830	rBV	154388	257554	19.53%	1.998%
14	8.910	933	940	950	rBV	210630	373831	28.35%	2.900%
15	9.040	958	962	965	rVB3	2608	2959	0.22%	0.023%
16	9.416	1019	1026	1034	rVB	171880	299096	22.68%	2.320%
17	9.522	1041	1044	1047	rVB	2408	2777	0.21%	0.022%
18	10.133	1141	1148	1157	rVB2	129726	241410	18.31%	1.873%
19	10.321	1178	1180	1185	rBV	2151	2751	0.21%	0.021%
20	10.661	1231	1238	1246	rBV	195697	350977	26.62%	2.723%
21	10.914	1275	1281	1283	rBV	2273	4053	0.31%	0.031%
22	11.061	1297	1306	1318	rVB	209062	381290	28.92%	2.958%
23	11.202	1322	1330	1338	rBV	219014	401079	30.42%	3.111%
24	11.343	1351	1354	1358	rVB	2884	3215	0.24%	0.025%
25	11.784	1427	1429	1433	rVB	2806	2806	0.21%	0.022%
26	11.819	1433	1435	1438	rBV	3608	3838	0.29%	0.030%
27	12.448	1538	1542	1544	rVV	1934	2784	0.21%	0.022%
28	12.536	1552	1557	1559	rVB	2279	2934	0.22%	0.023%
29	12.624	1568	1572	1576	rVB2	4585	6584	0.50%	0.051%
30	12.800	1599	1602	1604	rVB2	2082	2744	0.21%	0.021%
31	12.818	1604	1605	1609	rBV	3320	2938	0.22%	0.023%
32	13.270	1677	1682	1684	rVV	2955	3663	0.28%	0.028%
33	13.681	1748	1752	1757	rVB3	3666	6264	0.48%	0.049%
34	14.251	1842	1849	1857	rBV	391026	582665	44.19%	4.520%
35	14.433	1875	1880	1882	rBV2	2514	3688	0.28%	0.029%
36	14.557	1894	1901	1914	rVB	454317	702276	53.26%	5.448%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
 Data File : BG059445.D
 Acq On : 13 Oct 2023 16:36
 Operator : MA/JU
 Sample : PB156222BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

37	14.786	1938	1940	1945	rBV	1971	3431	0.26%	0.027%
38	14.856	1945	1952	1960	rVB	328824	511288	38.78%	3.966%
39	15.044	1978	1984	1992	rBV	159614	262638	19.92%	2.037%
40	15.191	2006	2009	2011	rVV3	3010	3418	0.26%	0.027%
41	15.215	2011	2013	2016	rVB2	4014	3373	0.26%	0.026%
42	15.315	2027	2030	2033	rVB	3094	3298	0.25%	0.026%
43	15.544	2062	2069	2072	rBV	2231	4286	0.33%	0.033%
44	15.844	2113	2120	2126	rBV	586370	867346	65.78%	6.728%
45	15.955	2133	2139	2148	rVB	182925	264601	20.07%	2.052%
46	16.084	2158	2161	2163	rVB	3548	3871	0.29%	0.030%
47	16.596	2245	2248	2251	rVB	2686	3336	0.25%	0.026%
48	16.643	2251	2256	2257	rBV	1953	3047	0.23%	0.024%
49	16.737	2270	2272	2275	rBV	2595	3147	0.24%	0.024%
50	16.907	2298	2301	2302	rBV	2370	2791	0.21%	0.022%
51	17.213	2349	2353	2355	rBV	3355	3442	0.26%	0.027%
52	17.606	2414	2420	2426	rVV	438944	655301	49.70%	5.083%
53	17.706	2430	2437	2444	rVV2	644697	988368	74.96%	7.667%
54	17.806	2452	2454	2459	rBV3	3077	4541	0.34%	0.035%
55	17.947	2475	2478	2481	rBV	2521	2971	0.23%	0.023%
56	18.170	2514	2516	2519	rVB	3558	2760	0.21%	0.021%
57	18.546	2577	2580	2583	rBV	2319	3360	0.25%	0.026%
58	18.740	2611	2613	2617	rVB2	2377	3122	0.24%	0.024%
59	19.193	2688	2690	2694	rVB	3162	3182	0.24%	0.025%
60	19.457	2733	2735	2739	rBV3	2621	3007	0.23%	0.023%
61	19.545	2745	2750	2754	rVV3	9922	13349	1.01%	0.104%
62	19.586	2754	2757	2758	rVV2	3495	3434	0.26%	0.027%
63	19.610	2758	2761	2766	rVV4	8210	14295	1.08%	0.111%
64	19.657	2768	2769	2772	rVB	3843	2867	0.22%	0.022%
65	19.827	2795	2798	2802	rVV5	5919	8659	0.66%	0.067%
66	19.892	2805	2809	2810	rBV2	2297	2757	0.21%	0.021%
67	19.980	2817	2824	2835	rBV	860496	1227455	93.09%	9.521%
68	20.227	2863	2866	2867	rBV2	2324	2991	0.23%	0.023%
69	20.550	2917	2921	2924	rVB5	3713	6130	0.46%	0.048%
70	21.008	2997	2999	3000	rBV2	5775	3658	0.28%	0.028%
71	21.272	3043	3044	3049	rBV4	3348	4929	0.37%	0.038%
72	21.431	3069	3071	3072	rBV2	4497	2762	0.21%	0.021%
73	21.531	3086	3088	3090	rBV3	3718	4419	0.34%	0.034%
74	21.907	3145	3152	3163	rBV	486190	804222	60.99%	6.238%
75	22.618	3271	3273	3275	rBV3	4897	4233	0.32%	0.033%
76	23.358	3394	3399	3400	rBV4	4231	6067	0.46%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
 Data File : BG059445.D
 Acq On : 13 Oct 2023 16:36
 Operator : MA/JU
 Sample : PB156222BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

77	24.234	3546	3548	3554	rVB6	11888	15255	1.16%	0.118%
78	25.144	3692	3703	3714	rBV2	441591	1318544	100.00%	10.228%
79	25.385	3734	3744	3755	rVB3	300056	870412	66.01%	6.752%
80	26.214	3883	3885	3886	rBV2	6638	4190	0.32%	0.033%
81	26.337	3905	3906	3909	rBV3	4133	2900	0.22%	0.022%
82	26.443	3920	3924	3925	rBV3	9263	11005	0.83%	0.085%
83	26.649	3957	3959	3960	rBV2	6079	3148	0.24%	0.024%
84	27.124	4038	4040	4042	rBV3	3656	3979	0.30%	0.031%
85	27.254	4060	4062	4066	rVB3	5985	6759	0.51%	0.052%
86	27.307	4069	4071	4074	rVV4	4092	3206	0.24%	0.025%
87	27.412	4087	4089	4092	rBV3	5465	7234	0.55%	0.056%
88	27.518	4105	4107	4108	rBV2	3500	2775	0.21%	0.022%
89	27.824	4158	4159	4162	rBV3	5371	6078	0.46%	0.047%
90	28.535	4278	4280	4283	rBV3	4375	3694	0.28%	0.029%
91	29.263	4403	4404	4407	rBV3	4298	3766	0.29%	0.029%
92	29.627	4464	4466	4467	rBV2	4676	3826	0.29%	0.030%
93	30.826	4668	4670	4673	rVB4	4421	3605	0.27%	0.028%
94	30.873	4677	4678	4682	rBV3	4512	4203	0.32%	0.033%
95	30.985	4695	4697	4698	rVB2	5345	2907	0.22%	0.023%
96	31.337	4755	4757	4760	rBV4	6471	7048	0.53%	0.055%
97	32.007	4869	4871	4874	rBV3	4942	3483	0.26%	0.027%
98	32.289	4917	4919	4920	rBV2	5181	4636	0.35%	0.036%
99	32.401	4936	4938	4939	rBV2	6542	3243	0.25%	0.025%
100	32.636	4976	4978	4979	rVB2	5283	2928	0.22%	0.023%




Sum of corrected areas: 12891649

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
Data File : BG059445.D
Acq On : 13 Oct 2023 16:36
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

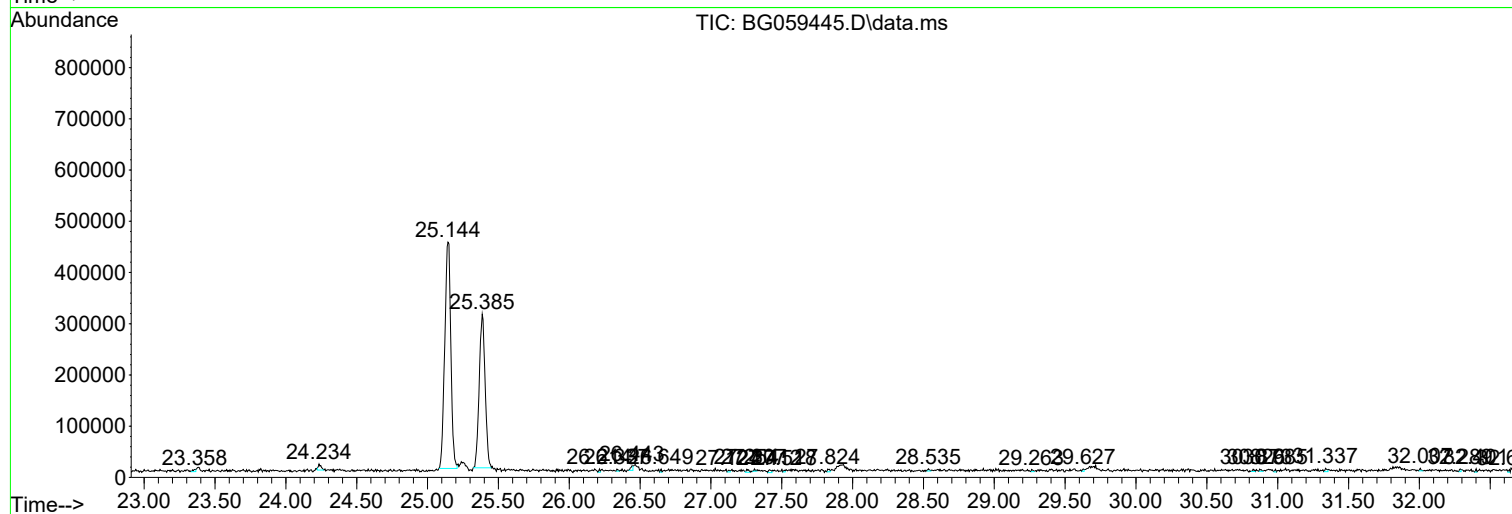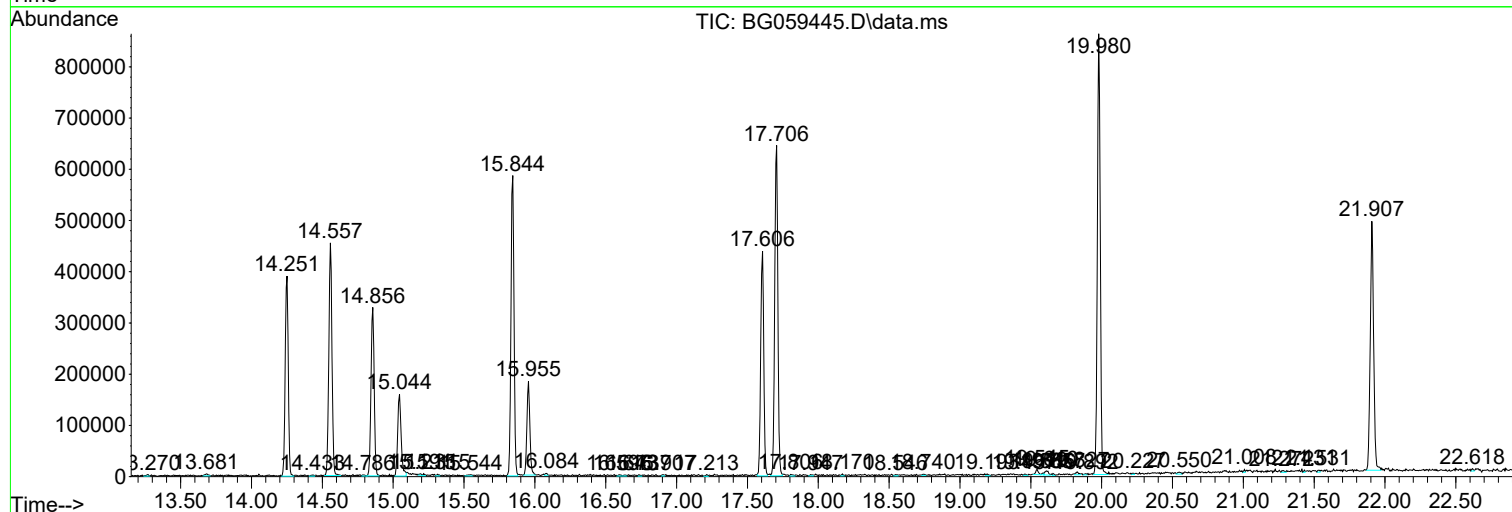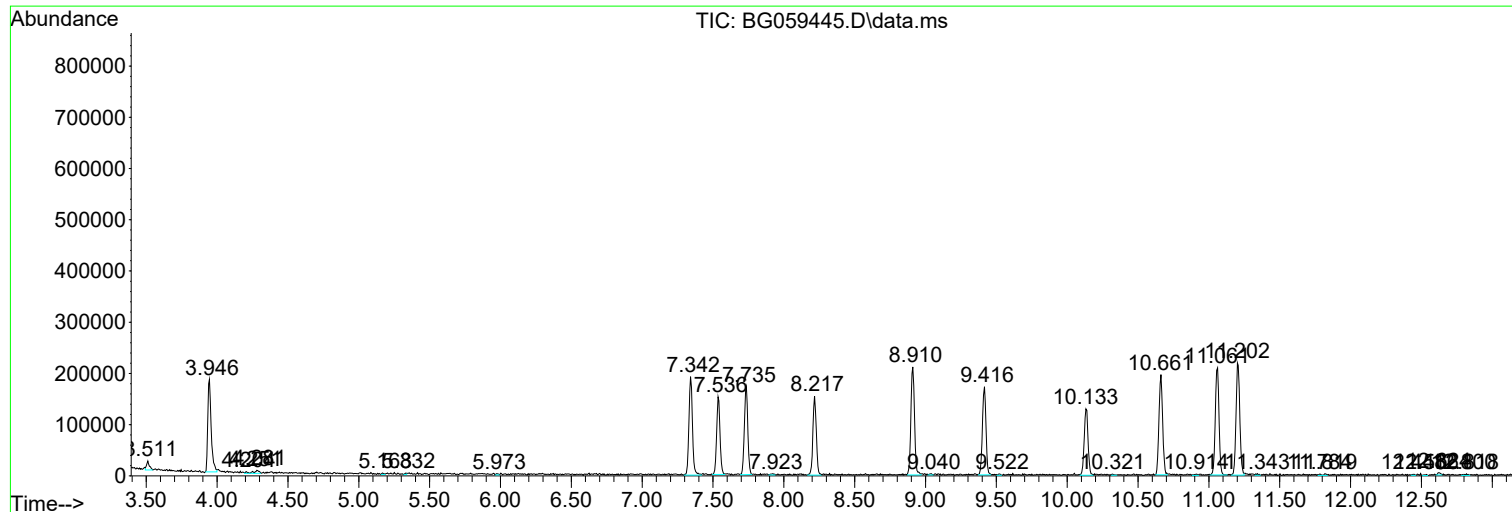

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
Data File : BG059445.D
Acq On : 13 Oct 2023 16:36
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101323\
Data File : BG059445.D
Acq On : 13 Oct 2023 16:36
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------