
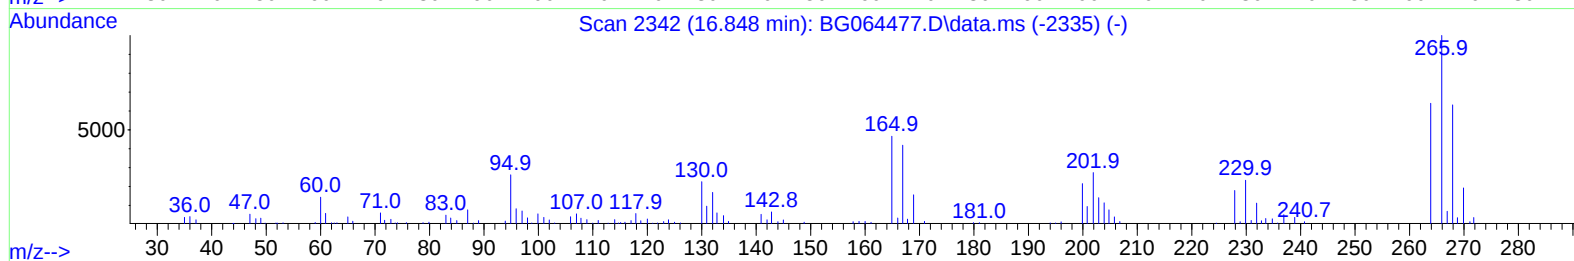
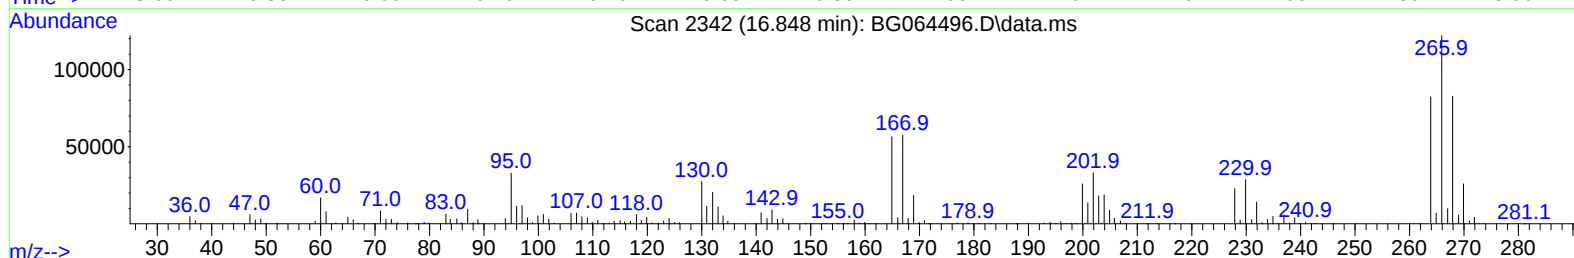


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101425\
Data File : BG064496.D
Acq On : 14 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 11:46:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

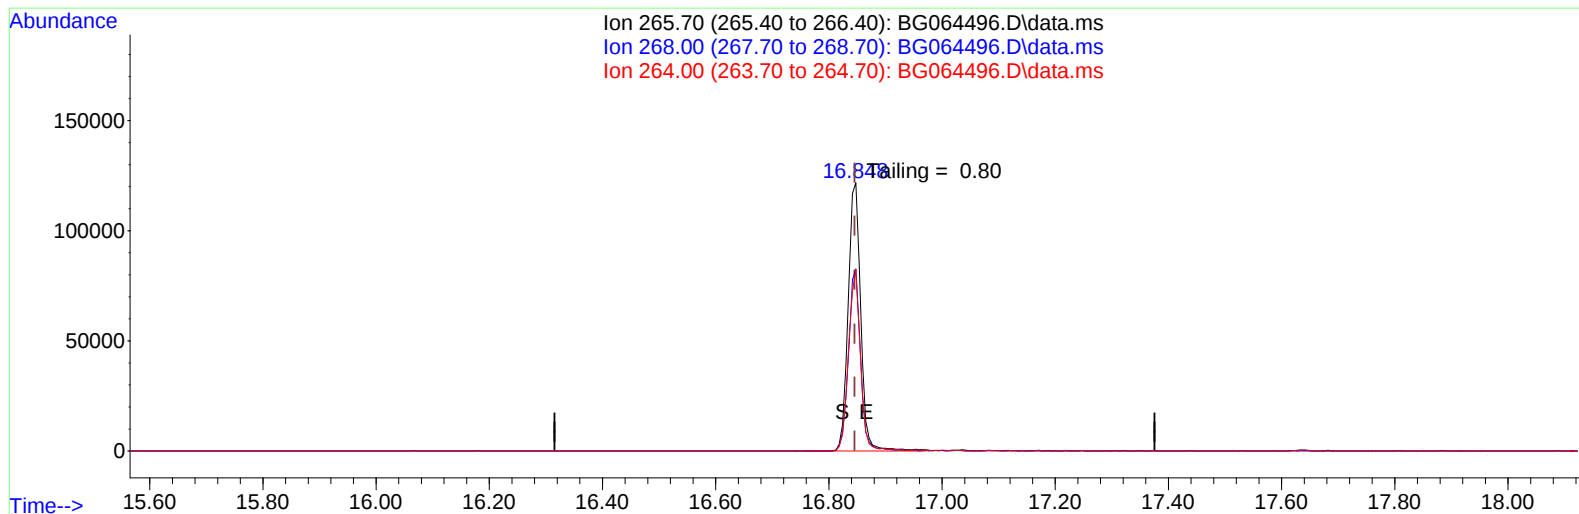

TIC: BG064496.D\data.ms

(70) Pentachlorophenol (C)




16.848min (+ 0.002) 22066.93 ng

response 187984

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	67.84
264.00	64.00	67.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101425\
Data File : BG064496.D
Acq On : 14 Oct 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 11:46:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

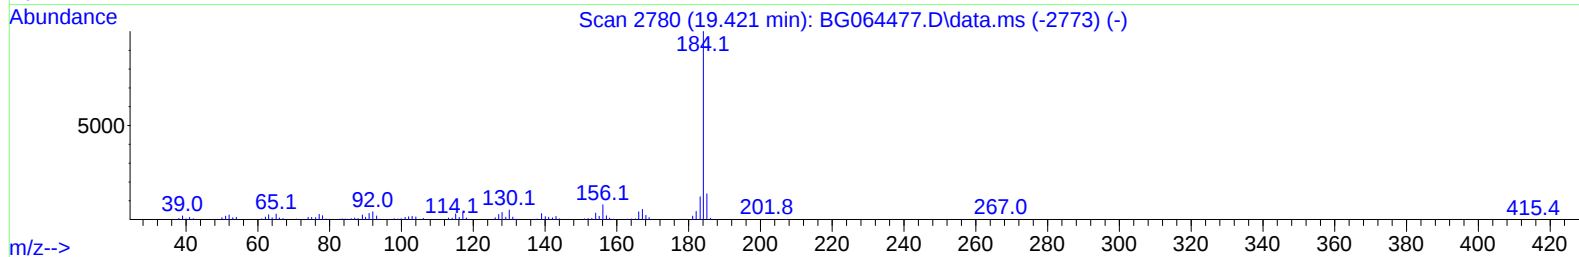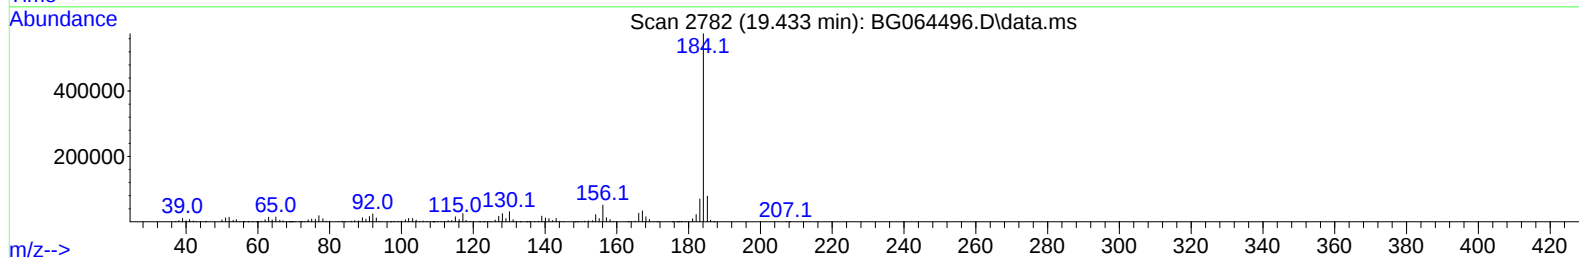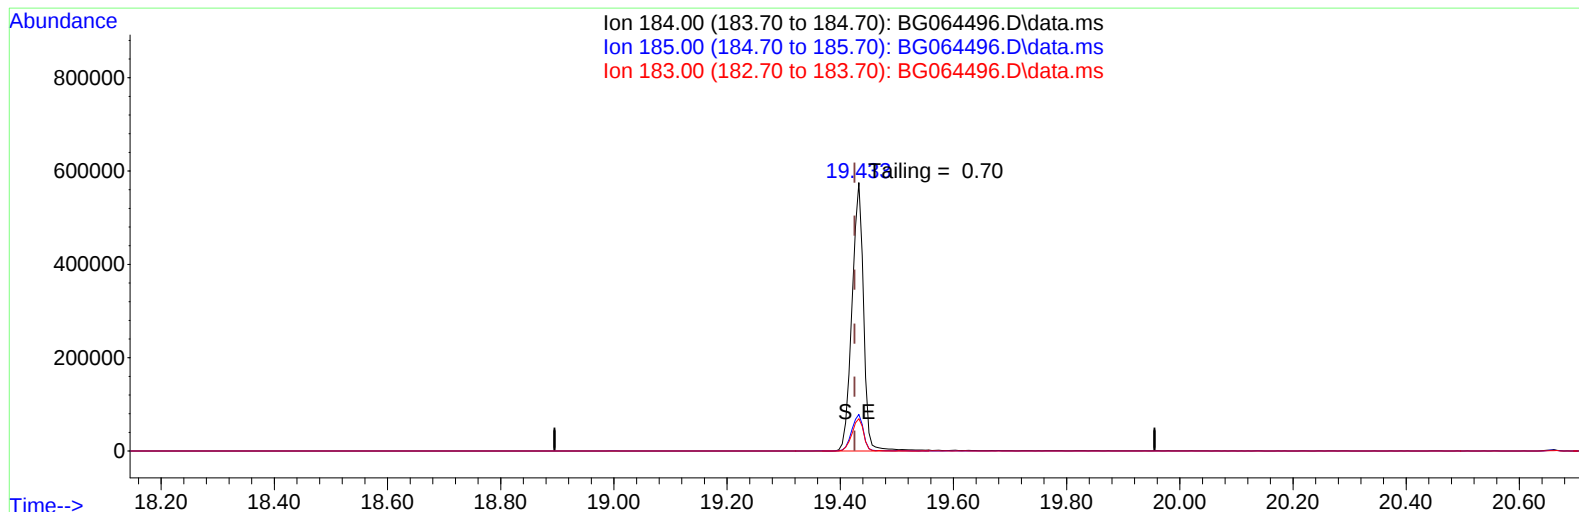

TIC: BG064496.D\data.ms

(77) Benzidine

19.433min (+ 0.008) 0.00 ng

response 816435

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.68
183.00	12.20	12.07
0.00	0.00	0.00