

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101519\
 Data File : BG043241.D
 Acq On : 16 Oct 2019 7:29
 Operator : JU
 Sample : K5355-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMP-32

Quant Time: Oct 16 08:31:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 09 01:11:45 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	59398	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	227217	20.00	ng	0.00
39) Acenaphthene-d10	14.68	164	153606	20.00	ng	0.00
64) Phenanthrene-d10	17.43	188	321454	20.00	ng	0.00
76) Chrysene-d12	21.70	240	357111	20.00	ng	0.00
87) Perylene-d12	24.92	264	419350	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	435365	130.81	ng	0.00
7) Phenol-d6	7.23	99	599094	124.99	ng	0.00
23) Nitrobenzene-d5	9.21	82	387233	82.84	ng	0.00
42) 2,4,6-Tribromophenol	16.17	330	354321	134.14	ng	0.00
45) 2-Fluorobiphenyl	13.30	172	993724	93.79	ng	0.00
79) Terphenyl-d14	20.04	244	1703704	101.66	ng	0.00
Target Compounds						
10) Phenol	7.25	94	14040	3.193	ng	Qvalue # 70
31) Naphthalene	10.91	128	24083	2.153	ng	# 94
50) Dimethylphthalate	14.12	163	83806	7.282	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101519\
Data File : BG043241.D
Acq On : 16 Oct 2019 7:29
Operator : JU
Sample : K5355-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMP-32

Quant Time: Oct 16 08:31:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:11:45 2019
Response via : Initial Calibration

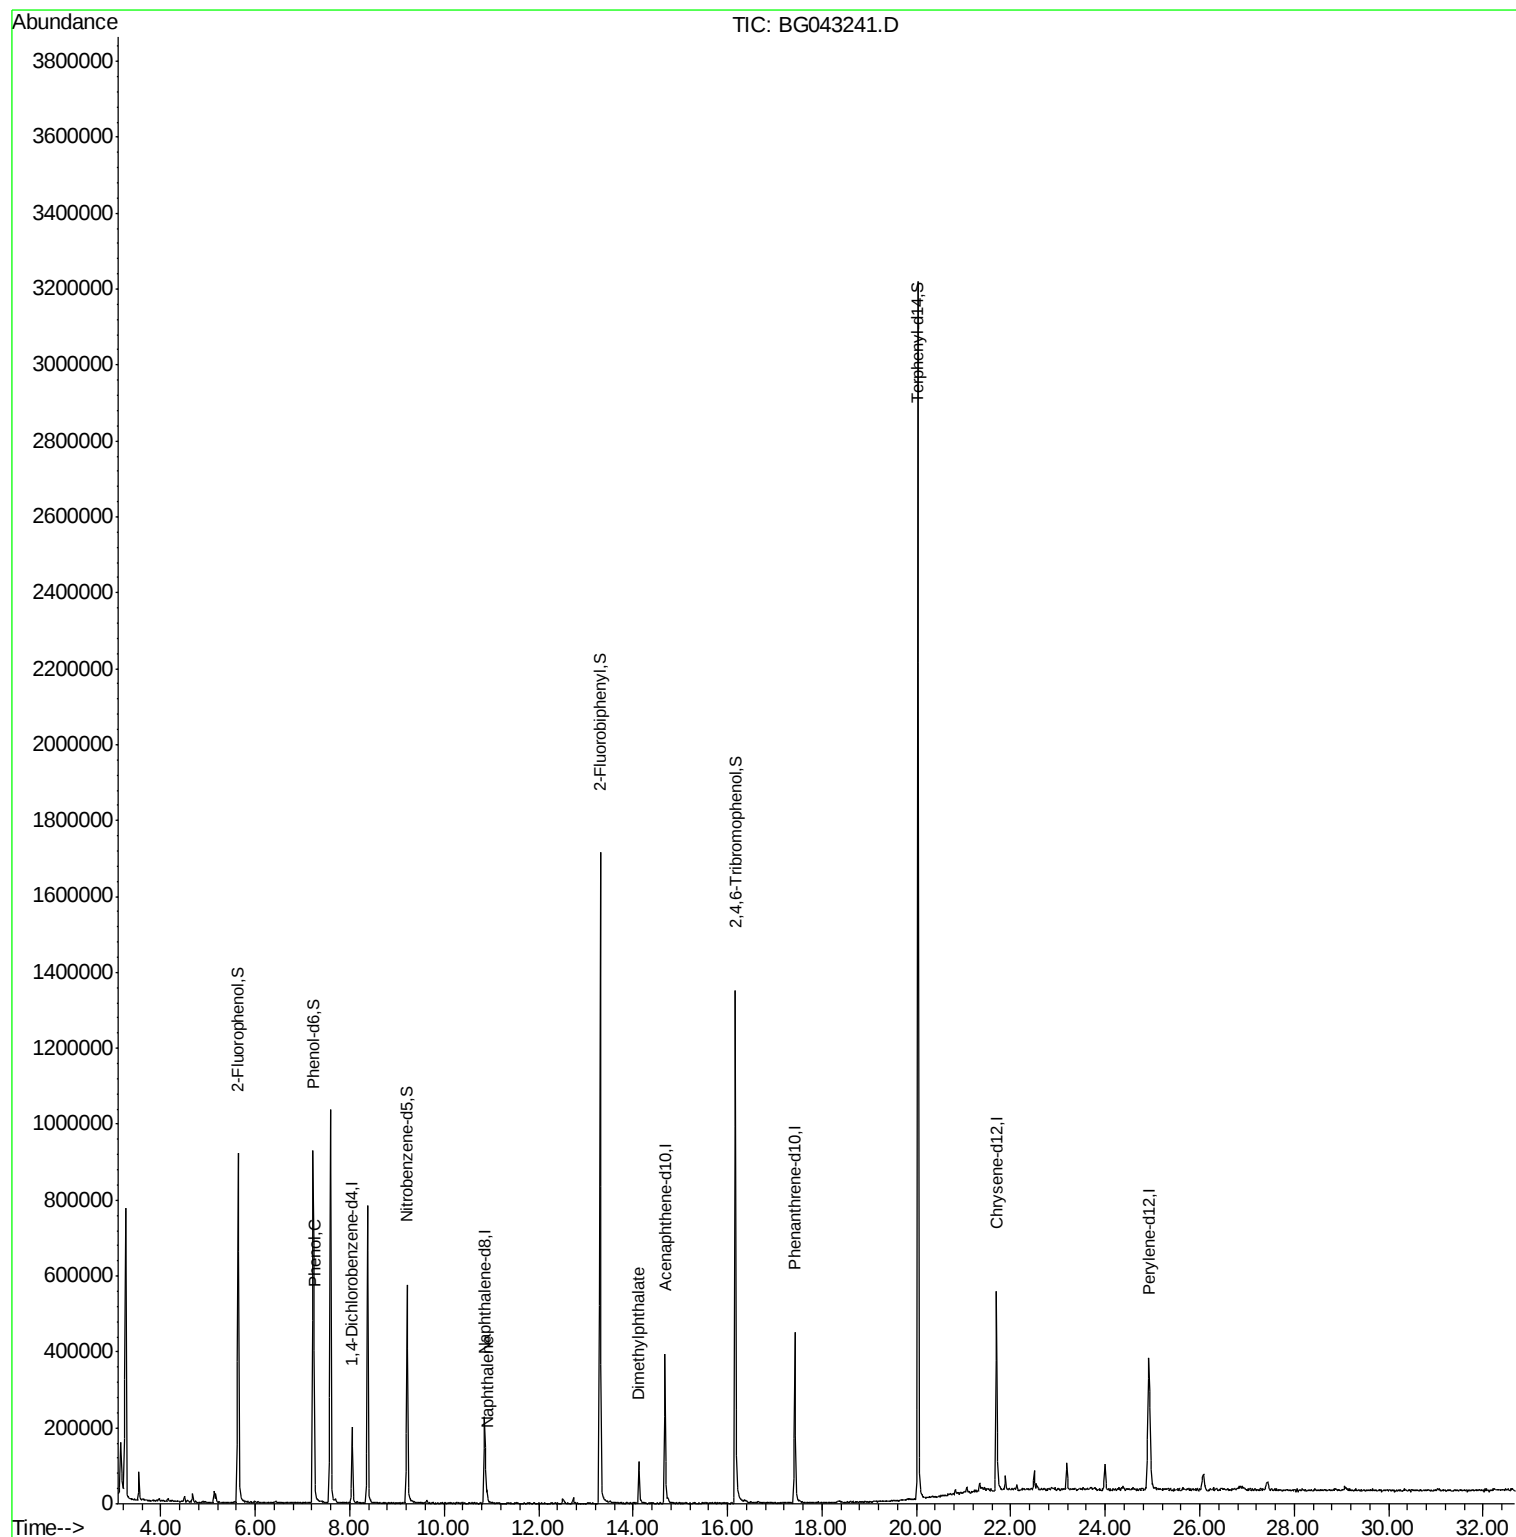




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 845
Delta R.T. -0.00 min
Lab File: BG043241.D
Acq: 16 Oct 2019 7:29

Instrument :
BNA_G
ClientSampleId :
COMP-32

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.0	115.0	172.4
115	57.1	47.0	70.6

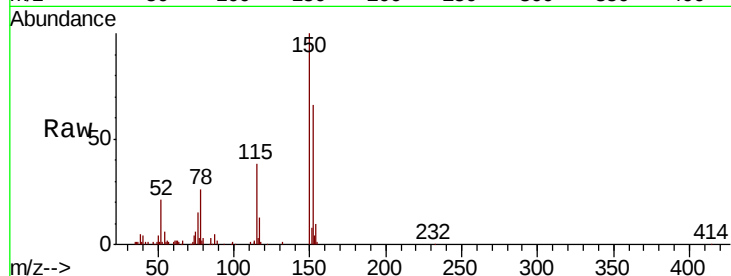


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

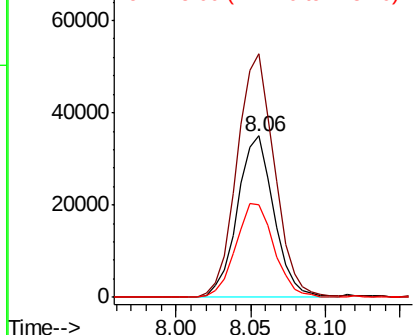



#5


2-Fluorophenol
Concen: 130.806 ng
RT: 5.64 min Scan# 434
Delta R.T. 0.00 min
Lab File: BG043241.D
Acq: 16 Oct 2019 7:29

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.4	56.6	84.8
63	34.7	35.1	52.7#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

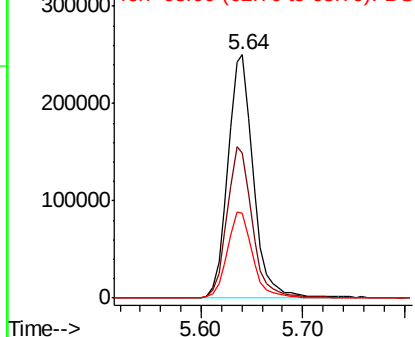

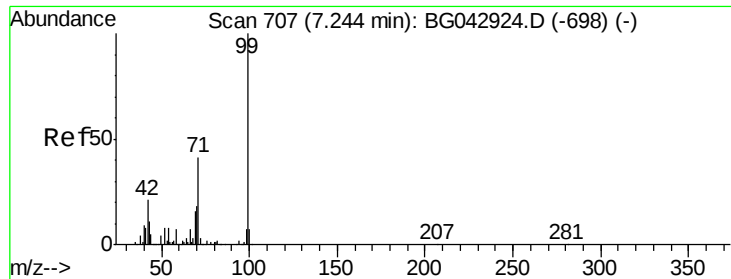

#7

Phenol-d6

Concen: 124.994 ng

RT: 7.23 min Scan# 704

Delta R.T. -0.00 min

Lab File: BG043241.D

Acq: 16 Oct 2019 7:29

Instrument :

BNA_G

ClientSampleId :

COMP-32


Tot Ion: 99 Resp: 599094

Ion Ratio Lower Upper




99 100

42 18.1 17.2 25.8

71 40.2 33.1 49.7

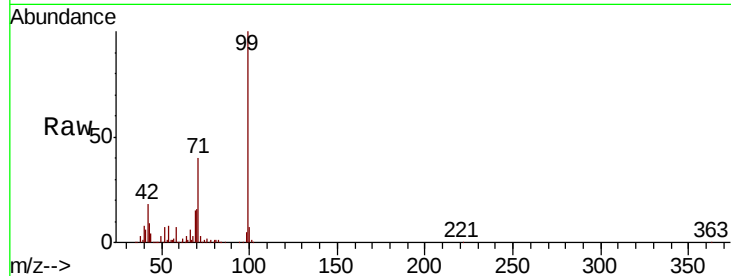

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

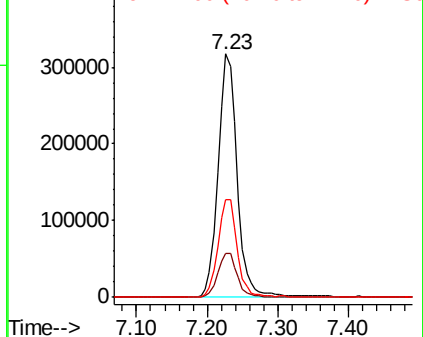

#10

Phenol

Concen: 3.193 ng

RT: 7.25 min Scan# 708

Delta R.T. -0.00 min

Lab File: BG043241.D

Acq: 16 Oct 2019 7:29


Tgt Ion: 94 Resp: 14040

Ion Ratio Lower Upper



94 100


65 39.6 16.6 56.6

66 85.3 32.4 72.4#



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC



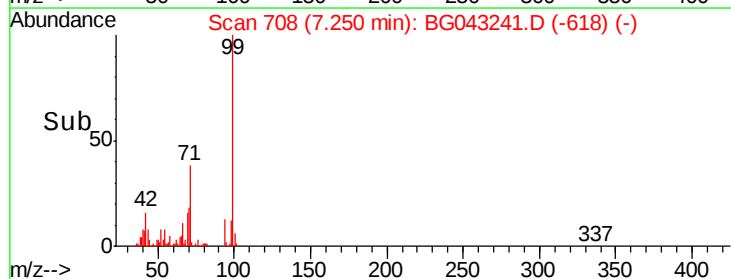
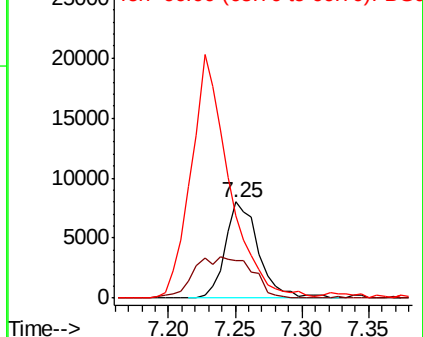




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.86 min Scan# 1322
Delta R.T. -0.00 min
Lab File: BG043241.D
Acq: 16 Oct 2019 7:29




Instrument :
BNA_G
ClientSampleId :
COMP-32


Tot Ion:136	Resp:	227217
Ion Ratio	Lower	Upper
136 100		
137 10.7	8.5	12.7
54 8.6	7.4	11.2
68 4.7	3.6	5.4

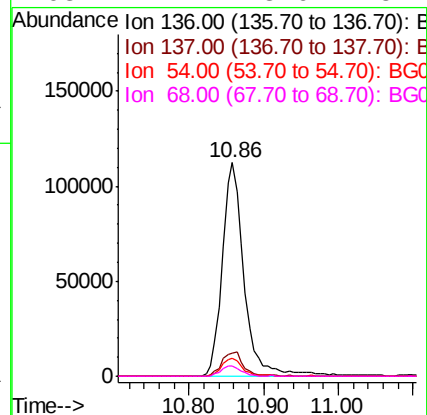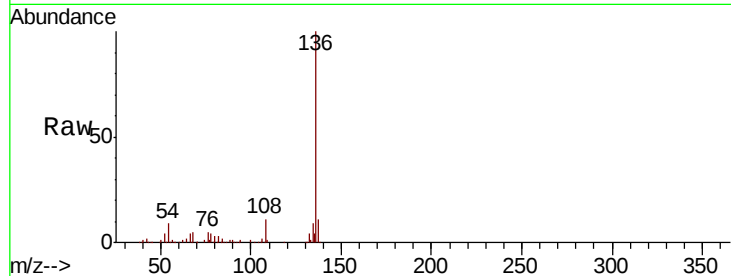

#23
Nitrobenzene-d5
Concen: 82.835 ng
RT: 9.21 min Scan# 1042
Delta R.T. -0.00 min
Lab File: BG043241.D
Acq: 16 Oct 2019 7:29

Tgt	Ion: 82	Resp:	387233
Ion	Ratio	Lower	Upper
82	100		
128	45.2	29.5	44.3#
54	53.5	44.6	67.0



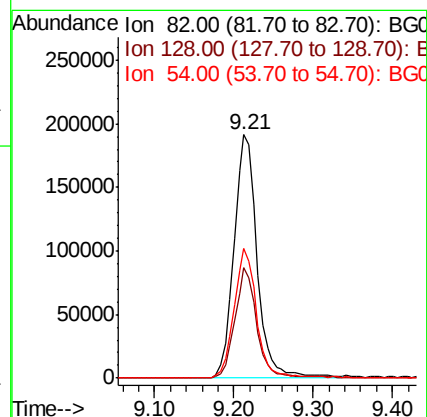
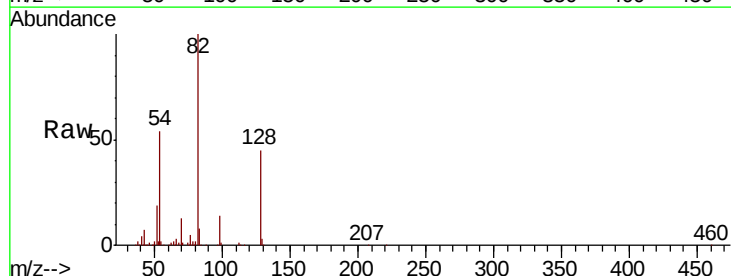




#31
Naphthalene
Concen: 2.153 ng
RT: 10.91 min Scan# 1330
Delta R.T. -0.00 min
Lab File: BG043241.D
Acq: 16 Oct 2019 7:29




Instrument :
BNA_G
ClientSampleId :
COMP-32


Tot Ion	Ratio	Lower	Upper
128	100		
129	9.3	8.8	13.2
127	11.2	11.3	16.9#

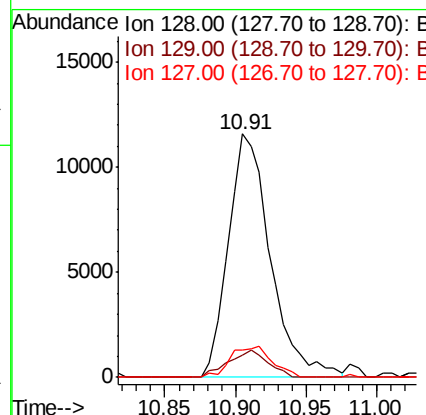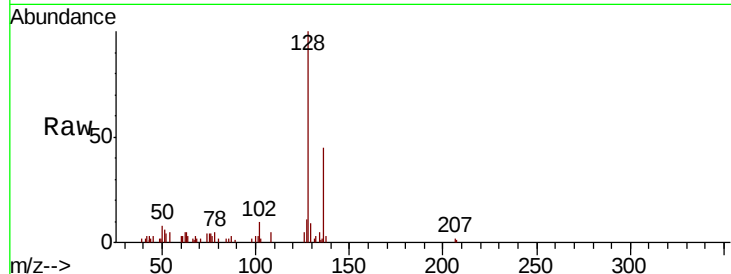

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1972
Delta R.T. -0.00 min
Lab File: BG043241.D
Acq: 16 Oct 2019 7:29

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.2	78.5	117.7
160	43.3	35.9	53.9



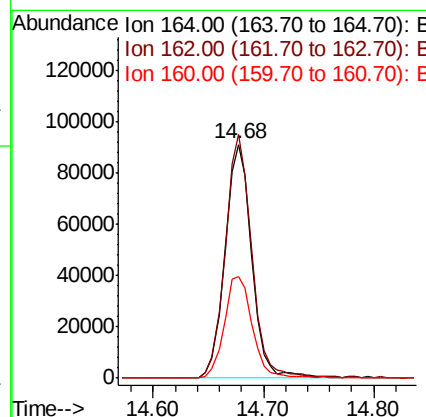
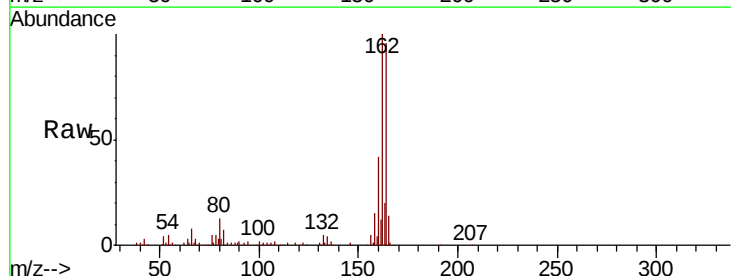




#42
 2,4,6-Tribromophenol
 Concen: 134.144 ng
 RT: 16.17 min Scan# 2226
 Delta R.T. 0.00 min
 Lab File: BG043241.D
 Acq: 16 Oct 2019 7:29




Instrument :
 BNA_G
 ClientSampleId :
 COMP-32


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.8	78.2	117.2
141	27.0	26.0	39.0

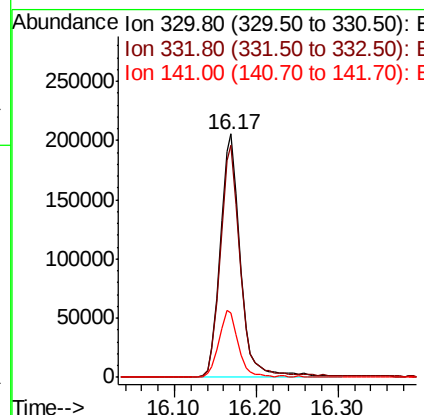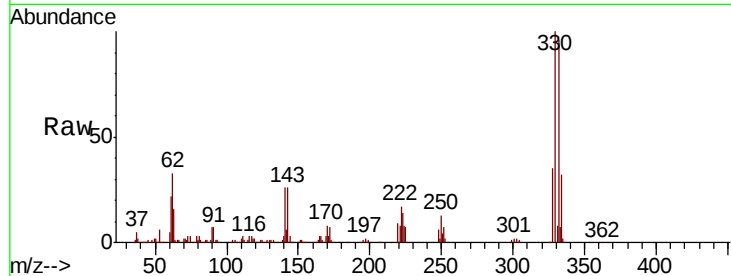

#45
 2-Fluorobiphenyl
 Concen: 93.785 ng
 RT: 13.30 min Scan# 1738
 Delta R.T. -0.00 min
 Lab File: BG043241.D
 Acq: 16 Oct 2019 7:29

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	29.6	44.4
170	23.0	19.6	29.4

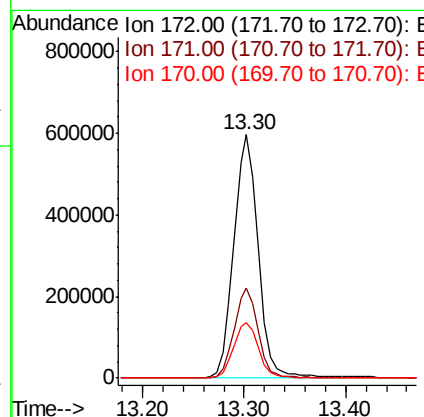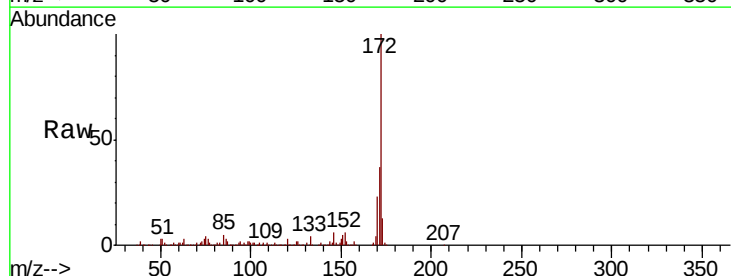







#50
Dimethylphthalate
Concen: 7.282 ng
RT: 14.12 min Scan# 1878
Delta R.T. -0.01 min
Lab File: BG043241.D
Acq: 16 Oct 2019 7:29

Instrument :
BNA_G
ClientSampleId :
COMP-32

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.6	4.4	6.6
164	9.1	8.6	12.8

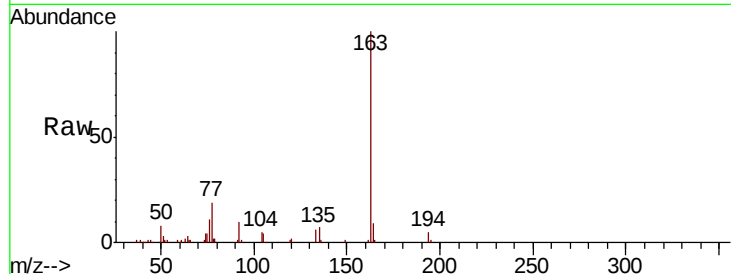


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

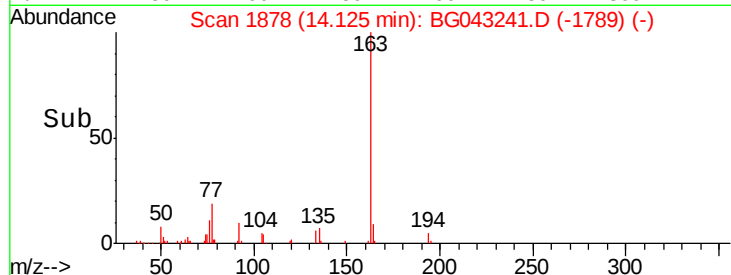
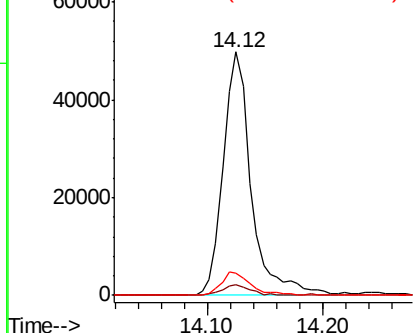



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2440
Delta R.T. 0.01 min
Lab File: BG043241.D
Acq: 16 Oct 2019 7:29

Tgt Ion	Ratio	Lower	Upper
188	100		
94	6.4	5.7	8.5
80	6.3	6.5	9.7#

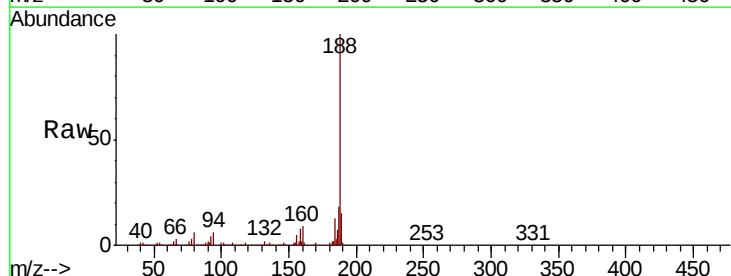

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

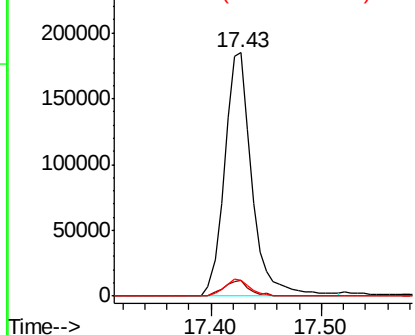



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.70 min Scan# 3167

Delta R.T. 0.01 min

Lab File: BG043241.D

Acq: 16 Oct 2019 7:29

Instrument :

BNA_G

ClientSampleId :

COMP-32


Tot Ion:240 Resp: 357111

Ion Ratio Lower Upper

240 100

120 5.4 4.8 7.2




236 25.3 21.4 32.0



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

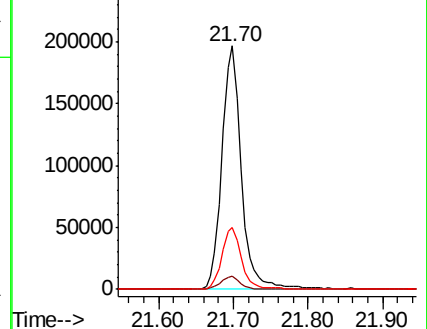

#79

Terphenyl-d14

Concen: 101.660 ng

RT: 20.04 min Scan# 2884

Delta R.T. 0.01 min

Lab File: BG043241.D

Acq: 16 Oct 2019 7:29


Tgt Ion:244 Resp: 1703704

Ion Ratio Lower Upper

244 100

212 7.7 7.4 11.0



122 7.1 7.0 10.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

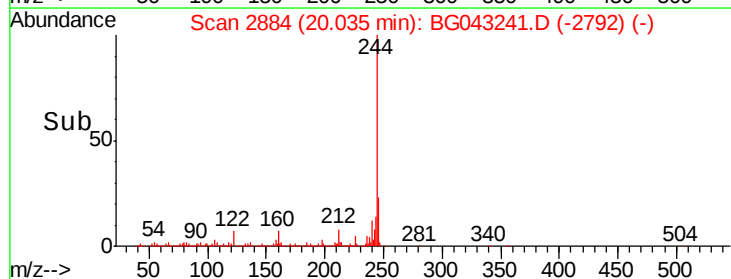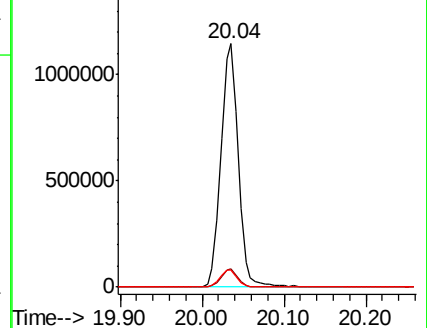


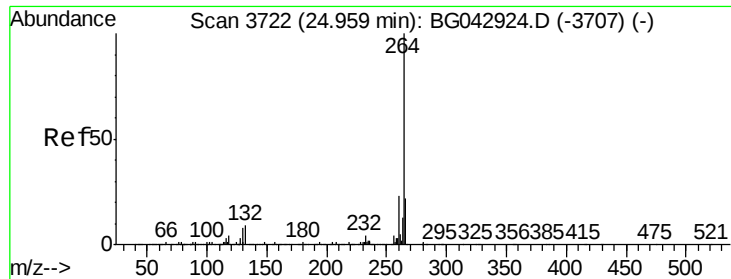

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 24.92 min Scan# 3716
 Delta R.T. 0.01 min
 Lab File: BG043241.D
 Acq: 16 Oct 2019 7:29

Instrument :
 BNA_G
 ClientSampleId :
 COMP-32

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.4	18.7	28.1
265	22.9	17.7	26.5



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

