


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG101519\
 Data File : BG043213.D
 Acq On : 15 Oct 2019 10:50
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 09 01:11:45 2019

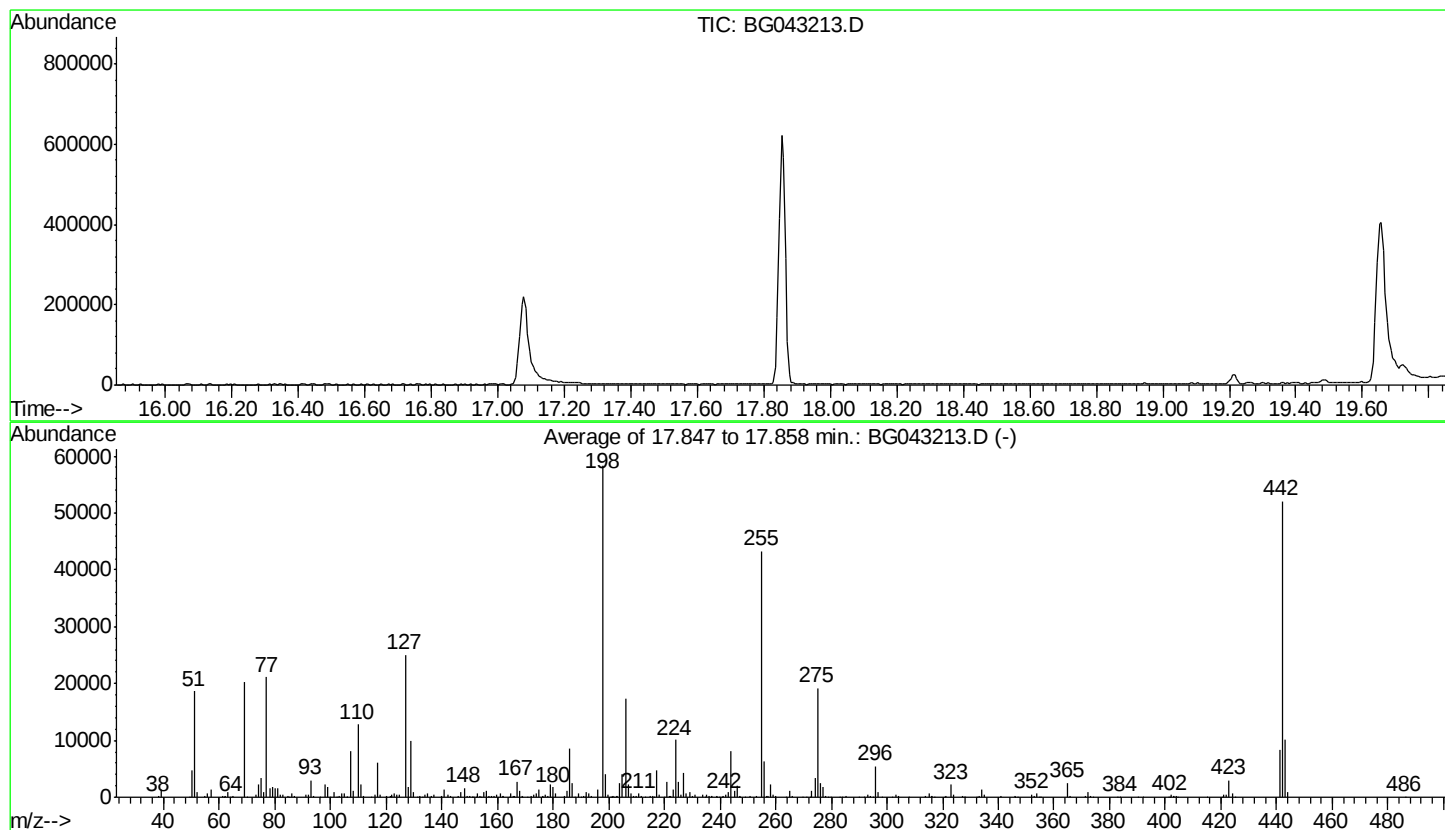

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	18607	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.6	20181	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	43.0	25104	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58336	PASS
199	198	5	9	6.9	3998	PASS
275	198	10	60	32.8	19158	PASS
365	198	1	100	4.3	2498	PASS
441	198	0.01	100	14.1	8244	PASS
442	198	50	100	89.2	52045	PASS
443	442	15	24	19.4	10079	PASS