


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101519\  
 Data File : BG043231.D  
 Acq On : 16 Oct 2019 1:03  
 Operator : JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG092519.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Oct 09 01:11:45 2019

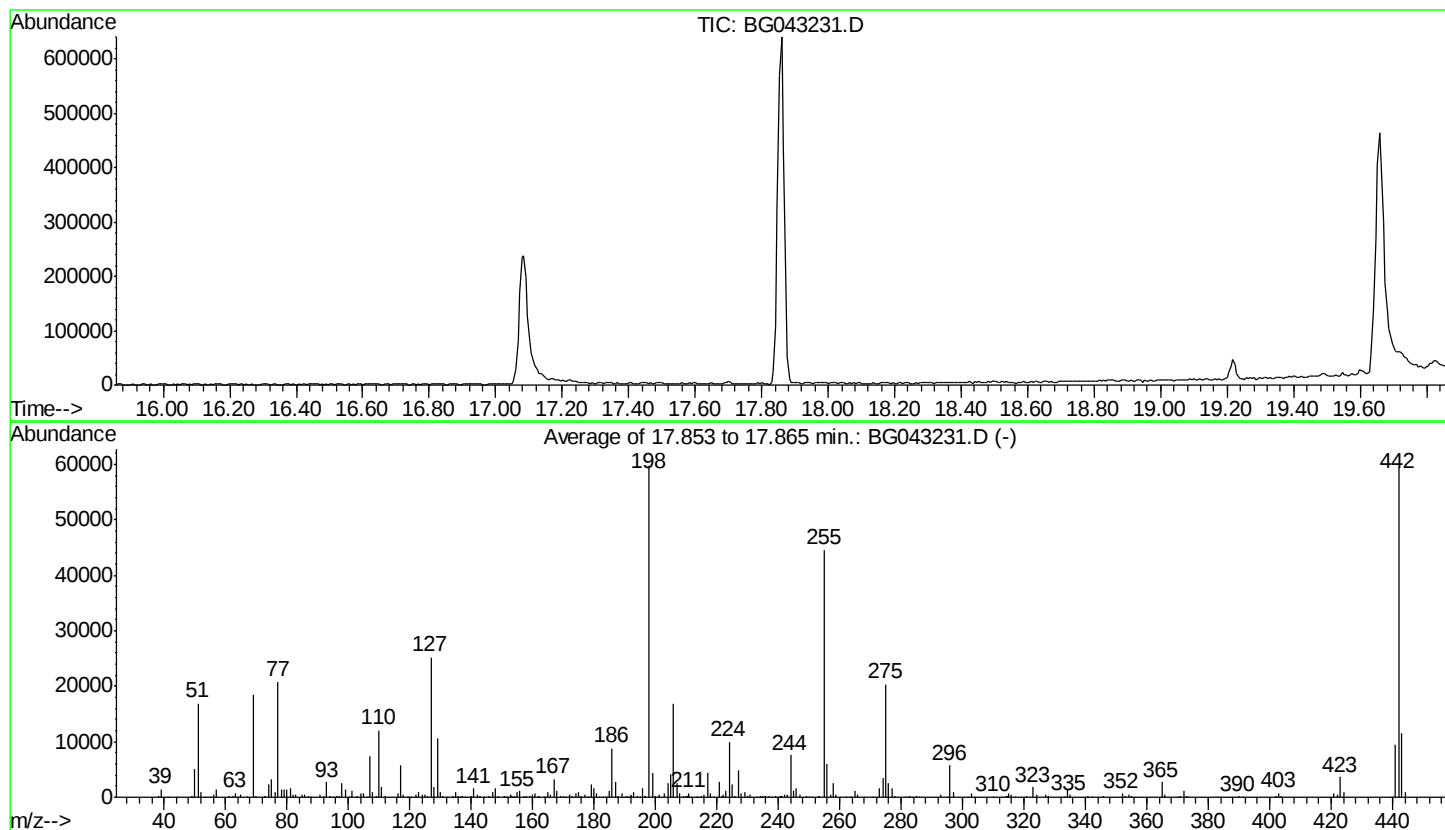

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 28.3      | 16925   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 30.9      | 18479   | PASS             |
| 70          | 69           | 0.00         | 2            | 1.0       | 192     | PASS             |
| 127         | 198          | 10           | 80           | 42.2      | 25216   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 288     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 59781   | PASS             |
| 199         | 198          | 5            | 9            | 7.5       | 4478    | PASS             |
| 275         | 198          | 10           | 60           | 34.0      | 20328   | PASS             |
| 365         | 198          | 1            | 100          | 4.5       | 2685    | PASS             |
| 441         | 198          | 0.01         | 100          | 15.9      | 9501    | PASS             |
| 442         | 198          | 50           | 100          | 99.5      | 59472   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 11647   | PASS             |