

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101618\
 Data File : BG037378.D
 Acq On : 17 Oct 2018 6:19
 Operator : JU/SJ
 Sample : J5198-18
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 17 07:13:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 13:59:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	69280	20.00	ng	-0.01
21) Naphthalene-d8	10.93	136	294964	20.00	ng	-0.02
39) Acenaphthene-d10	14.75	164	196879	20.00	ng	-0.01
64) Phenanthrene-d10	17.49	188	503597	20.00	ng	-0.02
76) Chrysene-d12	21.77	240	465791	20.00	ng	-0.02
87) Perylene-d12	25.12	264	460972	20.00	ng	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.65	112	421518	107.08	ng	0.00
7) Phenol-d6	7.25	99	542553	90.80	ng	0.00
23) Nitrobenzene-d5	9.29	82	376969	84.02	ng	-0.01
42) 2,4,6-Tribromophenol	16.23	330	204753	106.04	ng	-0.01
45) 2-Fluorobiphenyl	13.37	172	915111	69.80	ng	-0.01
79) Terphenyl-d14	20.09	244	1458336	65.74	ng	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) n-Nitroso-di-n-propylamine	9.29	70	45984	10.165	ng	# 71
31) Naphthalene	10.98	128	30059	2.097	ng	# 98
48) 2-Nitroaniline	13.98	65	54	5.769	ng	# 7
51) 2,6-Dinitrotoluene	14.75	165	26019	12.600	ng	# 25
57) 2,4-Dinitrotoluene	14.75	165	26019	11.413	ng	# 24
65) 4,6-Dinitro-2-methylphenol	16.24	198	549	6.251	ng	# 71
67) 4-Bromophenyl-phenylether	16.23	248	14375	2.645	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101618\
Data File : BG037378.D
Acq On : 17 Oct 2018 6:19
Operator : JU/SJ
Sample : J5198-18
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 17 07:13:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

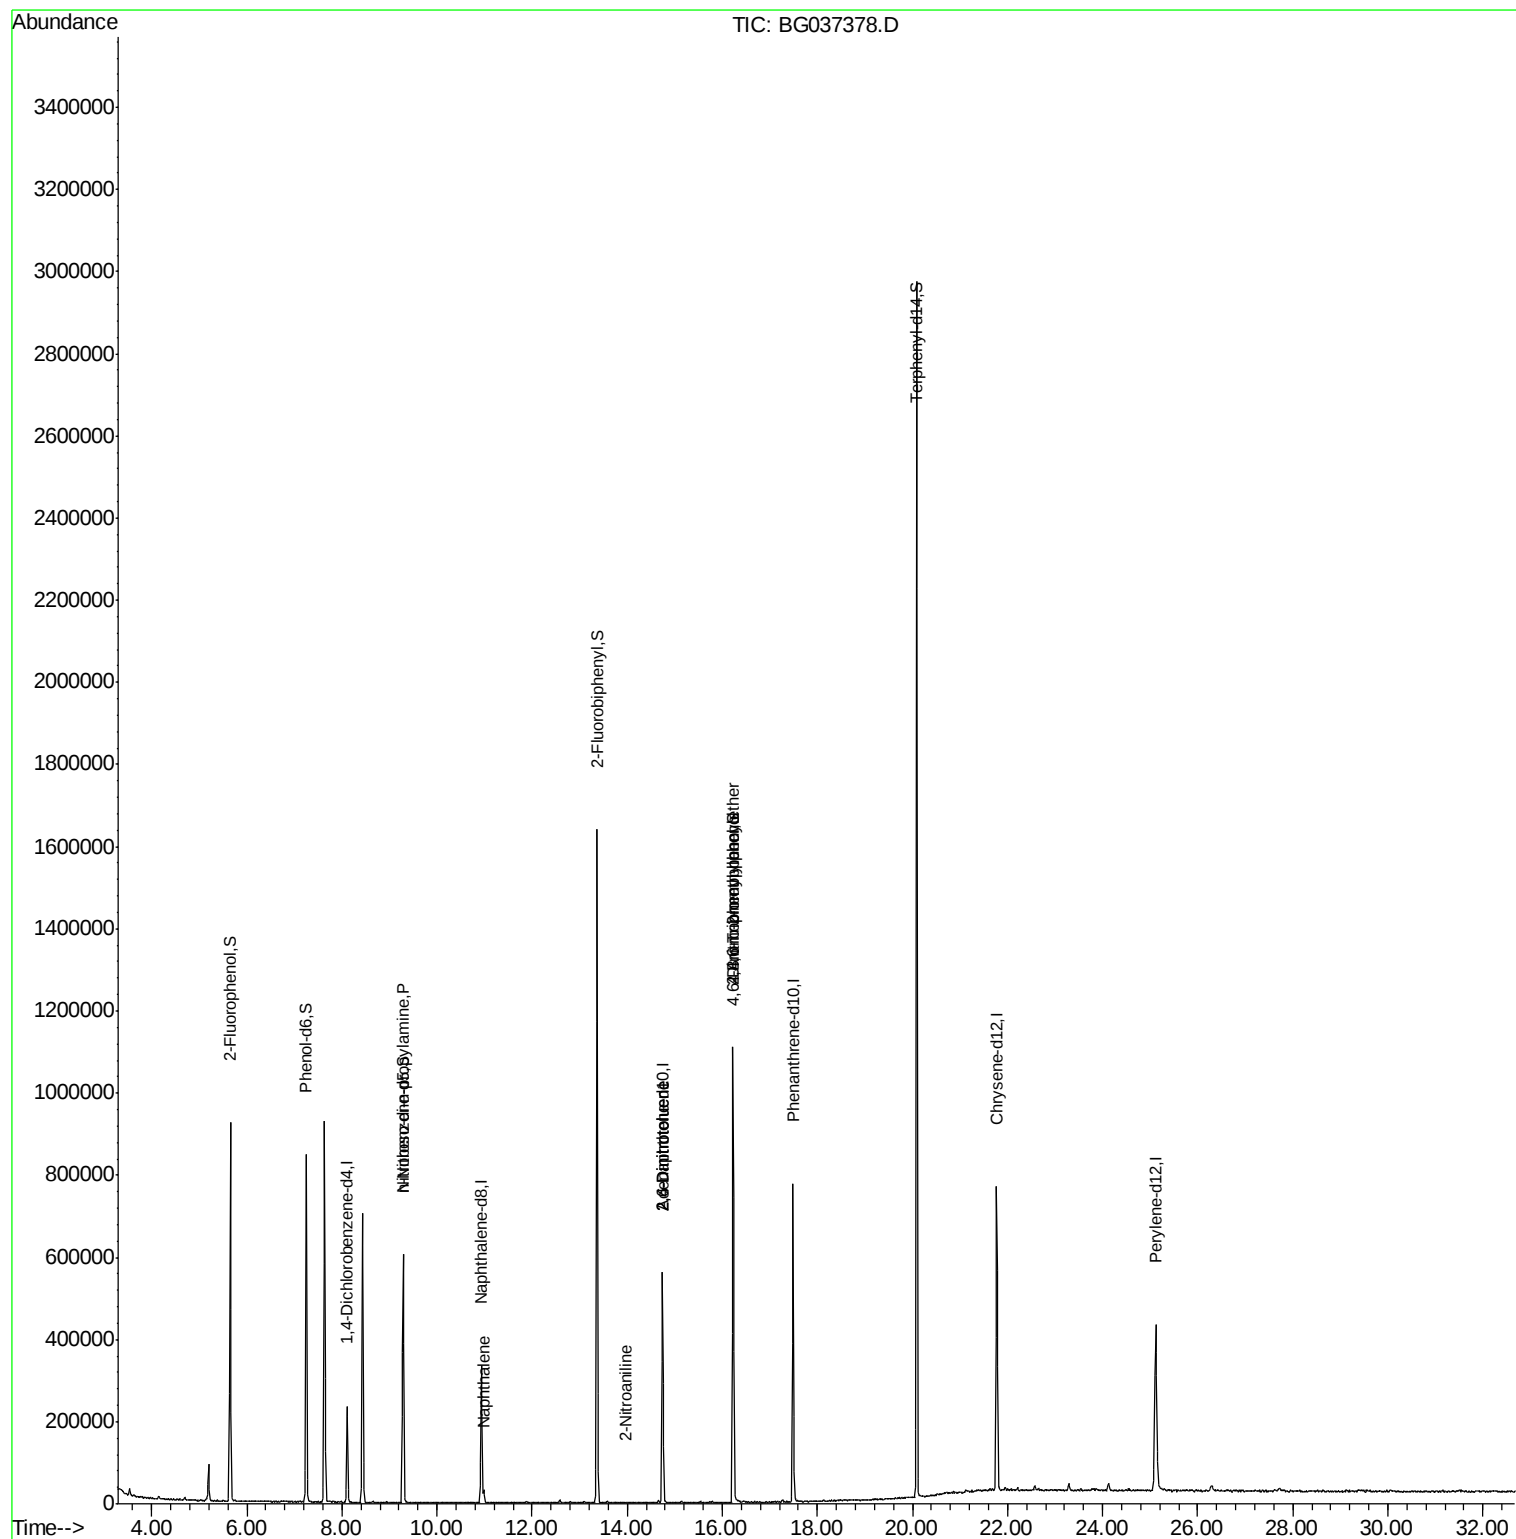

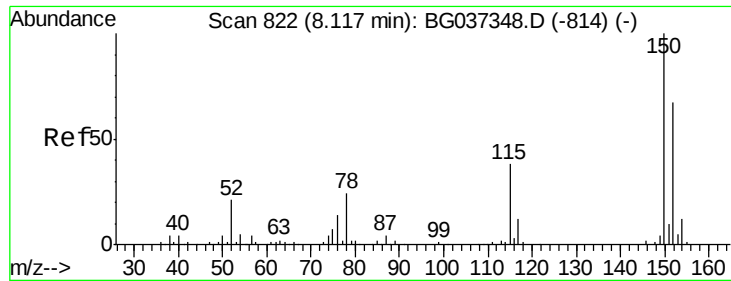


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.11 min Scan# 821
Delta R.T. -0.01 min
Lab File: BG037378.D
Acq: 17 Oct 2018 6:19

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	161.5	126.0	189.0
115	58.4	45.5	68.3



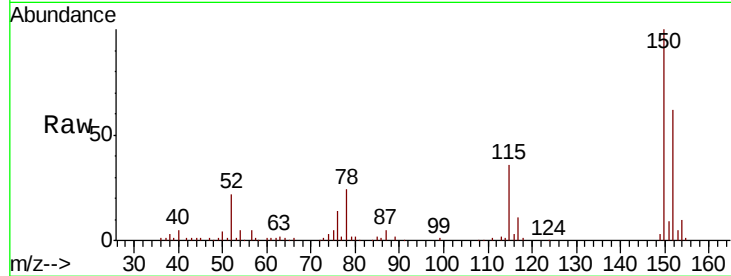


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

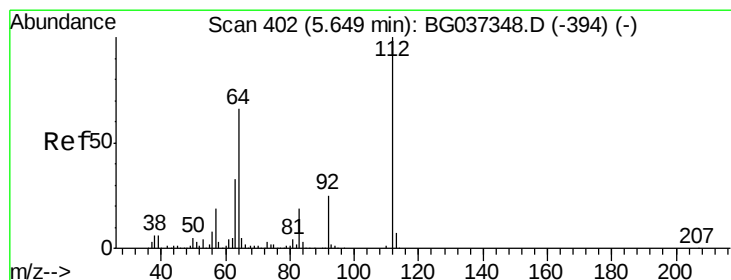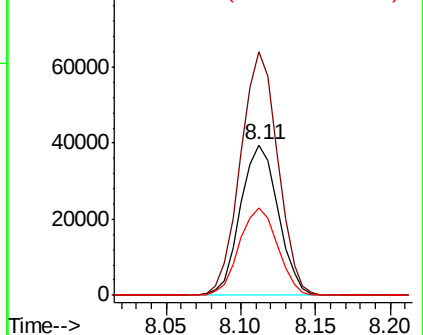

#5

2-Fluorophenol
Concen: 107.077 ng
RT: 5.65 min Scan# 402
Delta R.T. 0.00 min
Lab File: BG037378.D
Acq: 17 Oct 2018 6:19

Tgt Ion	Ratio	Lower	Upper
112	100		
64	64.2	53.1	79.7
63	33.2	27.3	40.9






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

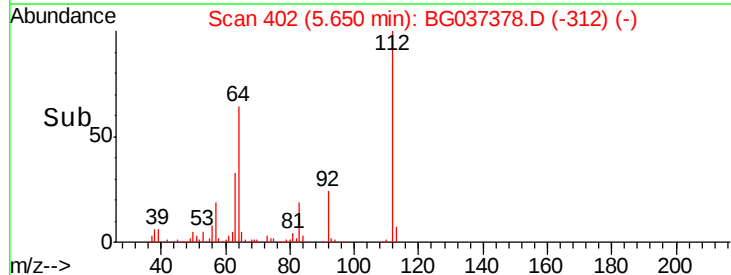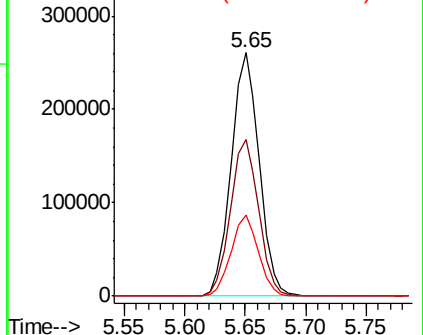

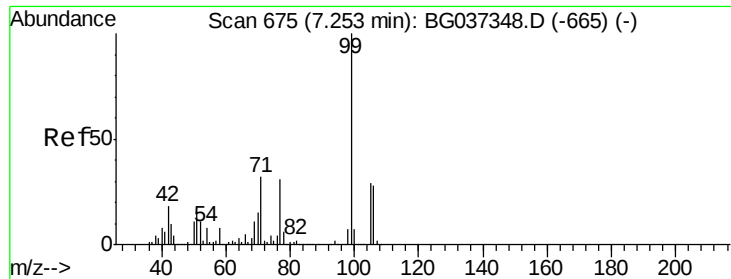

#7

Phenol-d6

Concen: 90.803 ng

RT: 7.25 min Scan# 674

Delta R.T. -0.01 min

Lab File: BG037378.D

Acq: 17 Oct 2018 6:19

Instrument :

BNA_G

ClientSampleId :





Tot Ion: 99 Resp: 542553

Ion Ratio Lower Upper

99 100

42 17.7 15.0 22.4

71 31.4 25.5 38.3

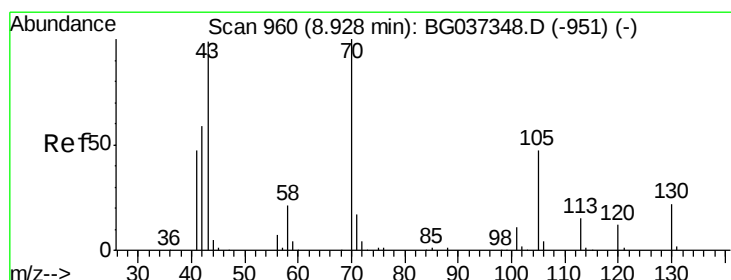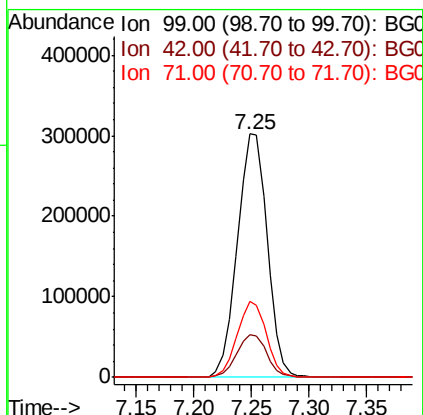

#19

n-Nitroso-di-n-propylamine

Concen: 10.165 ng

RT: 9.29 min Scan# 1021

Delta R.T. 0.36 min

Lab File: BG037378.D

Acq: 17 Oct 2018 6:19

Tgt Ion: 70 Resp: 45984




Ion Ratio Lower Upper


70 100

42 47.2 53.9 80.9#

101 0.0 8.2 12.2#

130 2.2 18.2 27.4#


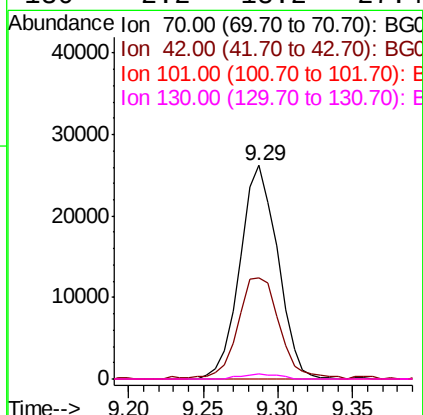




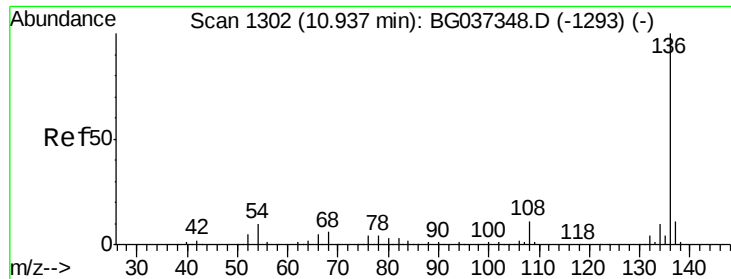

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1301
Delta R.T. -0.02 min
Lab File: BG037378.D
Acq: 17 Oct 2018 6:19




Instrument :
BNA_G
ClientSampled :


Tot Ion:136	Resp:	294964
Ion Ratio	Lower	Upper
136	100	
137	11.7	9.6 14.4
54	9.8	7.9 11.9
68	6.7	4.8 7.2

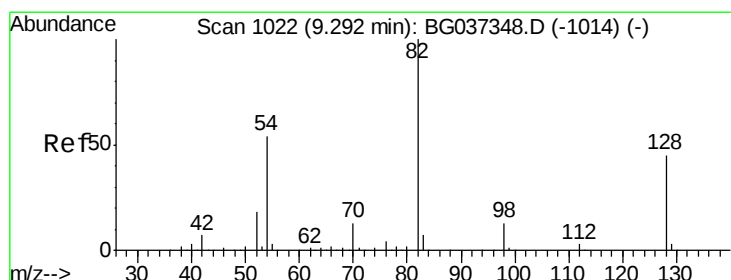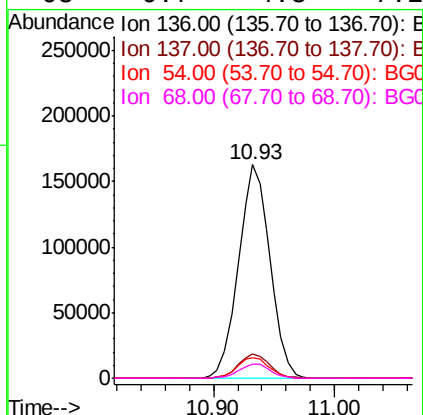

#23
Nitrobenzene-d5
Concen: 84.023 ng
RT: 9.29 min Scan# 1021
Delta R.T. -0.01 min
Lab File: BG037378.D
Acq: 17 Oct 2018 6:19

Tgt Ion: 82	Resp:	376969
Ion Ratio	Lower	Upper
82	100	
128	42.7	34.6 51.8
54	55.3	45.3 67.9

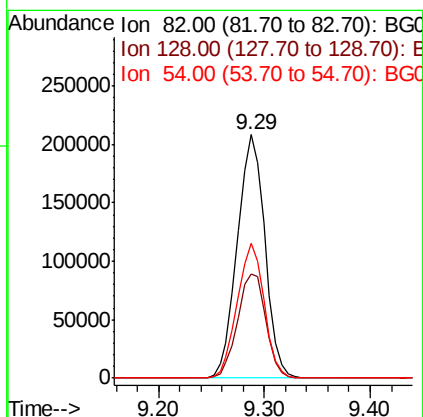


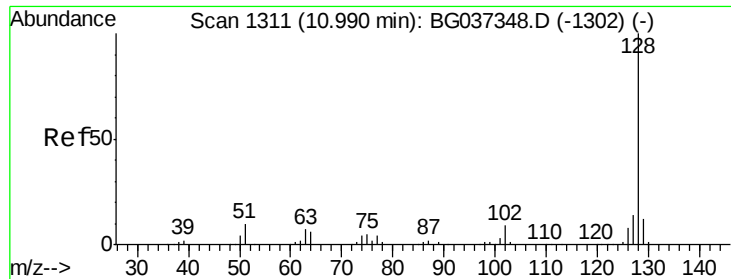




#31
Naphthalene
Concen: 2.097 ng
RT: 10.98 min Scan# 1309
Delta R.T. -0.02 min
Lab File: BG037378.D
Acq: 17 Oct 2018 6:19

Instrument :
BNA_G
ClientSampleId :

Tot Ion:128 Resp: 30059
Ion Ratio Lower Upper
128 100
129 10.7 9.0 13.6
127 13.2 11.1 16.7




Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E


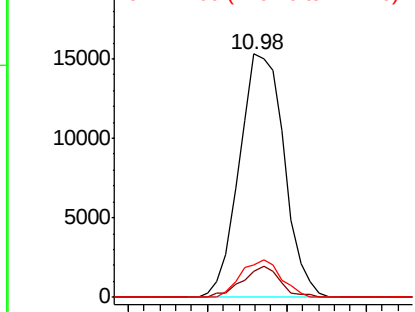



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.75 min Scan# 1950
Delta R.T. -0.01 min
Lab File: BG037378.D
Acq: 17 Oct 2018 6:19

Tgt Ion:164 Resp: 196879
Ion Ratio Lower Upper
164 100
162 100.9 81.3 121.9
160 45.5 36.3 54.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

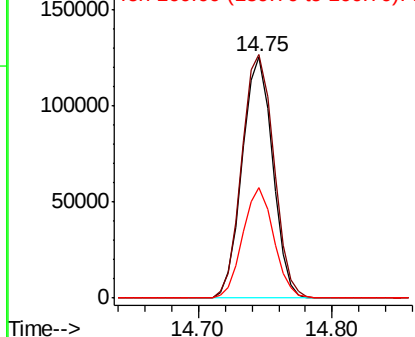


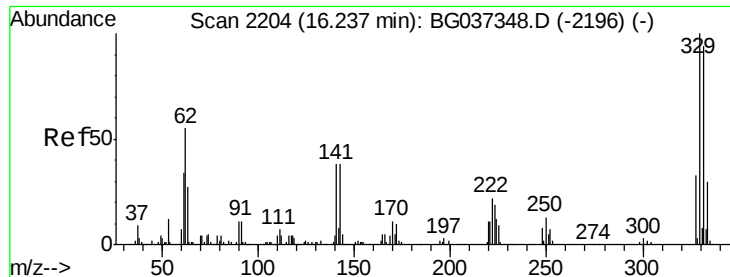




#42
 2,4,6-Tribromophenol
 Concen: 106.044 ng
 RT: 16.23 min Scan# 2203
 Delta R.T. -0.01 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	78.4	117.6
141	40.5	32.2	48.2

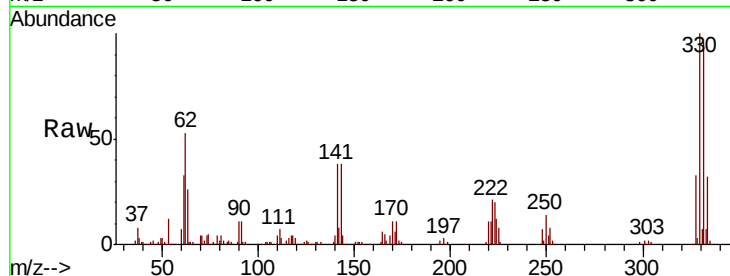


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

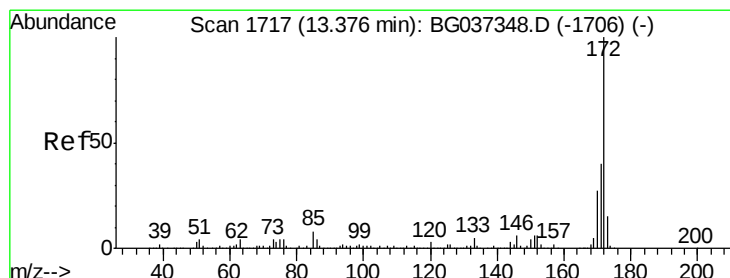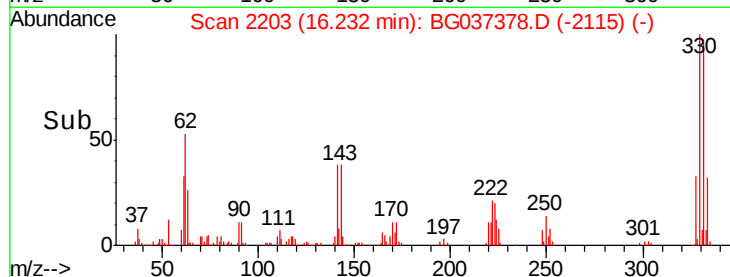
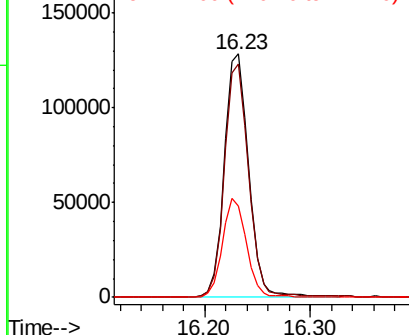



#45
 2-Fluorobiphenyl
 Concen: 69.803 ng
 RT: 13.37 min Scan# 1716
 Delta R.T. -0.01 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.1	31.0	46.4
170	25.2	20.2	30.2

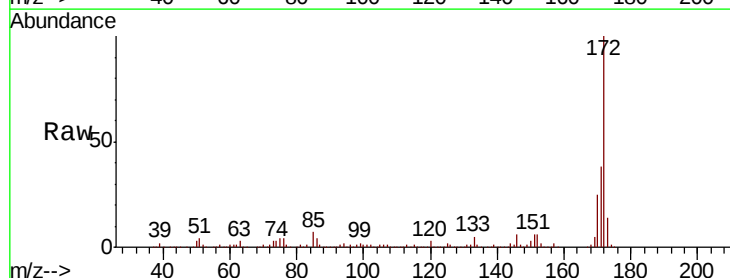

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



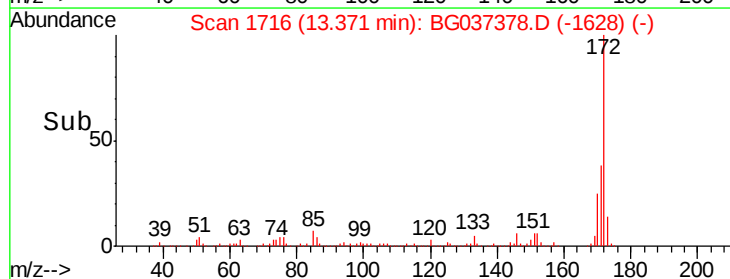
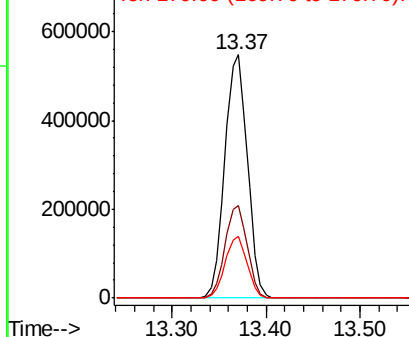


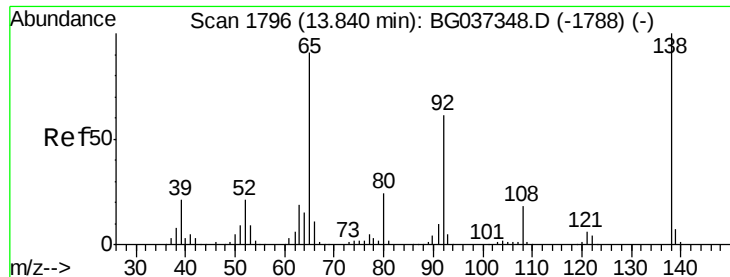

#48
 2-Nitroaniline
 Concen: 5.769 ng
 RT: 13.98 min Scan# 1819
 Delta R.T. 0.14 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
65	100		
92	0.0	53.2	79.8#
138	0.0	79.3	118.9#

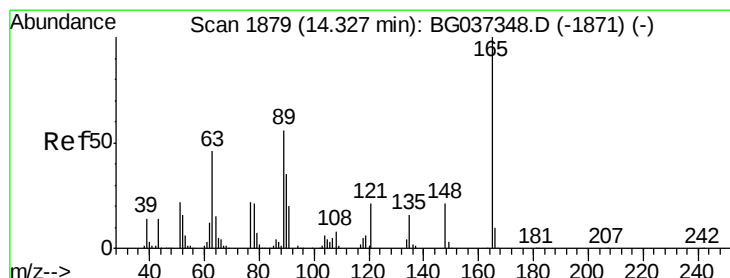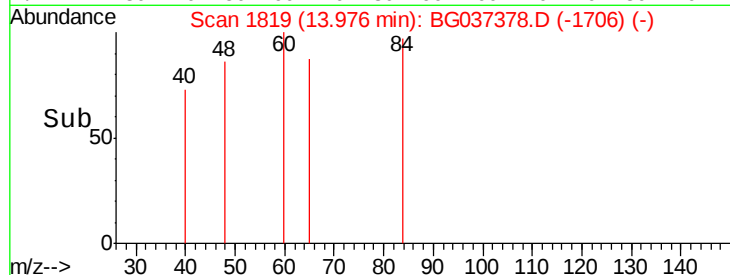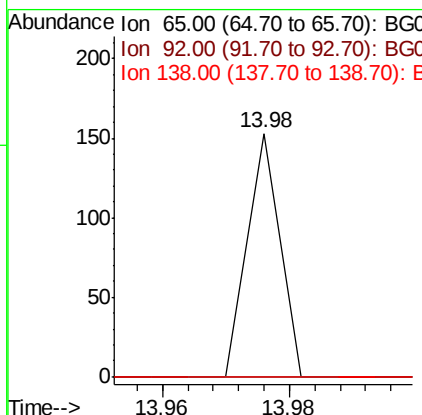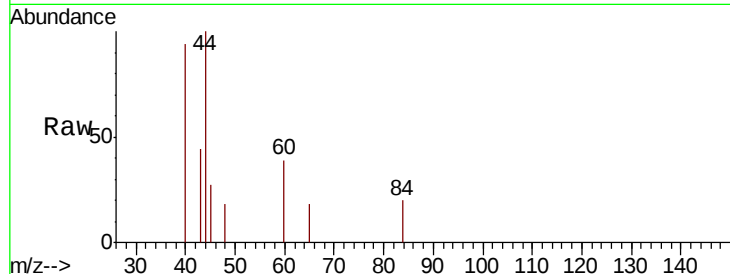

#51
 2,6-Dinitrotoluene
 Concen: 12.600 ng
 RT: 14.75 min Scan# 1950
 Delta R.T. 0.41 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	43.4	65.2#
89	1.7	45.8	68.6#

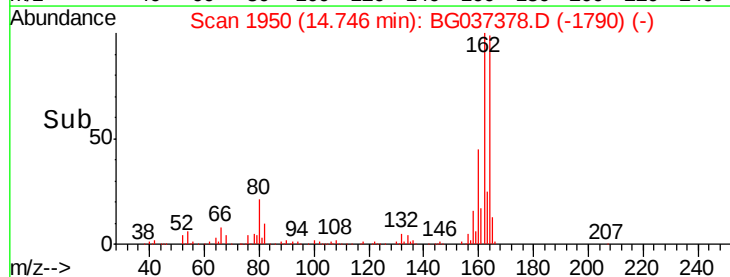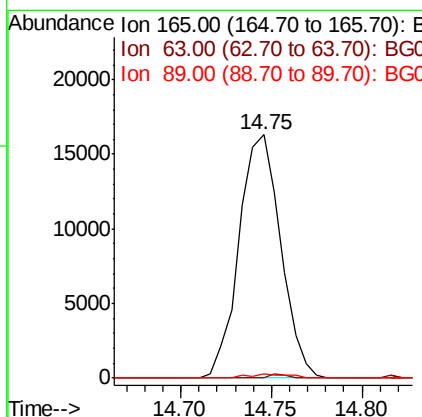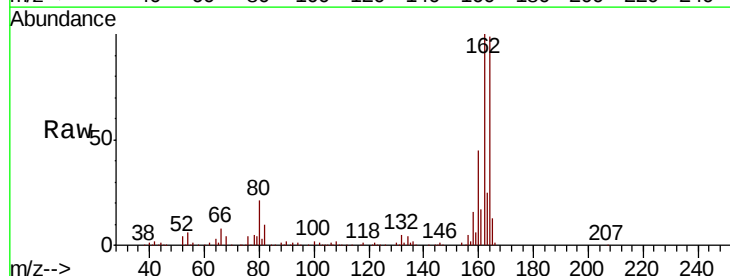




#57
 2,4-Dinitrotoluene
 Concen: 11.413 ng
 RT: 14.75 min Scan# 1950
 Delta R.T. -0.37 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	33.4	50.0#
89	1.7	57.2	85.8#
182	0.0	2.6	4.0#



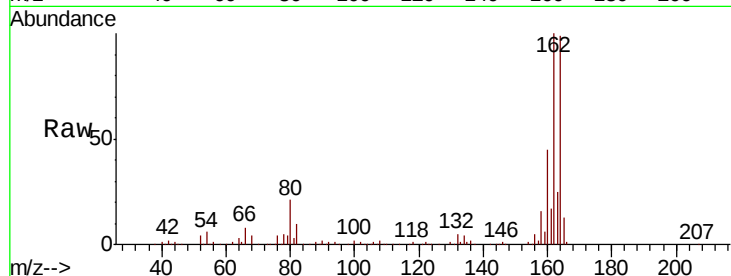


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

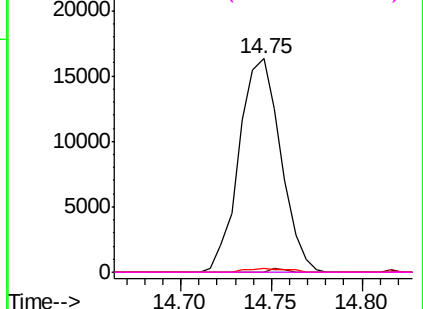

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.49 min Scan# 2417
 Delta R.T. -0.02 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19



Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.4	7.2	10.8
80	10.8	7.7	11.5




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

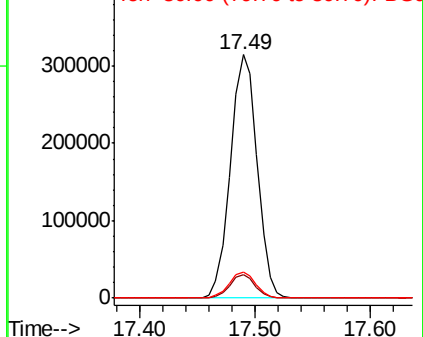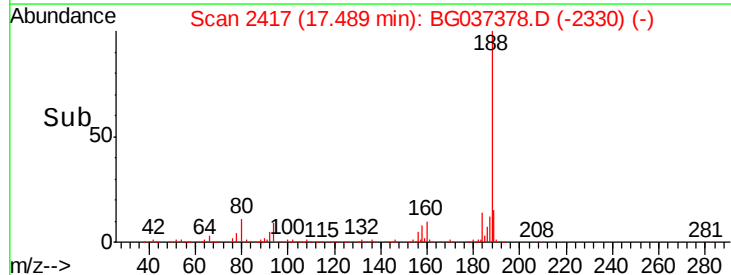


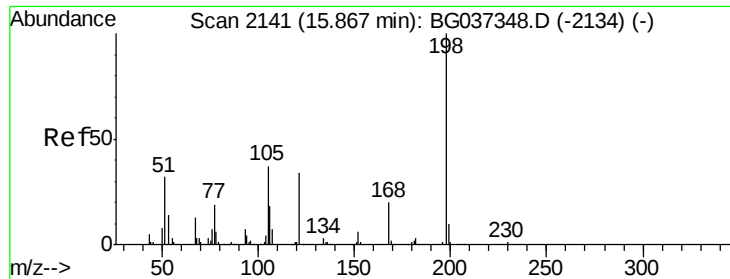




#65
 4,6-Dinitro-2-methylphenol
 Concen: 6.251 ng
 RT: 16.24 min Scan# 2204
 Delta R.T. 0.36 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:198 Resp: 549
 Ion Ratio Lower Upper
 198 100
 51 16.3 22.7 62.7#
 105 29.9 19.7 59.7

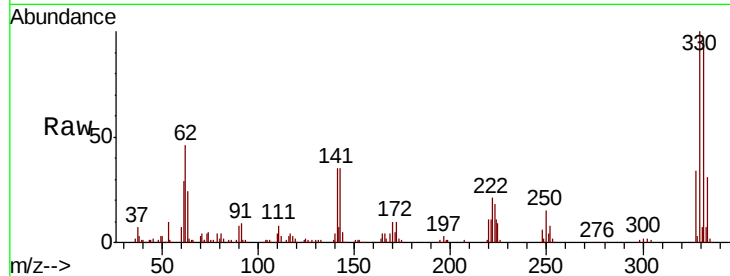


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BG
 Ion 105.00 (104.70 to 105.70): E

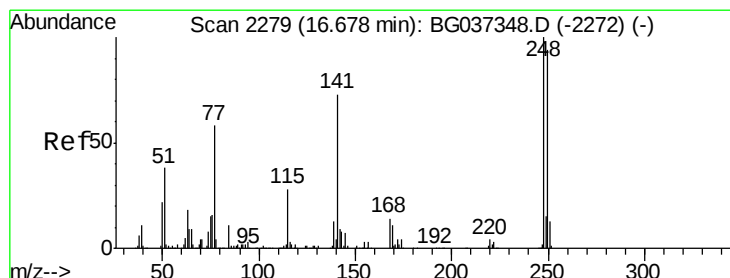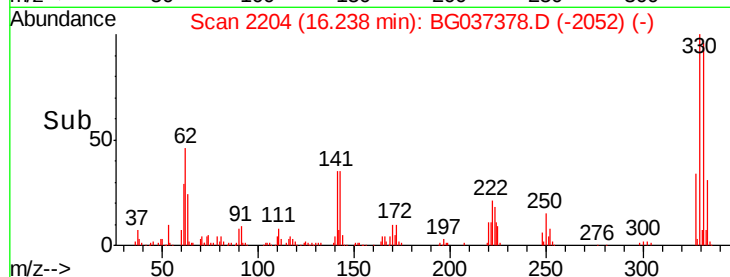
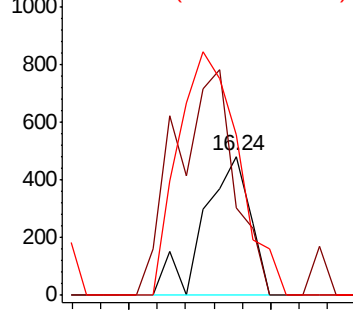



#67
 4-Bromophenyl-phenylether
 Concen: 2.645 ng
 RT: 16.23 min Scan# 2202
 Delta R.T. -0.46 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19

Tgt Ion:248 Resp: 14375
 Ion Ratio Lower Upper
 248 100
 250 201.4 77.0 115.6#
 141 425.5 55.5 83.3#

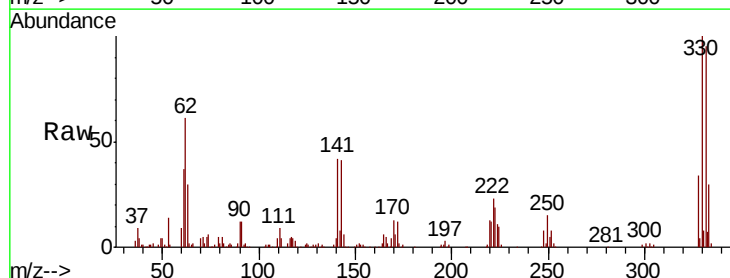

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E



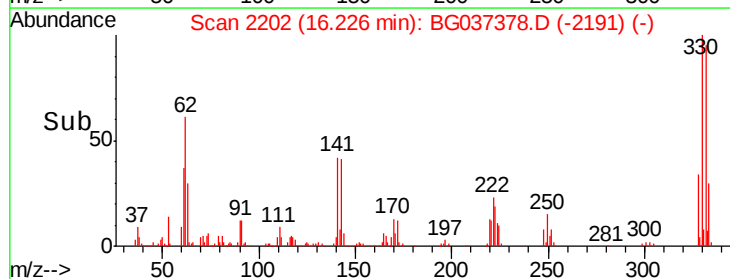
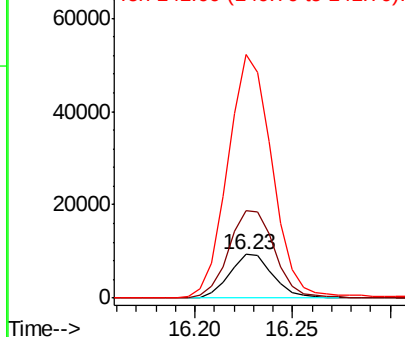


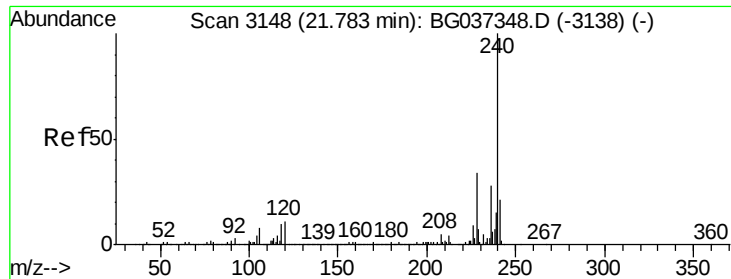

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.77 min Scan# 3146
 Delta R.T. -0.02 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:240 Resp: 465791
 Ion Ratio Lower Upper
 240 100
 120 11.9 8.1 12.1
 236 26.5 21.4 32.0

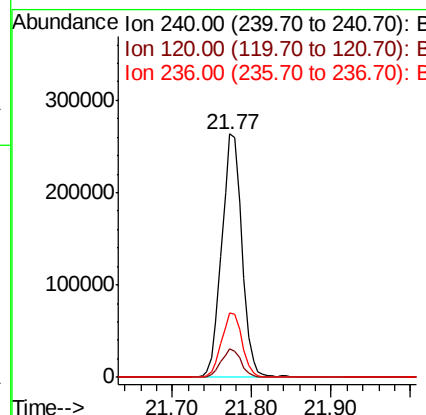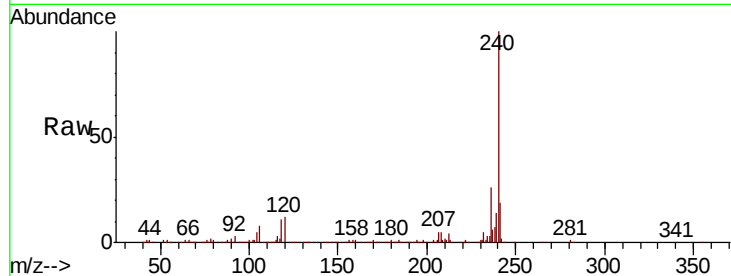

#79
 Terphenyl-d14
 Concen: 65.741 ng
 RT: 20.09 min Scan# 2860
 Delta R.T. -0.01 min
 Lab File: BG037378.D
 Acq: 17 Oct 2018 6:19

Tgt Ion:244 Resp: 1458336
 Ion Ratio Lower Upper
 244 100
 212 8.5 6.5 9.7
 122 11.4 9.0 13.4

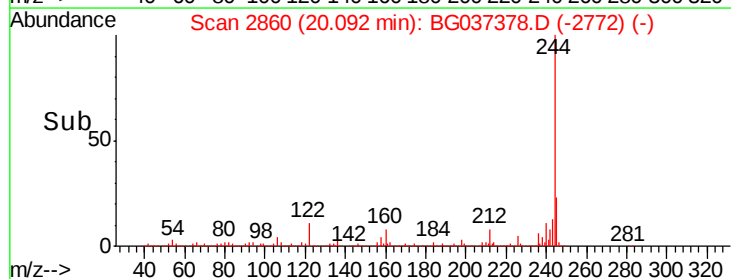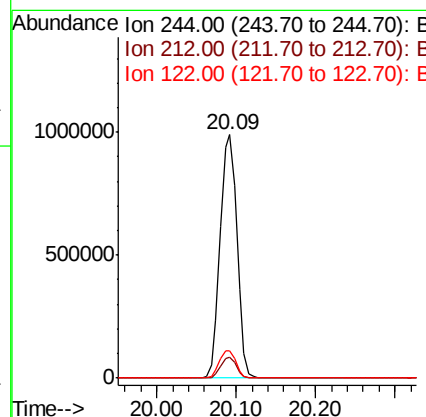

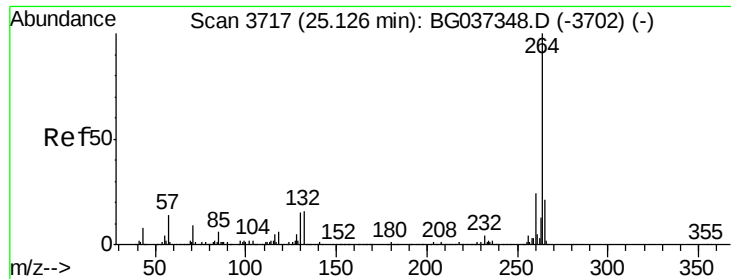

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.12 min Scan# 3715
Delta R.T. -0.03 min
Lab File: BG037378.D
Acq: 17 Oct 2018 6:19

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	18.2	27.4
265	22.3	17.9	26.9

