
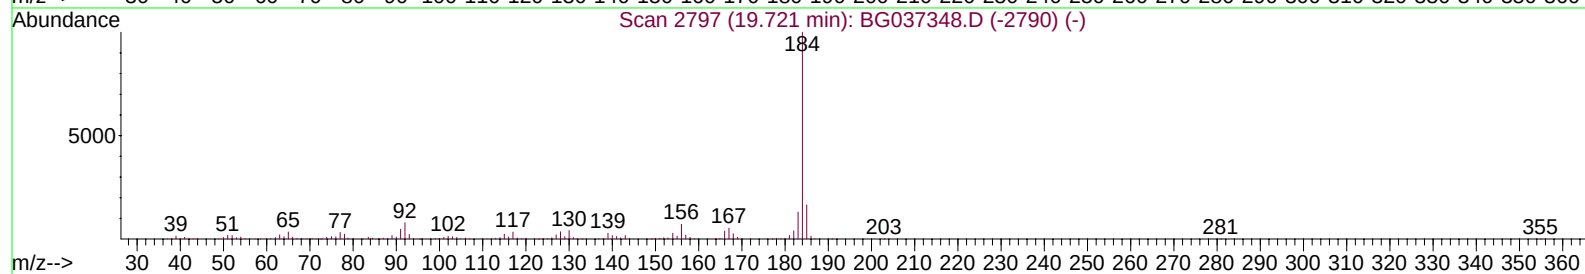
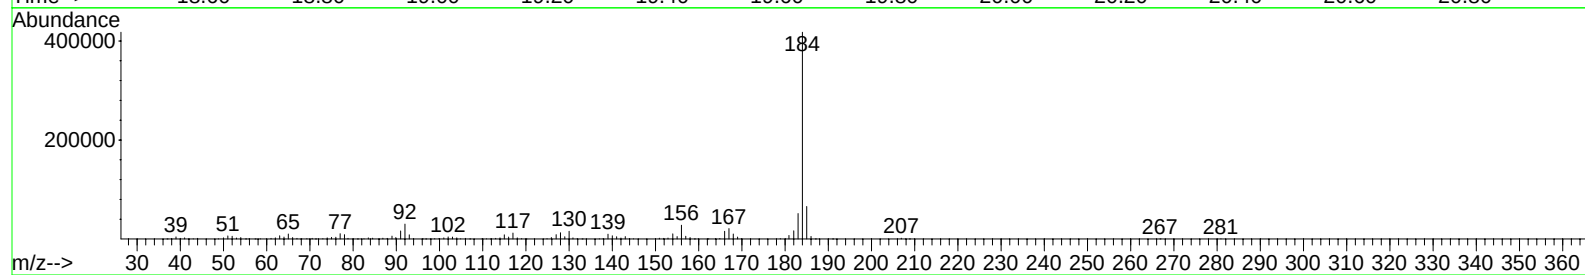


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101618\
Data File : BG037357.D
Acq On : 16 Oct 2018 13:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 06:56:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

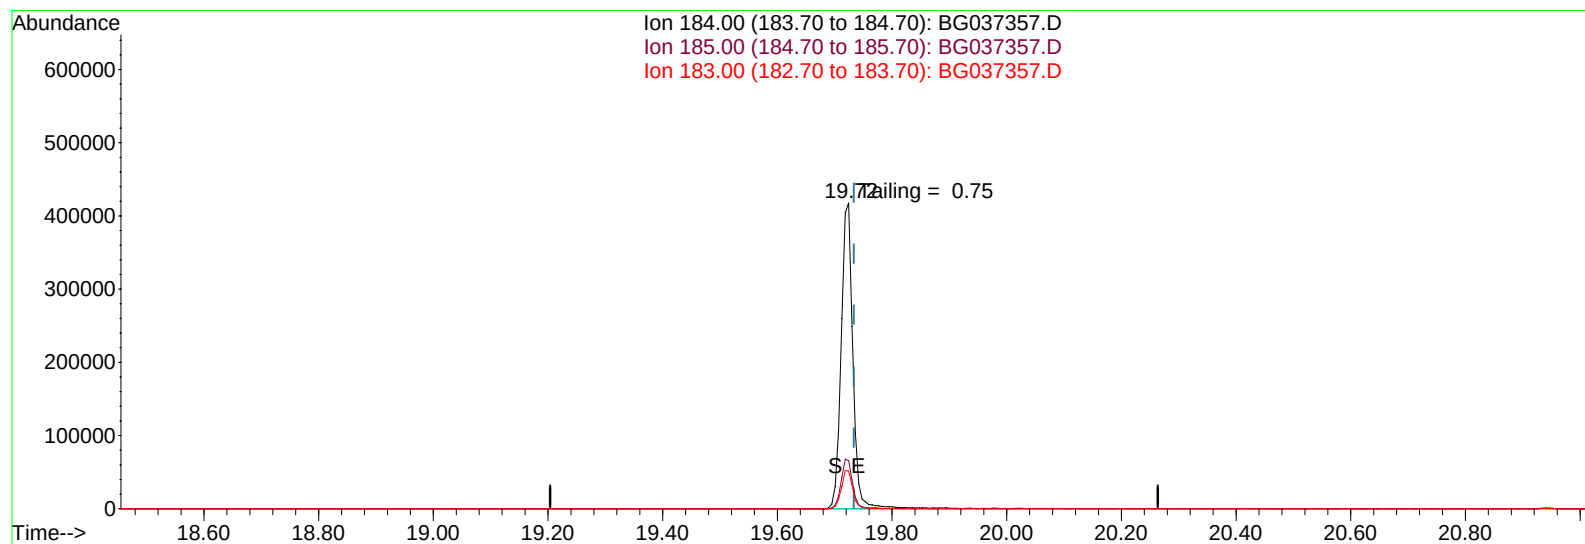

TIC: BG037357.D

(77) Benzidine




19.724min (-0.010) 212278.38ng

response 592822

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.74
183.00	12.70	12.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101618\
Data File : BG037357.D
Acq On : 16 Oct 2018 13:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 06:56:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

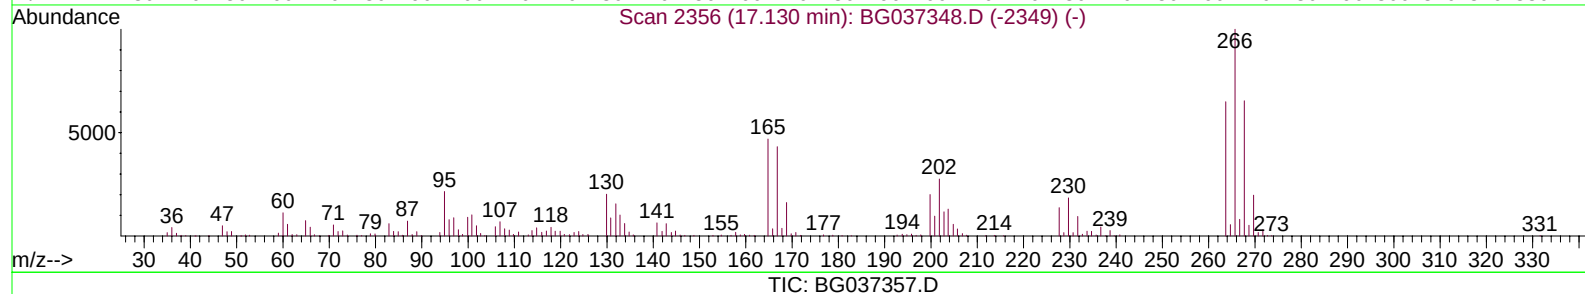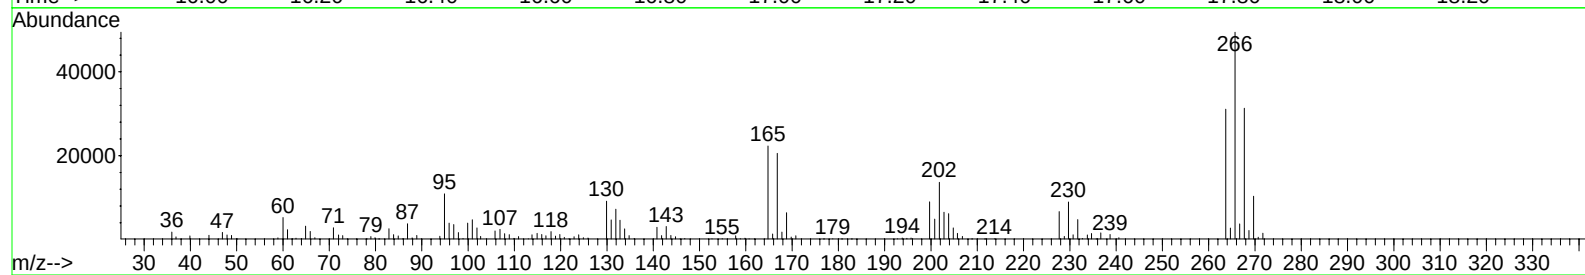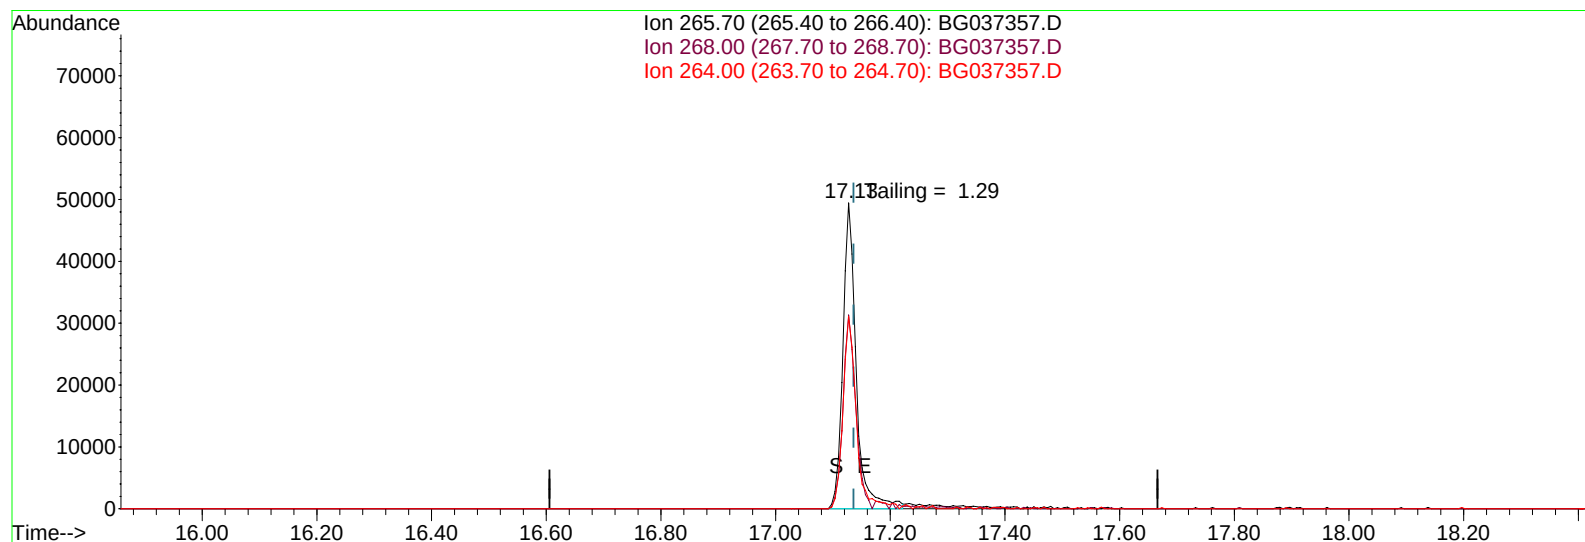

(70) Pentachlorophenol (C)

17.127min (-0.009) 22676.35ng

response 78909

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.72
264.00	73.60	68.44
0.00	0.00	0.00