


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101618\
 Data File : BG037375.D
 Acq On : 17 Oct 2018 3:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 11 13:59:58 2018

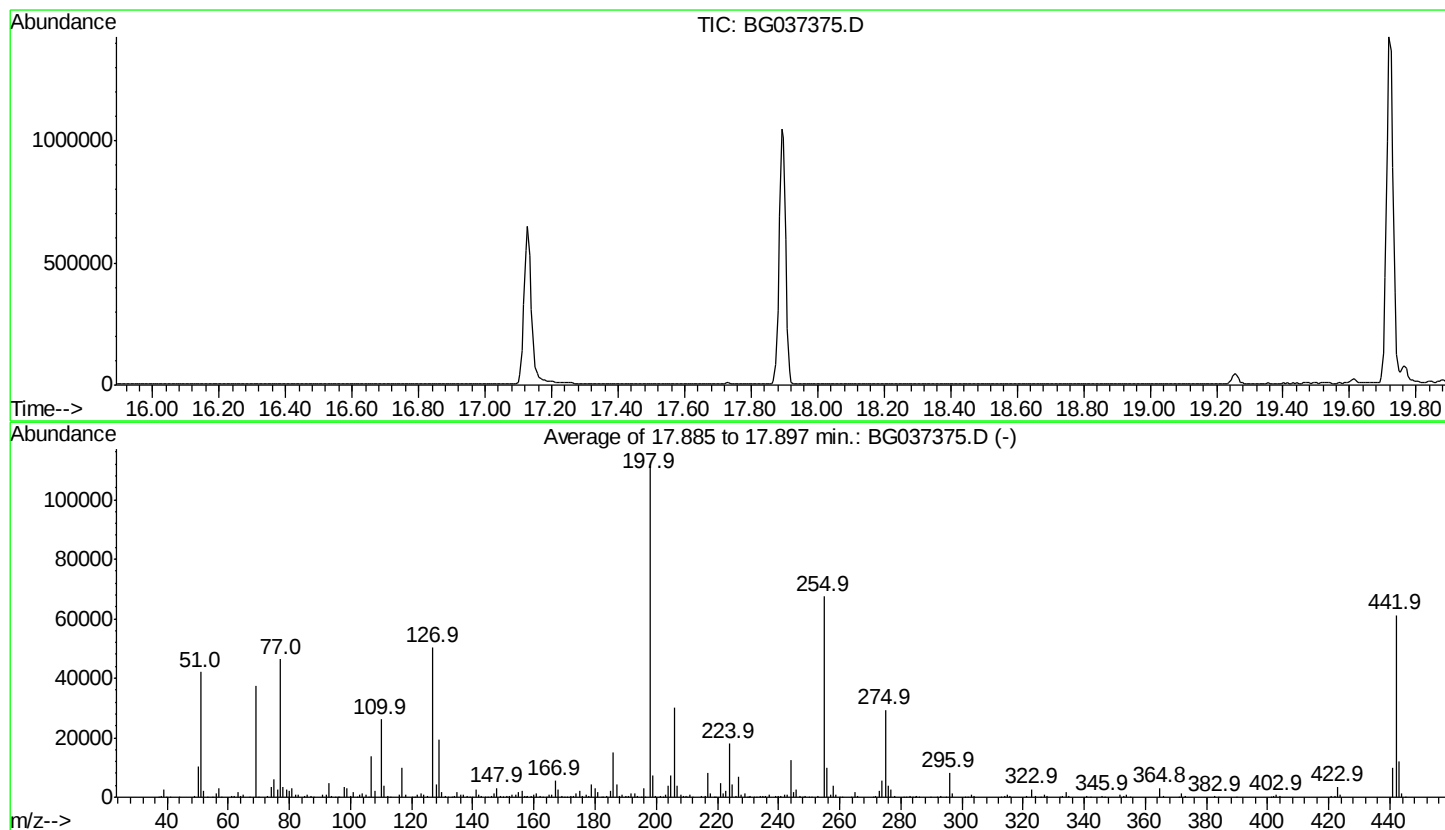

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	41988	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.5	37357	PASS
70	69	0.00	2	0.6	214	PASS
127	198	10	80	45.1	50245	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111458	PASS
199	198	5	9	6.6	7340	PASS
275	198	10	60	26.3	29280	PASS
365	198	1	100	2.8	3171	PASS
441	198	0.01	100	8.7	9719	PASS
442	198	50	100	54.9	61138	PASS
443	442	15	24	19.4	11869	PASS