
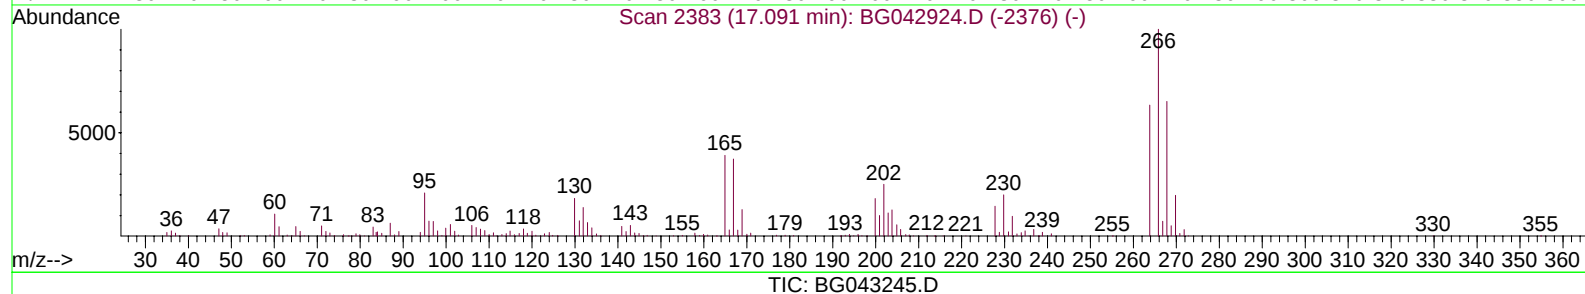
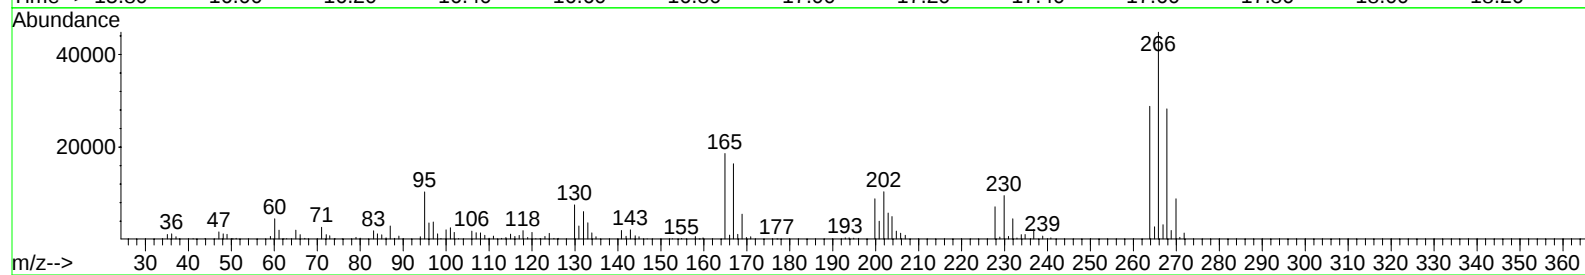


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101619\
Data File : BG043245.D
Acq On : 16 Oct 2019 14:24
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 18:29:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:11:45 2019
Response via : Initial Calibration

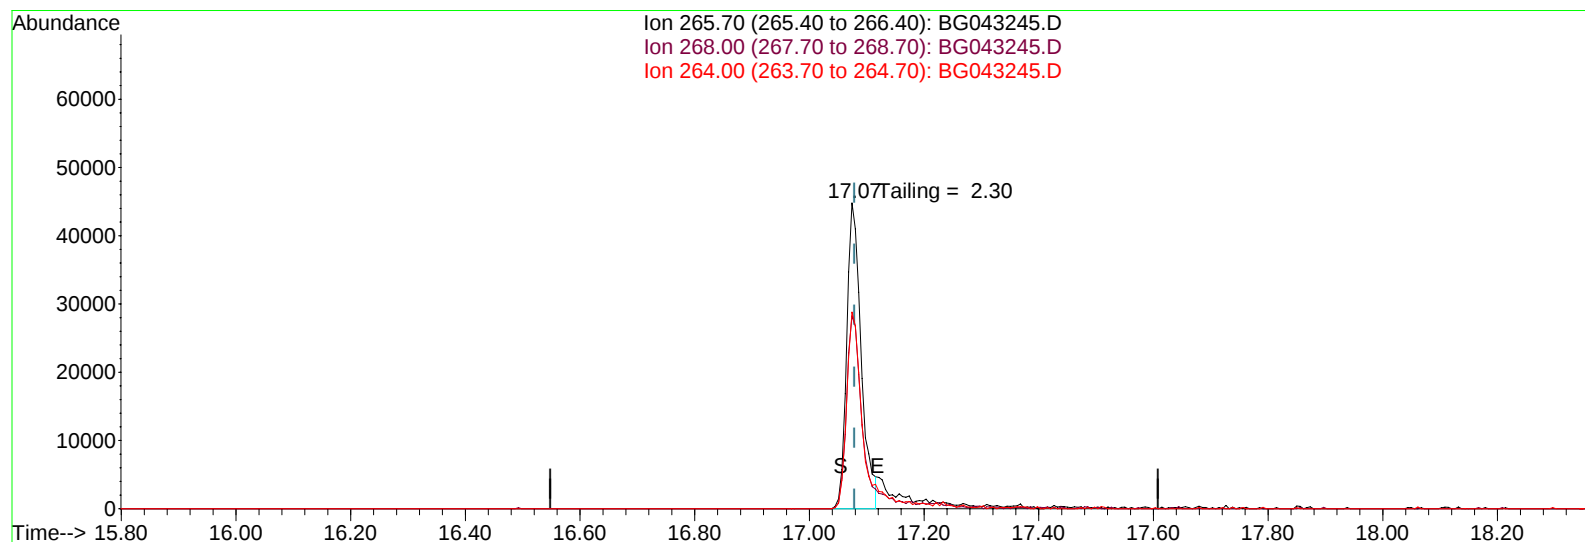

(70) Pentachlorophenol (C)




17.074min (-0.004) 20278.19ng

response 85029

Ion	Exp%	Act%
265.70	100	100
268.00	65.20	63.04
264.00	63.40	64.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101619\
Data File : BG043245.D
Acq On : 16 Oct 2019 14:24
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 18:29:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:11:45 2019
Response via : Initial Calibration

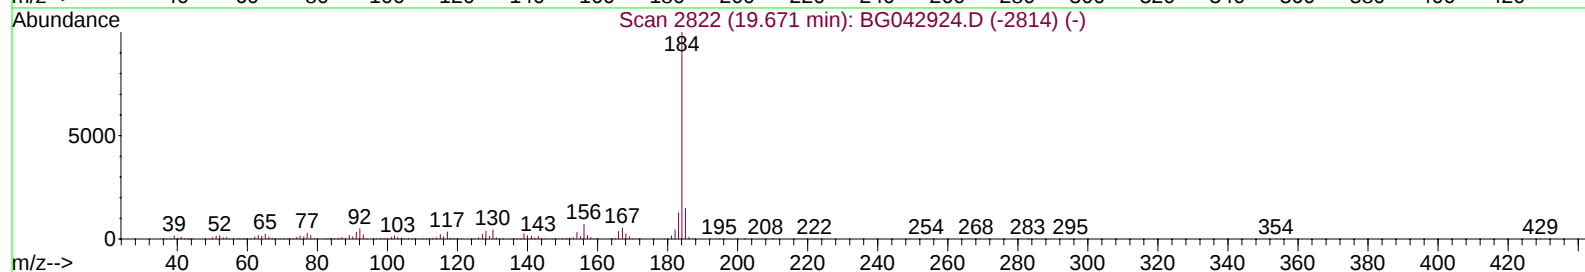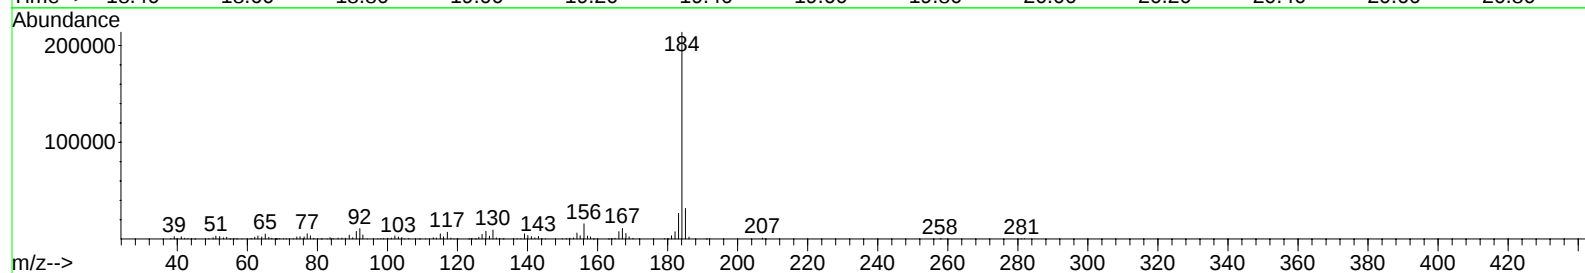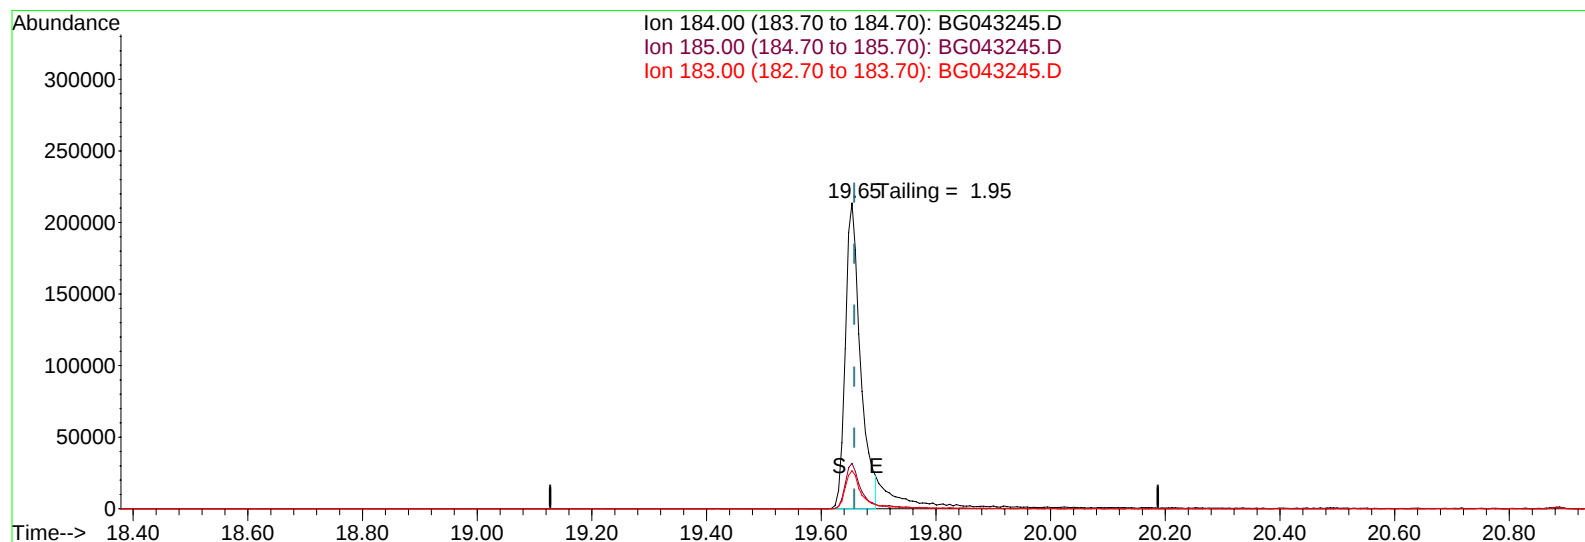

TIC: BG043245.D

(77) Benzidine

19.654min (-0.004) 312700.22ng

response 438463

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.85
183.00	12.60	12.46
0.00	0.00	0.00