


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101619\
 Data File : BG043245.D
 Acq On : 16 Oct 2019 14:24
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 09 01:11:45 2019

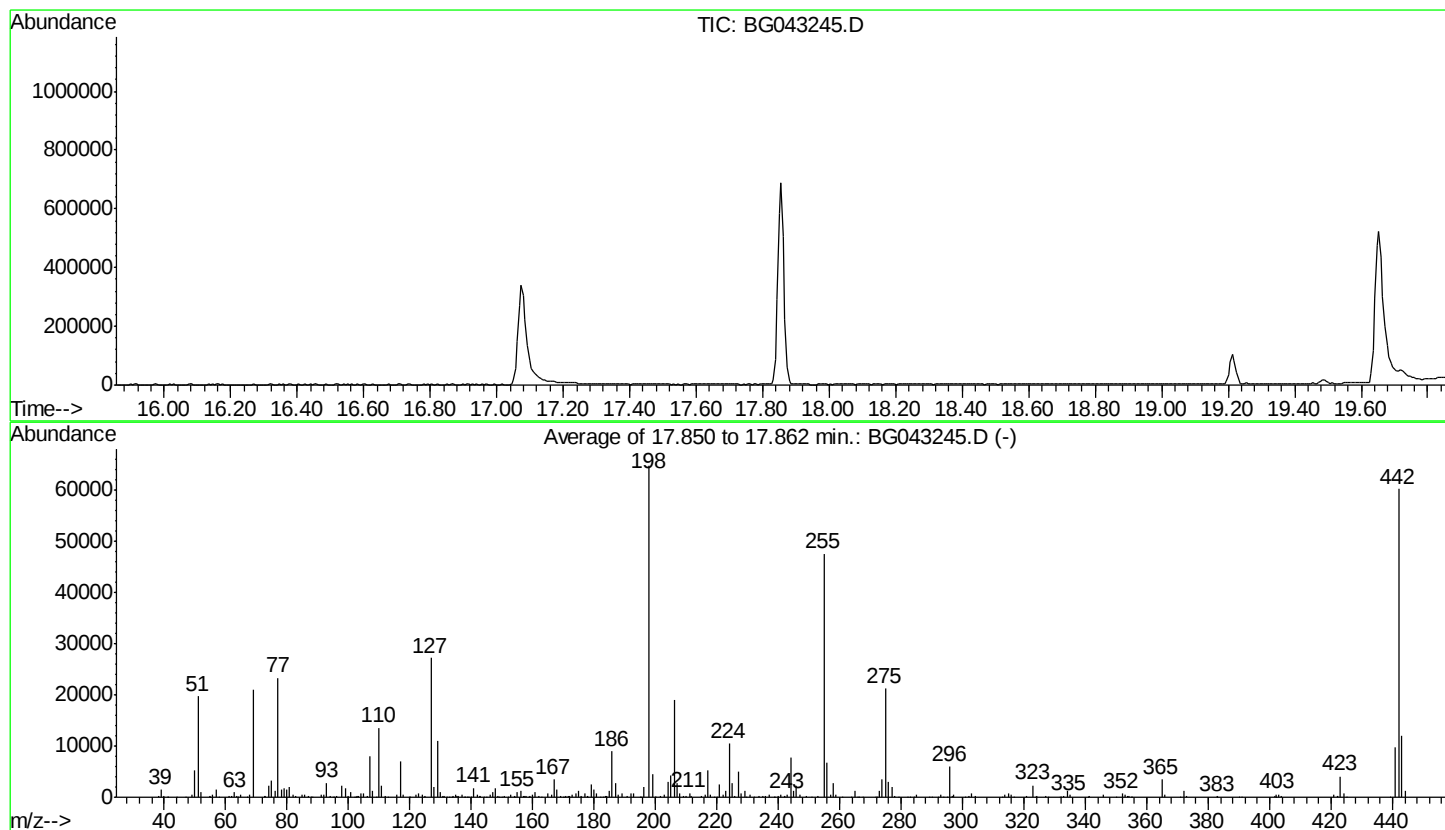

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	19726	PASS
68	69	0.00	2	2.0	412	PASS
69	198	0.00	100	32.6	21104	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.0	27181	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64725	PASS
199	198	5	9	6.9	4453	PASS
275	198	10	60	32.7	21154	PASS
365	198	1	100	5.2	3394	PASS
441	198	0.01	100	15.0	9684	PASS
442	198	50	100	92.9	60157	PASS
443	442	15	24	19.8	11928	PASS