

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101623\
 Data File : BG059450.D
 Acq On : 16 Oct 2023 10:04
 Operator : MA/JU
 Sample : PB156260BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.511	17	21	29	rVB4	14237	22715	1.58%	0.179%
2	3.664	46	47	50	rBV2	2494	2847	0.20%	0.022%
3	3.946	90	95	111	rBV	177890	293579	20.47%	2.313%
4	4.169	129	133	134	rBV4	2273	2906	0.20%	0.023%
5	4.234	142	144	149	rVB3	3003	3195	0.22%	0.025%
6	4.287	149	153	157	rBV4	3566	6427	0.45%	0.051%
7	4.352	161	164	167	rBV3	2550	3371	0.24%	0.027%
8	4.598	203	206	208	rVB3	3076	3356	0.23%	0.026%
9	4.622	208	210	213	rBV3	2466	3442	0.24%	0.027%
10	5.262	316	319	322	rVB2	2398	3321	0.23%	0.026%
11	5.497	355	359	361	rBV2	3248	3857	0.27%	0.030%
12	5.609	374	378	382	rVV2	2381	4377	0.31%	0.034%
13	5.773	403	406	409	rBV3	3615	3201	0.22%	0.025%
14	6.167	471	473	475	rVB2	3492	2913	0.20%	0.023%
15	6.426	515	517	519	rBV2	2967	3200	0.22%	0.025%
16	6.772	573	576	579	rBV2	2820	3127	0.22%	0.025%
17	7.066	625	626	630	rBV2	2439	3189	0.22%	0.025%
18	7.342	667	673	683	rVB	174422	300543	20.96%	2.368%
19	7.536	699	706	714	rVB	149250	241072	16.81%	1.899%
20	7.730	732	739	748	rBV	166853	295920	20.64%	2.332%
21	8.218	814	822	831	rBV	128446	220415	15.37%	1.737%
22	8.652	893	896	901	rBV2	1944	3038	0.21%	0.024%
23	8.911	933	940	950	rVV	202245	362947	25.31%	2.860%
24	9.322	1007	1010	1011	rBV	3420	2972	0.21%	0.023%
25	9.416	1018	1026	1036	rVV	167630	298435	20.81%	2.351%
26	10.133	1142	1148	1156	rVB2	122230	220472	15.37%	1.737%
27	10.662	1229	1238	1247	rBV2	189024	339961	23.71%	2.679%
28	11.061	1296	1306	1313	rVV	184195	331706	23.13%	2.614%
29	11.202	1323	1330	1340	rBV	214494	396263	27.63%	3.122%
30	11.431	1367	1369	1372	rBV	3208	2953	0.21%	0.023%
31	11.731	1416	1420	1422	rBV2	2293	3737	0.26%	0.029%
32	11.749	1422	1423	1428	rVV	3405	3454	0.24%	0.027%
33	11.901	1446	1449	1453	rBV	2124	3181	0.22%	0.025%
34	12.231	1502	1505	1507	rBV	3315	2961	0.21%	0.023%
35	12.354	1522	1526	1532	rVB	1820	3297	0.23%	0.026%
36	12.618	1570	1571	1577	rVB	4054	6166	0.43%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101623\
 Data File : BG059450.D
 Acq On : 16 Oct 2023 10:04
 Operator : MA/JU
 Sample : PB156260BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

37	12.759	1592	1595	1599	rBV	2432	4300	0.30%	0.034%
38	12.842	1606	1609	1614	rVB	1867	3370	0.24%	0.027%
39	13.212	1668	1672	1677	rBV	2001	3907	0.27%	0.031%
40	13.682	1749	1752	1760	rVB3	5029	9896	0.69%	0.078%

41	14.105	1822	1824	1827	rBV	3371	3470	0.24%	0.027%
42	14.252	1843	1849	1856	rBV	396706	581050	40.52%	4.578%
43	14.557	1892	1901	1910	rBV	446081	704015	49.09%	5.547%
44	14.857	1946	1952	1959	rVB2	288760	446393	31.13%	3.517%
45	15.045	1977	1984	1991	rBV2	165755	277872	19.38%	2.189%

46	15.521	2059	2065	2066	rVB	2642	3325	0.23%	0.026%
47	15.844	2113	2120	2130	rVB	587285	869503	60.63%	6.851%
48	15.956	2133	2139	2148	rVB	193091	279050	19.46%	2.199%
49	16.085	2155	2161	2168	rVV3	5175	7944	0.55%	0.063%
50	16.255	2187	2190	2194	rBV3	1877	3617	0.25%	0.028%

51	17.325	2368	2372	2375	rBV	3069	4310	0.30%	0.034%
52	17.607	2413	2420	2427	rVB	383213	583498	40.69%	4.597%
53	17.706	2430	2437	2445	rBV2	646014	1007682	70.27%	7.940%
54	18.987	2652	2655	2658	rBV2	2403	2963	0.21%	0.023%
55	19.087	2668	2672	2675	rVB	2819	4082	0.28%	0.032%

56	19.446	2727	2733	2737	rBV5	2559	4592	0.32%	0.036%
57	19.545	2745	2750	2754	rBV4	11431	17977	1.25%	0.142%
58	19.616	2758	2762	2763	rVV2	8261	12253	0.85%	0.097%
59	19.710	2775	2778	2782	rBV3	3410	5010	0.35%	0.039%
60	19.822	2794	2797	2802	rBV2	3935	6106	0.43%	0.048%

61	19.892	2808	2809	2815	rBV2	2580	3300	0.23%	0.026%
62	19.980	2818	2824	2832	rBV	927826	1295584	90.35%	10.208%
63	20.309	2878	2880	2882	rBV2	3468	3219	0.22%	0.025%
64	20.462	2903	2906	2908	rBV2	4535	3193	0.22%	0.025%
65	20.509	2912	2914	2917	rBV3	2621	3188	0.22%	0.025%

66	20.574	2924	2925	2927	rBV2	4388	3325	0.23%	0.026%
67	20.750	2953	2955	2957	rBV2	2590	3075	0.21%	0.024%
68	21.326	3051	3053	3054	rBV2	3362	3231	0.23%	0.025%
69	21.907	3145	3152	3161	rBV2	407651	717075	50.01%	5.650%
70	22.483	3248	3250	3252	rVB2	4632	3043	0.21%	0.024%

71	22.501	3252	3253	3255	rBV2	5269	4045	0.28%	0.032%
72	22.959	3329	3331	3334	rBV3	4318	3114	0.22%	0.025%
73	23.229	3375	3377	3379	rBV3	5626	3838	0.27%	0.030%
74	23.294	3386	3388	3390	rBV3	5203	3198	0.22%	0.025%
75	23.359	3396	3399	3400	rBV3	5650	6208	0.43%	0.049%

76	23.376	3400	3402	3408	rVB6	10890	16636	1.16%	0.131%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101623\
 Data File : BG059450.D
 Acq On : 16 Oct 2023 10:04
 Operator : MA/JU
 Sample : PB156260BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
 Title : SVOA CALIBRATION

77	23.482	3418	3420	3423	rBV4	4490	4490	0.31%	0.035%
78	23.823	3476	3478	3479	rBV2	4091	2976	0.21%	0.023%
79	24.146	3531	3533	3534	rBV2	5975	3251	0.23%	0.026%
80	24.240	3544	3549	3554	rVB8	12128	25059	1.75%	0.197%
81	24.316	3560	3562	3563	rBV2	6227	4675	0.33%	0.037%
82	24.451	3583	3585	3587	rVB3	7400	4665	0.33%	0.037%
83	25.145	3692	3703	3715	rBV2	504017	1434005	100.00%	11.299%
84	25.392	3734	3745	3757	rVB3	263210	768990	53.63%	6.059%
85	26.473	3921	3929	3935	rBV8	18266	52277	3.65%	0.412%
86	26.761	3976	3978	3980	rBV2	4333	4208	0.29%	0.033%
87	27.025	4021	4023	4025	rVB	6686	3084	0.22%	0.024%
88	27.571	4114	4116	4118	rBV2	4366	3495	0.24%	0.028%
89	28.570	4285	4286	4287	rBV	5911	3794	0.26%	0.030%
90	29.164	4385	4387	4389	rVB3	5517	4795	0.33%	0.038%
91	29.310	4410	4412	4415	rBV3	5229	5008	0.35%	0.039%
92	29.334	4415	4416	4420	rVV3	5632	4812	0.34%	0.038%
93	29.951	4519	4521	4522	rBV2	4372	3041	0.21%	0.024%
94	30.204	4562	4564	4566	rBV2	4403	2993	0.21%	0.024%
95	30.327	4582	4585	4586	rBV3	4819	4076	0.28%	0.032%
96	30.656	4640	4641	4644	rVB3	5583	3625	0.25%	0.029%
97	31.044	4705	4707	4708	rBV2	6262	3385	0.24%	0.027%
98	31.379	4762	4764	4767	rBV4	4842	5136	0.36%	0.040%
99	31.954	4860	4862	4865	rBV4	6692	6259	0.44%	0.049%
100	32.471	4948	4950	4952	rBV2	4093	3790	0.26%	0.030%




Sum of corrected areas: 12691862

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101623\
Data File : BG059450.D
Acq On : 16 Oct 2023 10:04
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

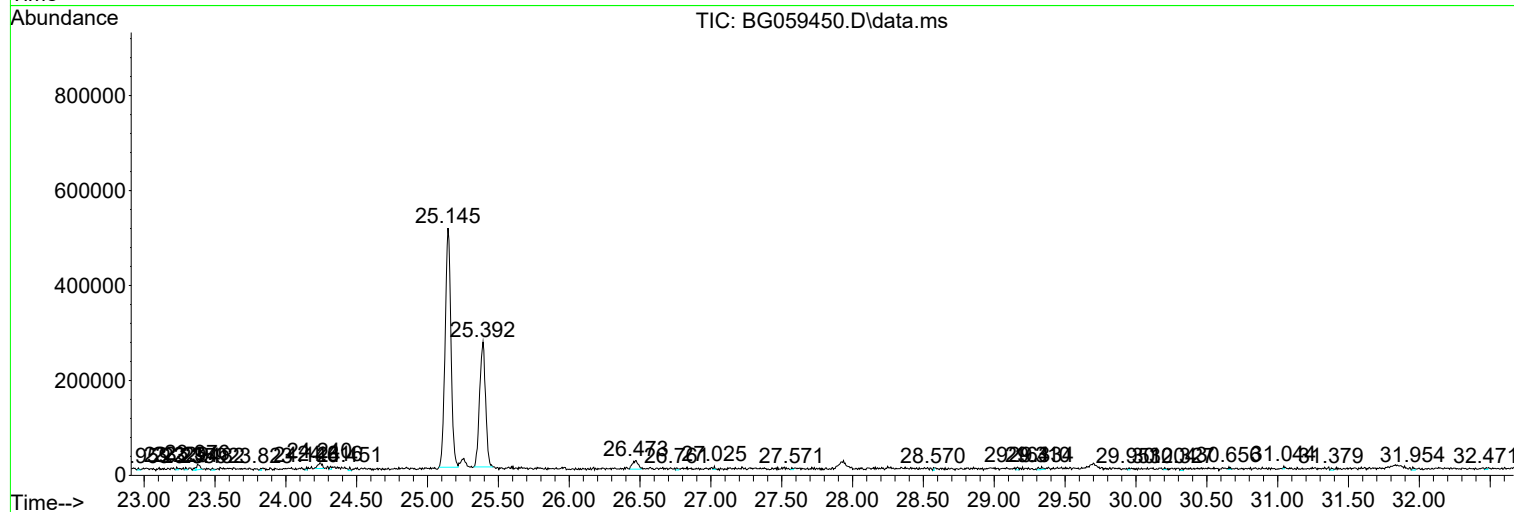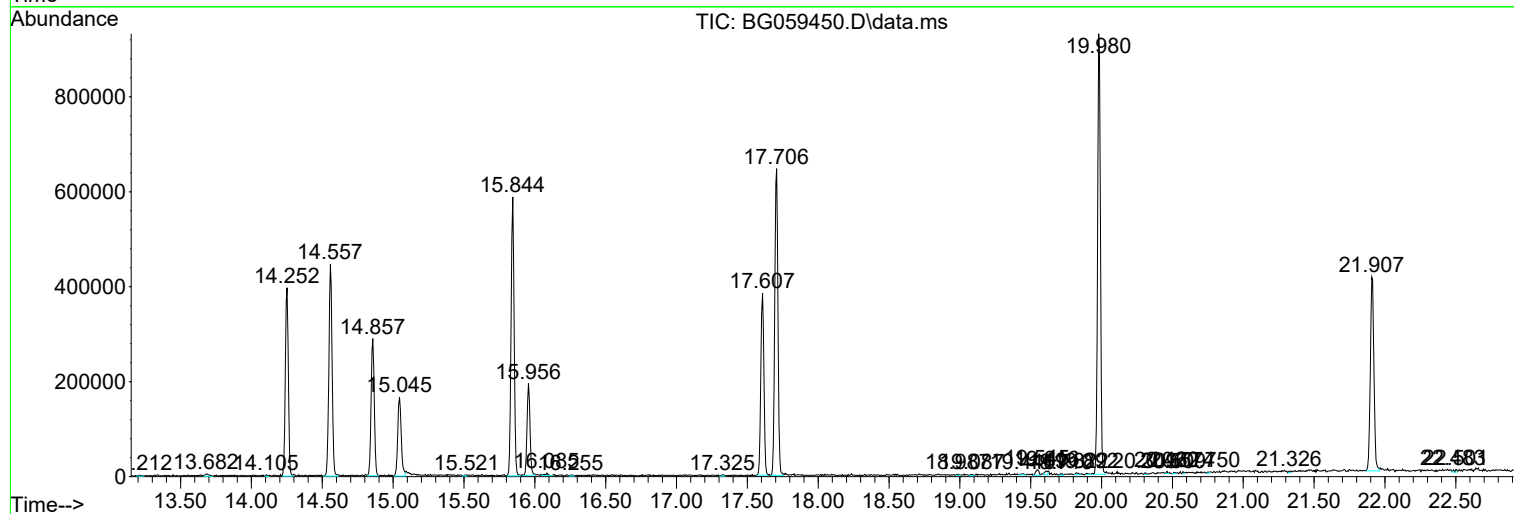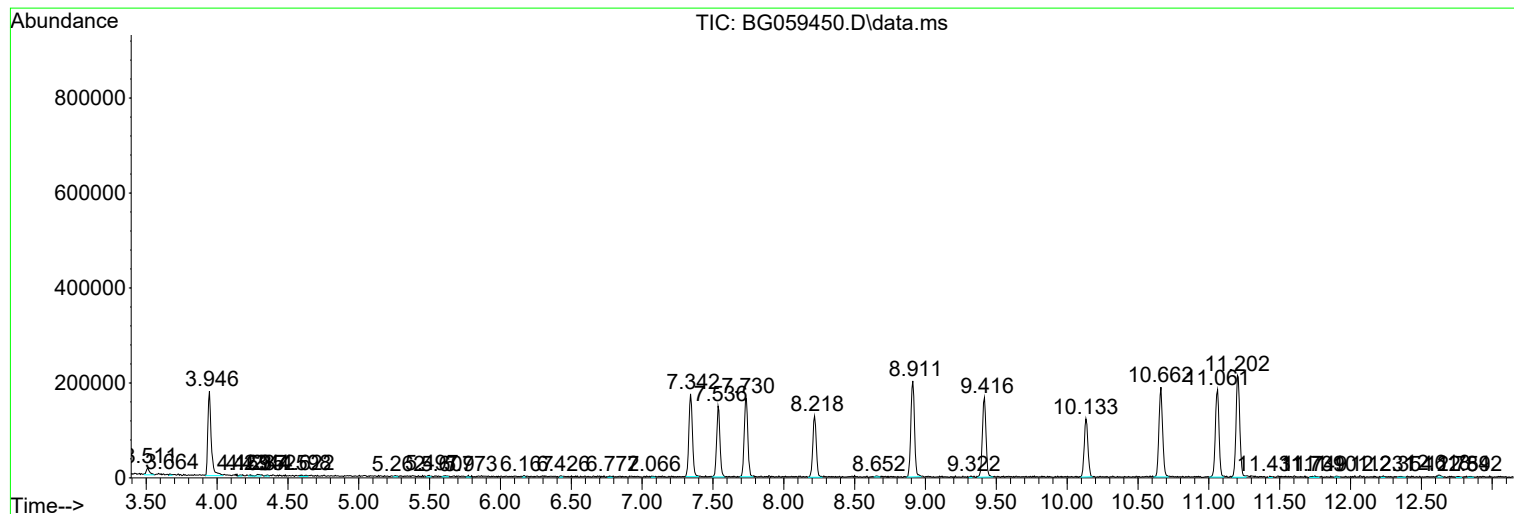

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101623\
Data File : BG059450.D
Acq On : 16 Oct 2023 10:04
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101623\
Data File : BG059450.D
Acq On : 16 Oct 2023 10:04
Operator : MA/JU
Sample : PB156260BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------