

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101723\
 Data File : BG059468.D
 Acq On : 17 Oct 2023 21:43
 Operator : MA/JU
 Sample : SST08053
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST080417

Quant Time: Oct 18 03:57:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 18 03:51:17 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.188	152	26557	20.000	ng/u1	0.00
20) Naphthalene-d8	11.032	136	117048	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.827	164	70483	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.577	188	161911	20.000	ng/u1	0.00
79) Chrysene-d12	21.878	240	158858	20.000	ng/u1	0.00
88) Perylene-d12	25.321	264	185281	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.482	96	23389	28.757	ng/uL	0.00
4) Pyridine-d5	3.916	84	275455	112.004	ng/u1	0.00
7) Phenol-d5	7.318	99	214265	74.200	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.512	67	118235	72.440	ng/u1	0.00
11) 2-Chlorophenol-d4	7.712	132	164804	79.779	ng/u1	0.00
15) 4-Methylphenol-d8	8.893	113	162168	74.422	ng/u1	0.00
21) Nitrobenzene-d5	9.392	128	80823	83.929	ng/u1	0.00
24) 2-Nitrophenol-d4	10.109	143	86259	91.471	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.638	165	157394	79.554	ng/u1	0.00
31) 4-Chloroaniline-d4	11.178	131	238991	77.291	ng/u1	0.00
46) Dimethylphthalate-d6	14.228	166	466762	78.263	ng/u1	0.00
49) Acenaphthylene-d8	14.533	160	512619	70.684	ng/u1	0.00
54) 4-Nitrophenol-d4	15.033	143	90457	86.687	ng/u1	0.01
60) Fluorene-d10	15.820	176	436823	77.019	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.938	200	89109	90.632	ng/u1	0.00
73) Anthracene-d10	17.683	188	676365	80.986	ng/u1	0.00
81) Pyrene-d10	19.956	212	764803	78.142	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.086	264	811111	78.900	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.517	88	26377	25.790	ng/uL	96
5) Pyridine	3.934	79	281771	117.344	ng/u1	94
6) Benzaldehyde	7.336	77	80681	63.856	ng/u1	95
8) Phenol	7.348	94	209016	73.159	ng/u1	92
10) Bis(2-Chloroethyl)ether	7.606	93	160859	70.732	ng/u1	94
12) 2-Chlorophenol	7.741	128	164491	76.634	ng/u1	98
13) 2-Methylphenol	8.623	108	155102	73.934	ng/u1	89
14) 2,2'-oxybis(1-Chloropr...	8.699	45	334714	71.642	ng/u1#	96
16) Acetophenone	9.040	105	239825	72.884	ng/u1	97
17) N-Nitroso-di-n-propyla...	9.010	70	111671	73.705	ng/u1	93
18) 4-Methylphenol	8.958	108	167575	73.481	ng/u1	90
19) Hexachloroethane	9.275	117	60637	74.333	ng/u1	87
22) Nitrobenzene	9.433	77	169571	78.639	ng/u1	99
23) Isophorone	9.945	82	344046	75.970	ng/u1	95
25) 2-Nitrophenol	10.144	139	90394	86.978	ng/u1	96
26) 2,4-Dimethylphenol	10.174	107	163055	76.582	ng/u1	94
27) Bis(2-Chloroethoxy)met...	10.426	93	216428	74.306	ng/u1	97
29) 2,4-Dichlorophenol	10.661	162	156124	81.653	ng/u1#	85
30) Naphthalene	11.084	128	539334	75.915	ng/u1	97
32) 4-Chloroaniline	11.208	127	219904	74.714	ng/u1	90
33) Hexachlorobutadiene	11.308	225	98641	78.245	ng/u1	99
34) Caprolactam	12.054	113	7889	11.964	ng/u1	90
35) 4-Chloro-3-methylphenol	12.289	107	149790	78.303	ng/u1	91
36) 2-Methylnaphthalene	12.671	142	349668	77.120	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101723\
 Data File : BG059468.D
 Acq On : 17 Oct 2023 21:43
 Operator : MA/JU
 Sample : SSTD08053
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD080417

Quant Time: Oct 18 03:57:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 18 03:51:17 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.888	142	351282	75.378	ng/ul#	100
39) 1,2,4,5-Tetrachloroben...	13.017	216	184462	79.786	ng/ul	97
40) Hexachlorocyclopentadiene	12.970	237	116509	86.996	ng/ul	92
41) 2,4,6-Trichlorophenol	13.264	196	120794	85.665	ng/ul	95
42) 2,4,5-Trichlorophenol	13.335	196	125818	82.045	ng/ul	97
43) 1,1'-Biphenyl	13.670	154	494821	77.633	ng/ul	98
44) 2-Chloronaphthalene	13.723	162	378309	77.248	ng/ul	97
45) 2-Nitroaniline	13.946	65	110698	85.679	ng/ul	95
47) Dimethylphthalate	14.275	163	471638	79.056	ng/ul	97
48) 2,6-Dinitrotoluene	14.422	165	94531	86.505	ng/ul	97
50) Acenaphthylene	14.563	152	599951	78.592	ng/ul	99
51) 3-Nitroaniline	14.762	138	99338	83.938	ng/ul#	89
52) Acenaphthene	14.898	153	413393	78.647	ng/ul	96
53) 2,4-Dinitrophenol	14.962	184	57198	96.389	ng/ul	95
55) 4-Nitrophenol	15.050	109	63207	84.388	ng/ul	91
56) Dibenzofuran	15.227	168	551988	77.250	ng/ul	98
57) 2,4-Dinitrotoluene	15.203	165	138486	87.629	ng/ul#	92
58) 2,3,4,6-Tetrachlorophenol	15.438	232	118119	84.996	ng/ul#	93
59) Diethylphthalate	15.620	149	450688	77.898	ng/ul	97
61) Fluorene	15.879	166	458297	77.567	ng/ul	89
62) 4-Chlorophenyl-phenyle...	15.855	204	232784	77.371	ng/ul	97
63) 4-Nitroaniline	15.932	138	91581	78.741	ng/ul#	81
66) 4,6-Dinitro-2-methylph...	15.955	198	91112	87.514	ng/ul#	90
67) N-Nitrosodiphenylamine	16.079	169	385273	80.444	ng/ul	95
68) 4-Bromophenyl-phenylether	16.754	248	135595	76.805	ng/ul	93
69) Hexachlorobenzene	16.848	284	156458	77.553	ng/ul	94
70) Atrazine	17.019	200	141547	75.913	ng/ul	95
71) Pentachlorophenol	17.207	266	99096	86.334	ng/ul	90
72) Phenanthrene	17.624	178	793612	78.626	ng/ul	98
74) Anthracene	17.718	178	816494	78.894	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.629	216	183278	78.401	ng/uL	96
76) Pentachlorobenzene	15.121	250	178999	78.570	ng/uL	94
77) Carbazole	17.994	167	694836	77.638	ng/ul#	96
78) Di-n-butylphthalate	18.493	149	820239	81.299	ng/ul	98
80) Fluoranthene	19.622	202	941443	80.708	ng/ul	97
82) Pyrene	19.986	202	977041	77.995	ng/ul	99
83) Butylbenzylphthalate	20.838	149	366322	86.791	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.772	252	330169	79.411	ng/ul	98
85) Benzo(a)anthracene	21.854	228	984881	78.409	ng/ul	96
86) Bis(2-ethylhexyl)phtha...	21.684	149	541488	88.013	ng/ul	97
87) Chrysene	21.925	228	914294	77.157	ng/ul	98
89) Di-n-octyl phthalate	22.965	149	946192	87.179	ng/ul	100
90) Benzo(b)fluoranthene	24.210	252	1006127	80.295	ng/ul	97
91) Benzo(k)fluoranthene	24.287	252	1018481	79.949	ng/ul	99
93) Benzo(a)pyrene	25.168	252	962507	79.206	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	29.304	276	1110015	81.322	ng/ul	99
95) Dibenzo(a,h)anthracene	29.381	278	495226	43.606	ng/ul	100
96) Benzo(g,h,i)perylene	30.591	276	1123118	100.683	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101723\
 Data File : BG059468.D
 Acq On : 17 Oct 2023 21:43
 Operator : MA/JU
 Sample : SST08053
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST080417

Quant Time: Oct 18 03:57:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG101723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 18 03:51:17 2023
 Response via : Initial Calibration




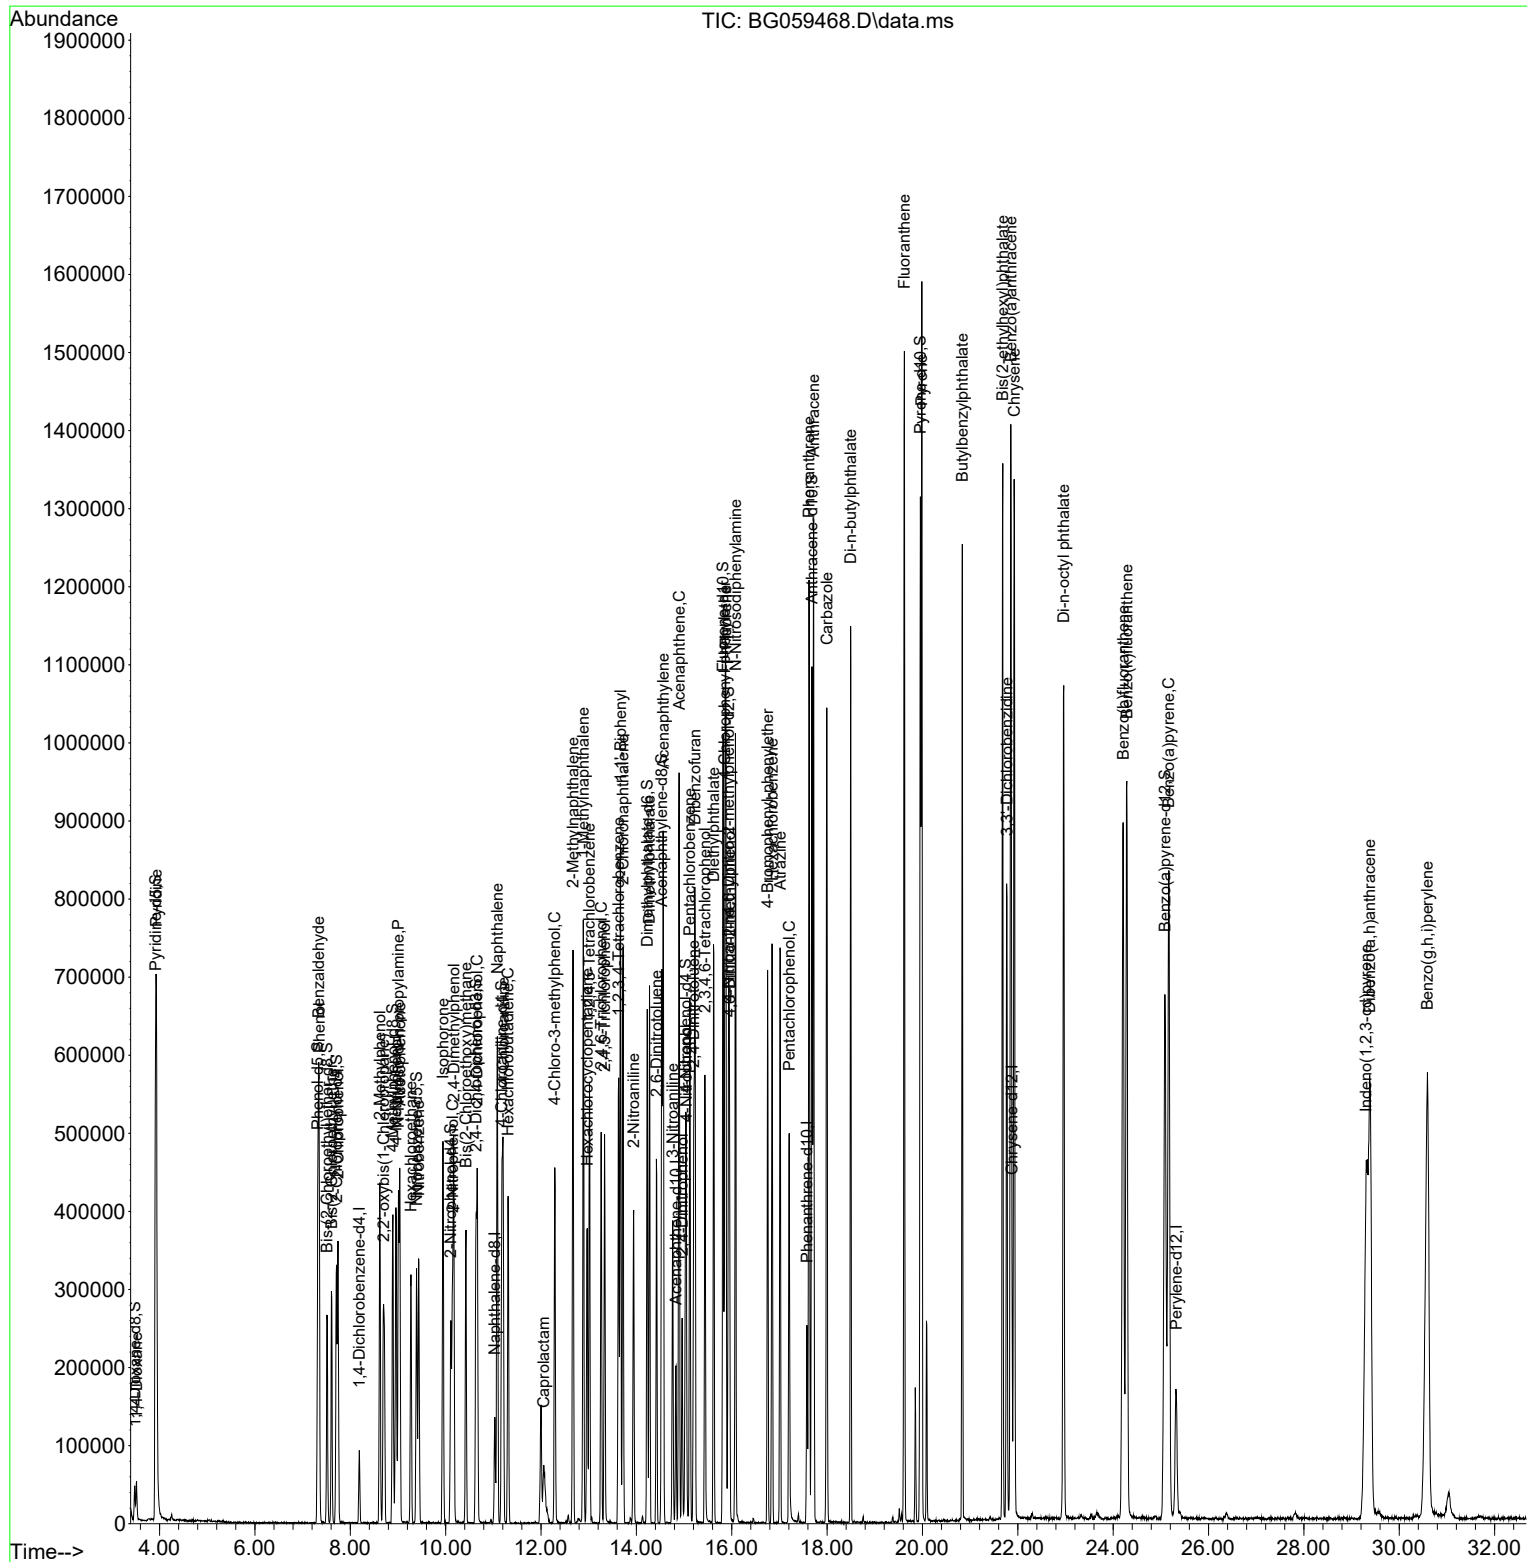




#2
1,4-Dioxane
Concen: 25.790 ng/uL
RT: 3.517 min Scan# 21
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion: 88 Resp: 26377
Ion Ratio Lower Upper
88 100
43 33.7 30.8 46.2
58 79.4 65.0 97.4

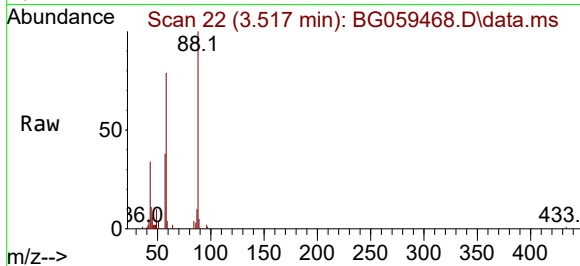

#5
Pyridine
Concen: 117.344 ng/uL
RT: 3.934 min Scan# 93
Delta R.T. -0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion: 79 Resp: 281771
Ion Ratio Lower Upper
79 100
52 106.0 80.9 121.3
51 50.4 45.0 67.4




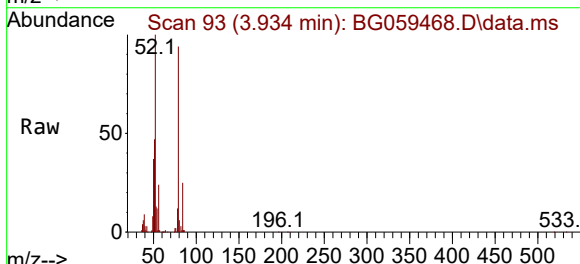




#6
Benzaldehyde
Concen: 63.856 ng/ul
RT: 7.336 min Scan# 671
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion: 77 Resp: 80681
Ion Ratio Lower Upper
77 100
105 110.2 83.0 124.6
106 100.0 82.8 124.2



#8
Phenol
Concen: 73.159 ng/ul
RT: 7.348 min Scan# 674
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion: 94 Resp: 209016
Ion Ratio Lower Upper
94 100
65 27.7 19.7 29.5
66 35.8 24.5 36.7



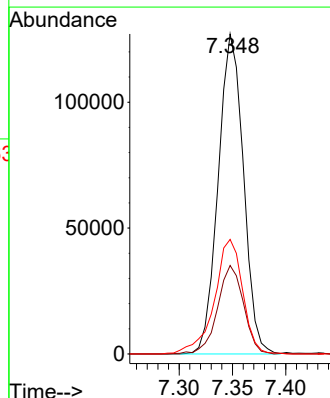





#10
Bis(2-Chloroethyl)ether
Concen: 70.732 ng/ul
RT: 7.606 min Scan# 718
Delta R.T. -0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion: 93 Resp: 160859
Ion Ratio Lower Upper
93 100
63 81.0 60.0 90.0
95 32.2 27.6 41.4

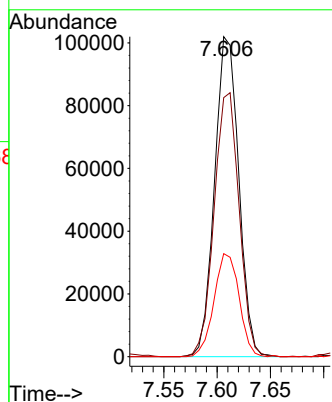

#12
2-Chlorophenol
Concen: 76.634 ng/ul
RT: 7.741 min Scan# 741
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:128 Resp: 164491
Ion Ratio Lower Upper
128 100
64 46.3 36.8 55.2
130 31.0 26.6 40.0









#13
2-Methylphenol
Concen: 73.934 ng/ul
RT: 8.623 min Scan# 890
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:108 Resp: 155102
Ion Ratio Lower Upper
108 100
107 90.3 64.4 96.6



#14
2,2'-oxybis(1-Chloropropane)
Concen: 71.642 ng/ul
RT: 8.699 min Scan# 904
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion: 45 Resp: 334714
Ion Ratio Lower Upper
45 100
77 8.8 6.4 9.6
79 6.3 6.4 9.6#



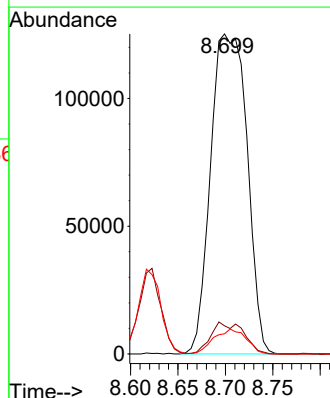





#16
Acetophenone
Concen: 72.884 ng/ul
RT: 9.040 min Scan# 90
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:105 Resp: 239825
Ion Ratio Lower Upper
105 100
77 70.5 55.4 83.0
51 36.7 31.6 47.4



#17
N-Nitroso-di-n-propylamine
Concen: 73.705 ng/ul
RT: 9.010 min Scan# 957
Delta R.T. 0.014 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion: 70 Resp: 111671
Ion Ratio Lower Upper
70 100
42 85.4 62.1 93.1
101 9.5 7.3 10.9
130 22.7 18.6 28.0









#18
4-Methylphenol
Concen: 73.481 ng/ul
RT: 8.958 min Scan# 94
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:108 Resp: 167575
Ion Ratio Lower Upper
108 100
107 108.2 78.7 118.1

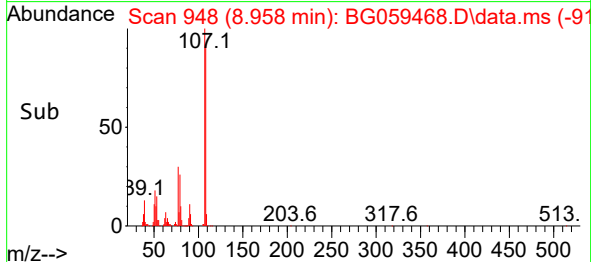

#19
Hexachloroethane
Concen: 74.333 ng/ul
RT: 9.275 min Scan# 1002
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:117 Resp: 60637
Ion Ratio Lower Upper
117 100
201 109.5 76.1 114.1
199 72.5 65.0 97.4









#22
Nitrobenzene
Concen: 78.639 ng/ul
RT: 9.433 min Scan# 1109
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion: 77 Resp: 169571
Ion Ratio Lower Upper
77 100
123 49.2 38.5 57.7
65 14.1 11.1 16.7



#23
Isophorone
Concen: 75.970 ng/ul
RT: 9.945 min Scan# 1116
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion: 82 Resp: 344046
Ion Ratio Lower Upper
82 100
95 6.4 5.6 8.4
138 18.9 13.0 19.6









#25
2-Nitrophenol
Concen: 86.978 ng/ul
RT: 10.144 min Scan# 1149
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:139 Resp: 90394
Ion Ratio Lower Upper
139 100
65 53.4 40.5 60.7
109 29.4 25.7 38.5

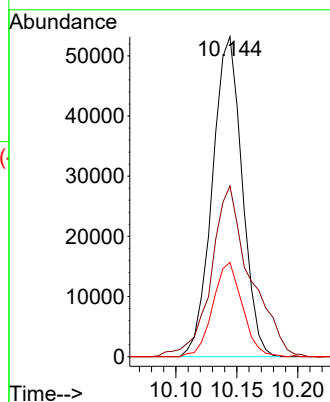

#26
2,4-Dimethylphenol
Concen: 76.582 ng/ul
RT: 10.174 min Scan# 1155
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:107 Resp: 163055
Ion Ratio Lower Upper
107 100
121 52.3 44.9 67.3
122 93.6 69.6 104.4









#27
 Bis(2-Chloroethoxy)methane
 Concen: 74.306 ng/ul
 RT: 10.426 min Scan# 1197
 Delta R.T. 0.003 min
 Lab File: BG059468.D
 Acq: 17 Oct 2023 21:43




Instrument :
 BNA_G
 ClientSampleId :
 SSTD080417


Tgt Ion: 93 Resp: 216428
 Ion Ratio Lower Upper
 93 100
 95 32.1 24.8 37.2
 123 9.6 9.1 13.7



#29
 2,4-Dichlorophenol
 Concen: 81.653 ng/ul
 RT: 10.661 min Scan# 1238
 Delta R.T. 0.003 min
 Lab File: BG059468.D
 Acq: 17 Oct 2023 21:43

Tgt Ion:162 Resp: 156124
 Ion Ratio Lower Upper
 162 100
 164 63.7 40.9 61.3#
 98 33.0 22.2 33.4





#30

Naphthalene

Concen: 75.915 ng/ul

RT: 11.084 min Scan# 11

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Instrument :

BNA_G

ClientSampleId :

SSTD080417





Tgt Ion:128 Resp: 539334

Ion Ratio Lower Upper

128 100

129 11.6 8.0 12.0

127 12.5 9.5 14.3

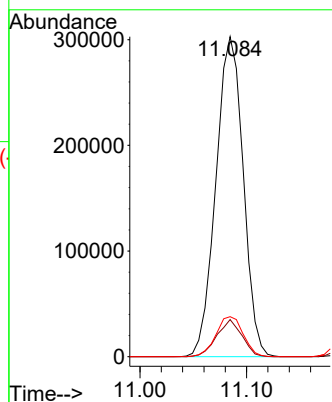

#32

4-Chloroaniline

Concen: 74.714 ng/ul

RT: 11.208 min Scan# 1331

Delta R.T. 0.009 min

Lab File: BG059468.D




Acq: 17 Oct 2023 21:43


Tgt Ion:127 Resp: 219904

Ion Ratio Lower Upper

127 100

129 32.5 21.9 32.9









#33
Hexachlorobutadiene
Concen: 78.245 ng/ul
RT: 11.308 min Scan# 11
Delta R.T. -0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:225 Resp: 98641
Ion Ratio Lower Upper
225 100
223 63.0 48.7 73.1
227 63.2 50.5 75.7

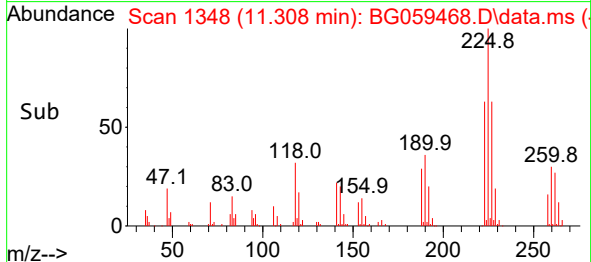

#34
Caprolactam
Concen: 11.964 ng/ul
RT: 12.054 min Scan# 1475
Delta R.T. 0.073 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:113 Resp: 7889
Ion Ratio Lower Upper
113 100
55 233.3 191.8 287.6
56 163.3 109.6 164.4









#35
4-Chloro-3-methylphenol
Concen: 78.303 ng/ul
RT: 12.289 min Scan# 1
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:107 Resp: 149790
Ion Ratio Lower Upper
107 100
144 27.5 22.5 33.7
142 85.6 60.6 90.8

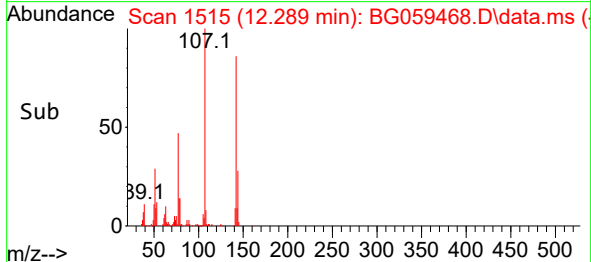

#36
2-Methylnaphthalene
Concen: 77.120 ng/ul
RT: 12.671 min Scan# 1580
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:142 Resp: 349668
Ion Ratio Lower Upper
142 100
141 88.4 69.4 104.0





#37

1-Methylnaphthalene

Concen: 75.378 ng/ul

RT: 12.888 min Scan# 1

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Instrument :

BNA_G

ClientSampleId :

SSTD080417





Tgt Ion:142 Resp: 351282

Ion Ratio Lower Upper

142 100

141 91.8 73.4 110.2

116 3.4 3.8 5.6#



#39

1,2,4,5-Tetrachlorobenzene

Concen: 79.786 ng/ul

RT: 13.017 min Scan# 1639

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Tgt Ion:216 Resp: 184462




Ion Ratio Lower Upper


216 100

214 81.2 62.8 94.2

179 19.8 16.4 24.6

108 15.7 15.1 22.7



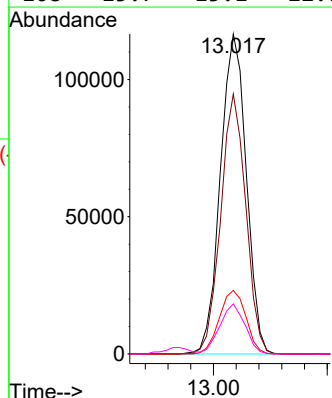





#40
 Hexachlorocyclopentadiene
 Concen: 86.996 ng/ul
 RT: 12.970 min Scan# 1631
 Delta R.T. 0.003 min
 Lab File: BG059468.D
 Acq: 17 Oct 2023 21:43




Instrument :
 BNA_G
 ClientSampleId :
 SSTD080417


Tgt Ion:237 Resp: 116509
 Ion Ratio Lower Upper
 237 100
 235 64.5 46.2 69.2
 272 12.5 10.9 16.3

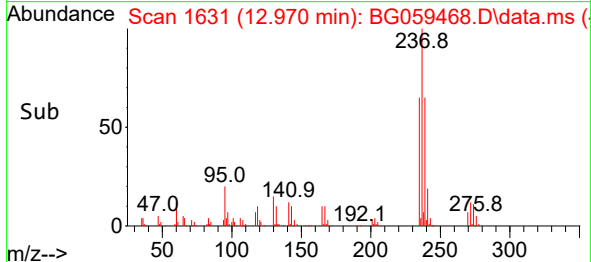

#41
 2,4,6-Trichlorophenol
 Concen: 85.665 ng/ul
 RT: 13.264 min Scan# 1681
 Delta R.T. 0.003 min
 Lab File: BG059468.D
 Acq: 17 Oct 2023 21:43

Tgt Ion:196 Resp: 120794
 Ion Ratio Lower Upper
 196 100
 198 107.5 81.2 121.8
 200 35.6 29.8 44.6





#42

2,4,5-Trichlorophenol

Concen: 82.045 ng/ul

RT: 13.335 min Scan# 1

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Instrument :

BNA_G

ClientSampleId :

SSTD080417





Tgt Ion:196 Resp: 125818

Ion Ratio Lower Upper

196 100

198 102.9 81.0 121.6

200 34.5 25.0 37.6

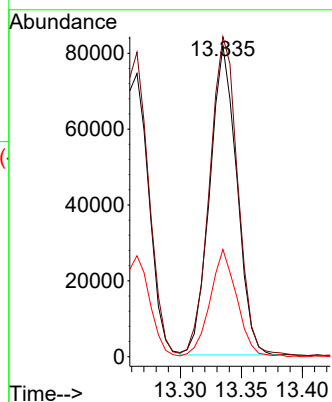

#43

1,1'-Biphenyl

Concen: 77.633 ng/ul

RT: 13.670 min Scan# 1750

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43




Tgt Ion:154 Resp: 494821


Ion Ratio Lower Upper

154 100

153 37.0 30.3 45.5

76 10.8 9.4 14.0









#44
2-Chloronaphthalene
Concen: 77.248 ng/ul
RT: 13.723 min Scan# 1758
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:162 Resp: 378309
Ion Ratio Lower Upper
162 100
164 31.8 28.0 42.0
127 35.1 27.7 41.5



#45
2-Nitroaniline
Concen: 85.679 ng/ul
RT: 13.946 min Scan# 1797
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion: 65 Resp: 110698
Ion Ratio Lower Upper
65 100
92 68.1 47.0 70.4
138 113.8 89.8 134.8









#47
Dimethylphthalate
Concen: 79.056 ng/ul
RT: 14.275 min Scan# 1853
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:163 Resp: 471638
Ion Ratio Lower Upper
163 100
194 3.3 3.1 4.7
164 10.3 7.3 10.9

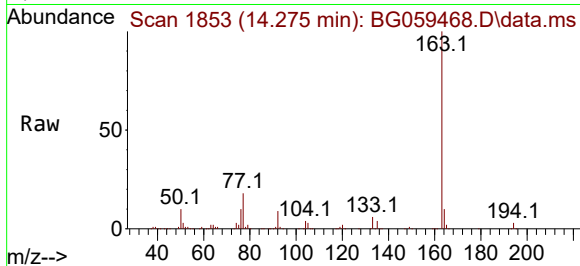

#48
2,6-Dinitrotoluene
Concen: 86.505 ng/ul
RT: 14.422 min Scan# 1878
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:165 Resp: 94531
Ion Ratio Lower Upper
165 100
89 58.0 45.3 67.9
121 19.4 17.4 26.0




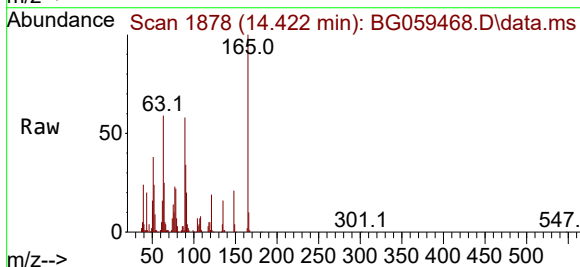




#50
Acenaphthylene
Concen: 78.592 ng/ul
RT: 14.563 min Scan# 1901
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:152 Resp: 599951
Ion Ratio Lower Upper
152 100
151 18.1 14.5 21.7
153 13.8 10.4 15.6

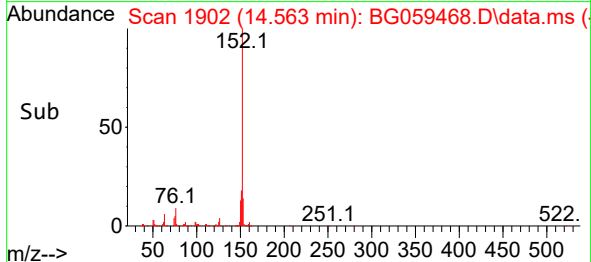

#51
3-Nitroaniline
Concen: 83.938 ng/ul
RT: 14.762 min Scan# 1936
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:138 Resp: 99338
Ion Ratio Lower Upper
138 100
108 8.0 5.3 7.9#
92 104.1 74.4 111.6









#52
Acenaphthene
Concen: 78.647 ng/ul
RT: 14.898 min Scan# 1958
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:153 Resp: 413393
Ion Ratio Lower Upper
153 100
152 44.2 40.0 60.0
154 87.8 72.0 108.0

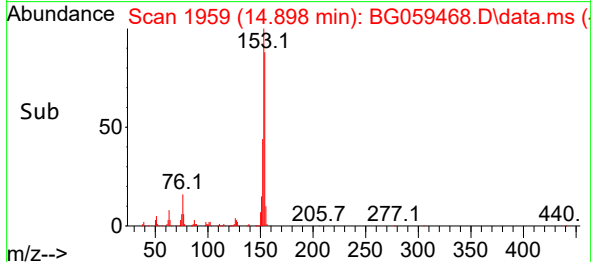

#53
2,4-Dinitrophenol
Concen: 96.389 ng/ul
RT: 14.962 min Scan# 1970
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:184 Resp: 57198
Ion Ratio Lower Upper
184 100
63 56.0 43.0 64.6
154 56.4 48.9 73.3









#55
4-Nitrophenol
Concen: 84.388 ng/ul
RT: 15.050 min Scan# 1982
Delta R.T. 0.014 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:109 Resp: 63207
Ion Ratio Lower Upper
109 100
139 150.6 109.6 164.4
65 143.0 121.4 182.0

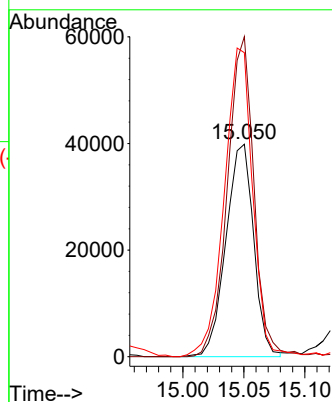

#56
Dibenzofuran
Concen: 77.250 ng/ul
RT: 15.227 min Scan# 2015
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:168 Resp: 551988
Ion Ratio Lower Upper
168 100
139 32.3 27.0 40.4

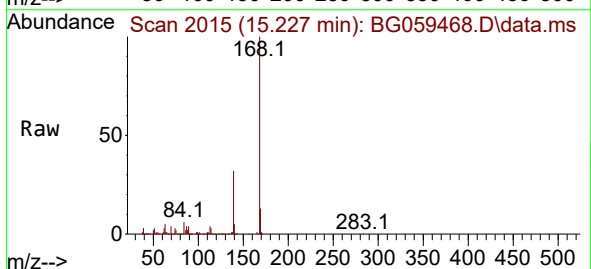



#57

2,4-Dinitrotoluene

Concen: 87.629 ng/ul

RT: 15.203 min Scan# 2011

Delta R.T. 0.009 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Instrument :

BNA_G

ClientSampleId :

SSTD080417





Tgt Ion:165 Resp: 138486

Ion Ratio Lower Upper

165 100

63 46.0 41.1 61.7

182 1.6 3.0 4.4#

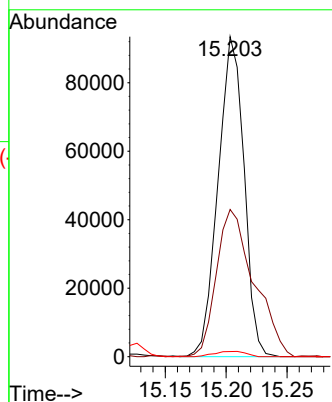

#58

2,3,4,6-Tetrachlorophenol

Concen: 84.996 ng/ul

RT: 15.438 min Scan# 2051

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Tgt Ion:232 Resp: 118119




Ion Ratio Lower Upper


232 100

131 37.7 28.6 43.0

130 2.2 2.2 3.2

166 28.8 18.2 27.2#


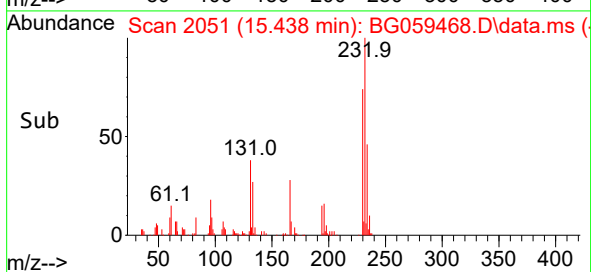






#59
Diethylphthalate
Concen: 77.898 ng/ul
RT: 15.620 min Scan# 2081
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:149 Resp: 450688
Ion Ratio Lower Upper
149 100
177 24.7 18.2 27.2
150 11.5 9.9 14.9



#61
Fluorene
Concen: 77.567 ng/ul
RT: 15.879 min Scan# 2126
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:166 Resp: 458297
Ion Ratio Lower Upper
166 100
165 94.9 85.6 128.4
167 13.0 9.8 14.8









#62
4-Chlorophenyl-phenylether
Concen: 77.371 ng/ul
RT: 15.855 min Scan# 2122
Delta R.T. -0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:204 Resp: 232784
Ion Ratio Lower Upper
204 100
206 32.4 25.7 38.5
141 50.1 37.6 56.4

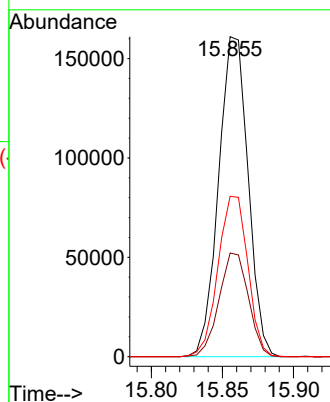

#63
4-Nitroaniline
Concen: 78.741 ng/ul
RT: 15.932 min Scan# 2135
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:138 Resp: 91581
Ion Ratio Lower Upper
138 100
92 50.0 33.3 49.9#
108 88.0 55.4 83.2#









#66
4,6-Dinitro-2-methylphenol
Concen: 87.514 ng/ul
RT: 15.955 min Scan# 2139
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:198 Resp: 91112
Ion Ratio Lower Upper
198 100
182 3.1 2.7 4.1
77 21.2 13.0 19.6#

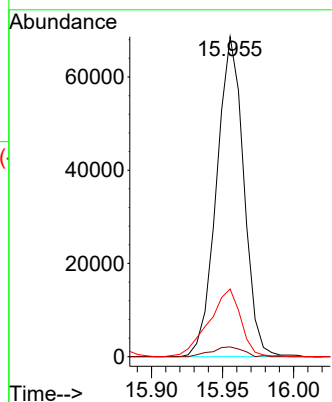

#67
N-Nitrosodiphenylamine
Concen: 80.444 ng/ul
RT: 16.079 min Scan# 2160
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:169 Resp: 385273
Ion Ratio Lower Upper
169 100
168 65.7 56.9 85.3
167 37.8 29.4 44.0



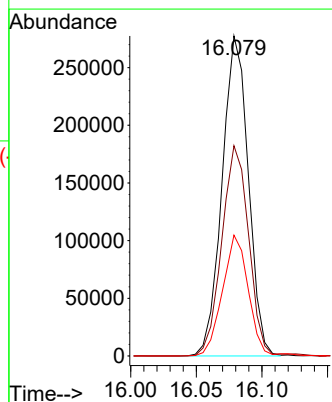





#68
4-Bromophenyl-phenylether
Concen: 76.805 ng/ul
RT: 16.754 min Scan# 21
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:248 Resp: 135595
Ion Ratio Lower Upper
248 100
250 98.7 71.8 107.8
141 71.6 54.8 82.2

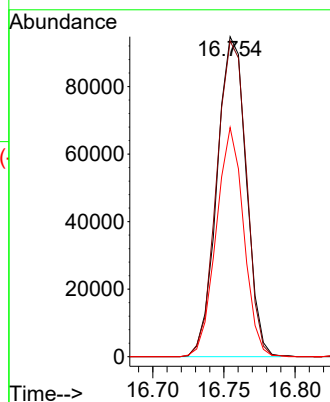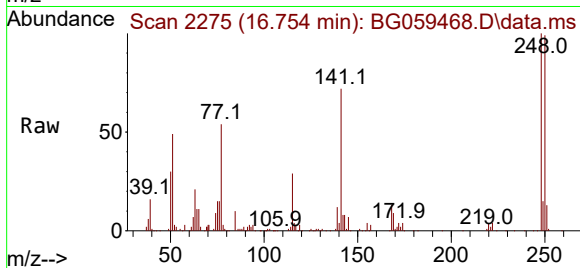

#69
Hexachlorobenzene
Concen: 77.553 ng/ul
RT: 16.848 min Scan# 2291
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:284 Resp: 156458
Ion Ratio Lower Upper
284 100
142 30.2 21.4 32.0
249 31.8 28.1 42.1

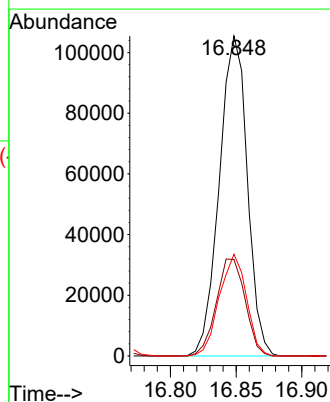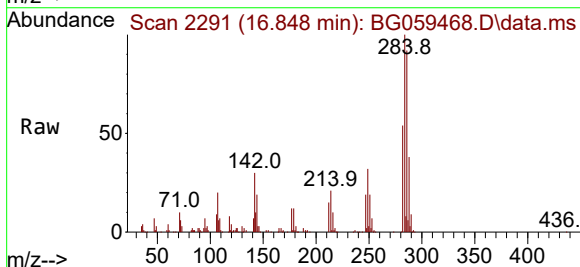



#70

Atrazine

Concen: 75.913 ng/ul

RT: 17.019 min Scan# 21

Delta R.T. 0.009 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Instrument :

BNA_G

ClientSampleId :

SSTD080417





Tgt Ion:200 Resp: 141547

Ion Ratio Lower Upper

200 100

173 25.5 21.7 32.5

215 47.4 34.8 52.2



#71

Pentachlorophenol

Concen: 86.334 ng/ul

RT: 17.207 min Scan# 2352

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43




Tgt Ion:266 Resp: 99096


Ion Ratio Lower Upper

266 100

264 63.0 56.9 85.3

268 61.7 56.4 84.6





#72

Phenanthrene

Concen: 78.626 ng/ul

RT: 17.624 min Scan# 2422

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Instrument :

BNA_G

ClientSampleId :

SSTD080417





Tgt Ion:178 Resp: 793612

Ion Ratio Lower Upper

178 100

179 14.5 11.8 17.8

176 19.1 14.2 21.4



#74

Anthracene

Concen: 78.894 ng/ul

RT: 17.718 min Scan# 2439

Delta R.T. 0.009 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43




Tgt Ion:178 Resp: 816494


Ion Ratio Lower Upper

178 100

179 15.1 13.2 19.8

176 18.6 15.1 22.7



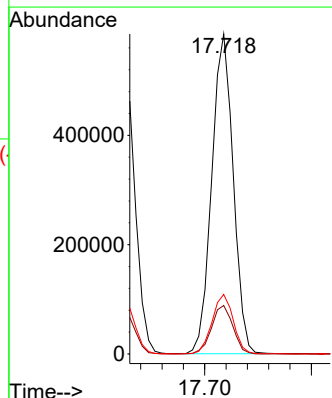





#75
1,2,3,4-Tetrachlorobenzene
Concen: 78.401 ng/uL
RT: 13.629 min Scan# 1742
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:216 Resp: 183278
Ion Ratio Lower Upper
216 100
214 79.5 64.5 96.7
218 49.5 34.7 52.1

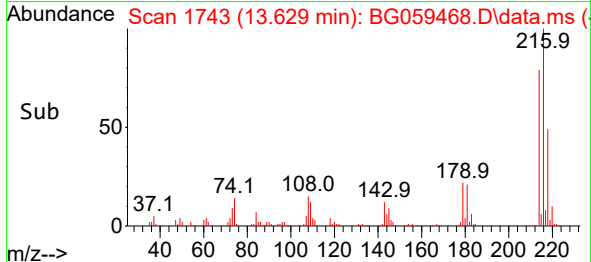

#76
Pentachlorobenzene
Concen: 78.570 ng/uL
RT: 15.121 min Scan# 1997
Delta R.T. -0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:250 Resp: 178999
Ion Ratio Lower Upper
250 100
248 62.2 46.5 69.7
252 71.0 53.3 79.9







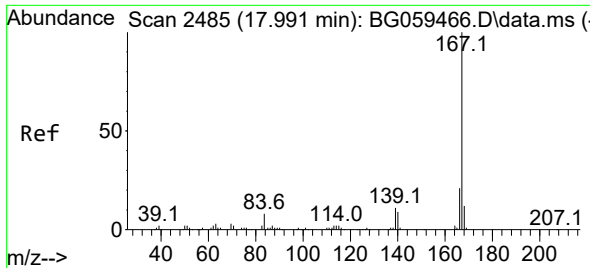

#77
 Carbazole
 Concen: 77.638 ng/ul
 RT: 17.994 min Scan# 2486
 Delta R.T. 0.003 min
 Lab File: BG059468.D
 Acq: 17 Oct 2023 21:43




Instrument :
 BNA_G
 ClientSampleId :
 SSTD080417


Tgt Ion:167 Resp: 694836
 Ion Ratio Lower Upper
 167 100
 166 22.7 17.0 25.4
 139 12.9 8.6 12.8#

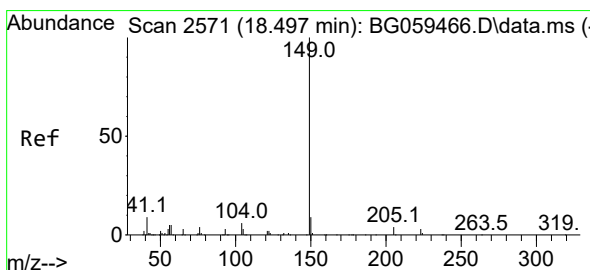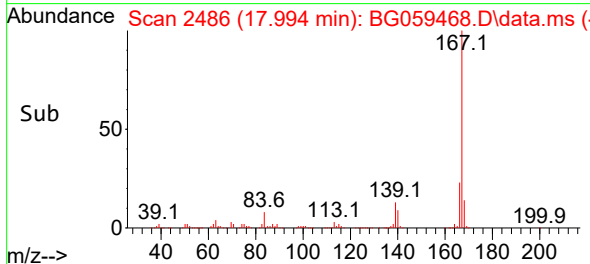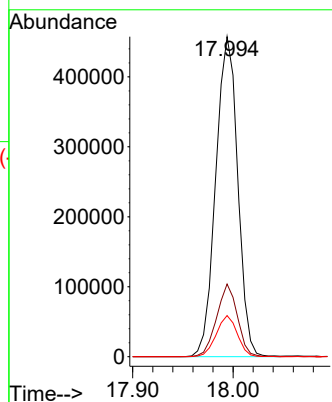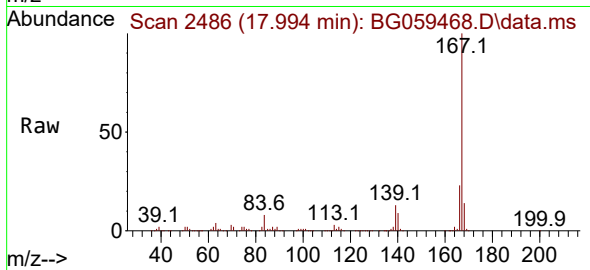

#78
 Di-n-butylphthalate
 Concen: 81.299 ng/ul
 RT: 18.493 min Scan# 2571
 Delta R.T. -0.003 min
 Lab File: BG059468.D
 Acq: 17 Oct 2023 21:43

Tgt Ion:149 Resp: 820239
 Ion Ratio Lower Upper
 149 100
 150 9.1 6.9 10.3
 104 5.2 4.6 7.0


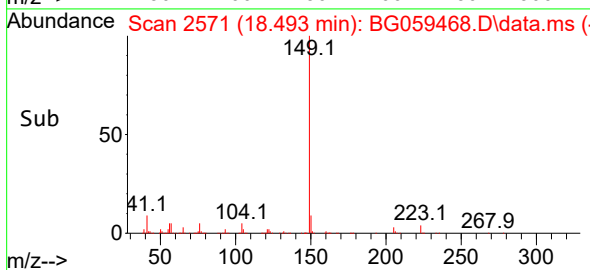
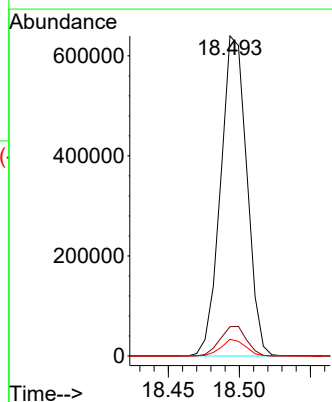
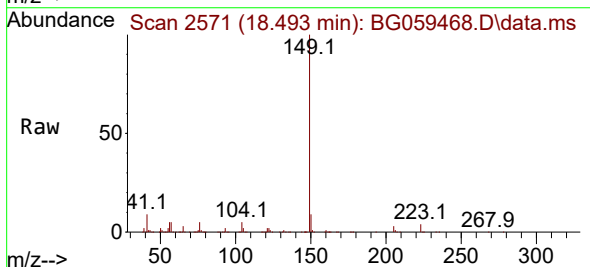




#80
Fluoranthene
Concen: 80.708 ng/u1
RT: 19.622 min Scan# 21
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:202 Resp: 941443
Ion Ratio Lower Upper
202 100
101 10.2 7.4 11.0
100 9.4 6.6 10.0



#82
Pyrene
Concen: 77.995 ng/u1
RT: 19.986 min Scan# 2825
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:202 Resp: 977041
Ion Ratio Lower Upper
202 100
101 12.2 10.5 15.7
100 11.3 9.2 13.8





#83

Butylbenzylphthalate

Concen: 86.791 ng/ul

RT: 20.838 min Scan# 2969

Delta R.T. 0.003 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Instrument :

BNA_G

ClientSampleId :

SSTD080417





Tgt Ion:149 Resp: 366322

Ion Ratio Lower Upper

149 100

91 74.0 58.4 87.6

206 21.4 17.8 26.8

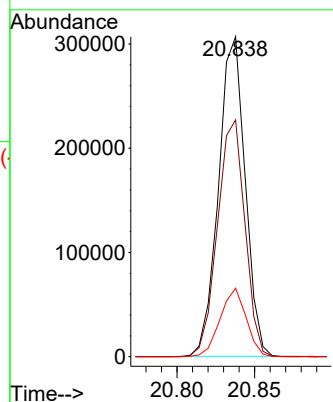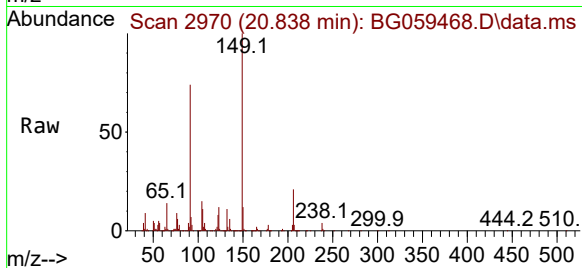

#84

3,3'-Dichlorobenzidine

Concen: 79.411 ng/ul

RT: 21.772 min Scan# 3129

Delta R.T. 0.009 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43




Tgt Ion:252 Resp: 330169


Ion Ratio Lower Upper

252 100

254 61.7 50.6 75.8

126 9.1 7.8 11.8



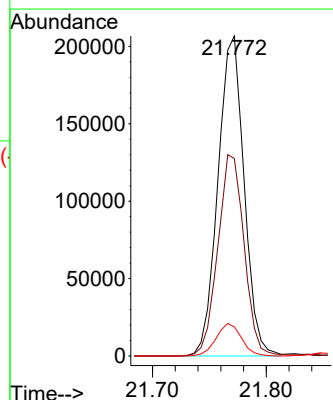
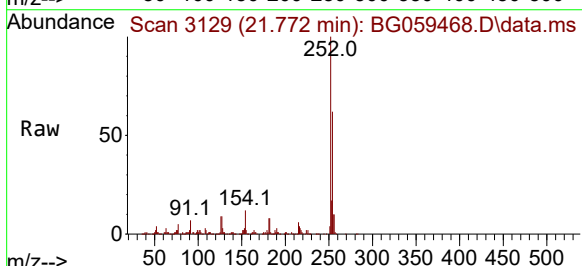




#85
Benzo(a)anthracene
Concen: 78.409 ng/ul
RT: 21.854 min Scan# 3142
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:228 Resp: 984881
Ion Ratio Lower Upper
228 100
229 20.3 14.6 21.8
226 27.4 20.2 30.2



#86
Bis(2-ethylhexyl)phthalate
Concen: 88.013 ng/ul
RT: 21.684 min Scan# 3114
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:149 Resp: 541488
Ion Ratio Lower Upper
149 100
167 25.5 18.9 28.3
279 3.0 2.6 4.0









#87
Chrysene
Concen: 77.157 ng/ul
RT: 21.925 min Scan# 3153
Delta R.T. 0.009 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:228 Resp: 914294
Ion Ratio Lower Upper
228 100
226 28.8 23.4 35.0
229 19.8 14.3 21.5

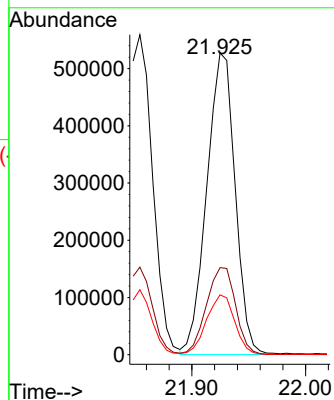

#89
Di-n-octyl phthalate
Concen: 87.179 ng/ul
RT: 22.965 min Scan# 3332
Delta R.T. 0.003 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:149 Resp: 946192



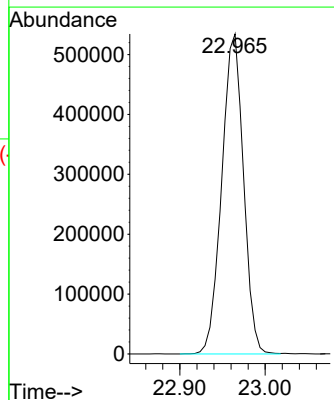





#90
Benzo(b)fluoranthene
Concen: 80.295 ng/ul
RT: 24.210 min Scan# 3544
Delta R.T. 0.014 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43




Instrument :
BNA_G
ClientSampleId :
SSTD080417


Tgt Ion:252 Resp: 1006127
Ion Ratio Lower Upper
252 100
253 22.4 17.2 25.8
125 9.8 9.8 14.6

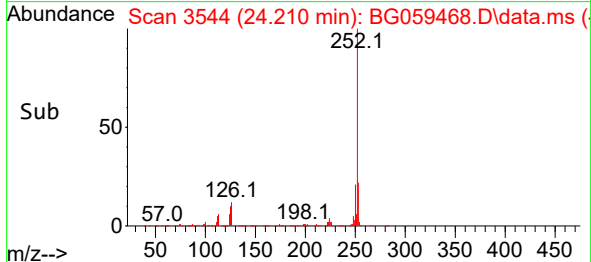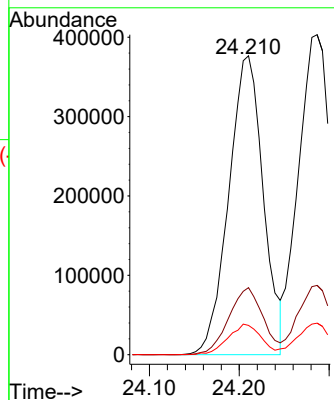

#91
Benzo(k)fluoranthene
Concen: 79.949 ng/ul
RT: 24.287 min Scan# 3557
Delta R.T. 0.015 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:252 Resp: 1018481
Ion Ratio Lower Upper
252 100
253 21.7 17.6 26.4
125 9.8 7.2 10.8

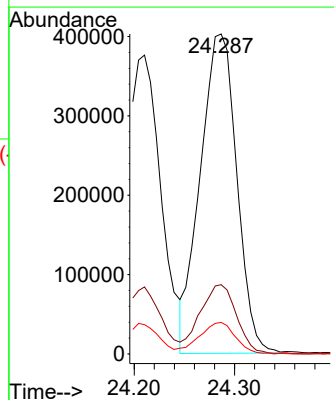



#93

Benzo(a)pyrene

Concen: 79.206 ng/ul

RT: 25.168 min Scan# 31

Delta R.T. 0.020 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43

Instrument :

BNA_G

ClientSampleId :

SSTD080417





Tgt Ion:252 Resp: 962507

Ion Ratio Lower Upper

252 100

253 22.5 16.2 24.4

125 10.7 9.6 14.4

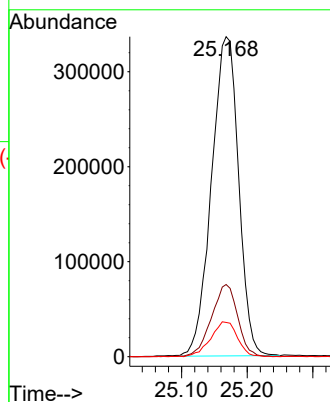

#94

Indeno(1,2,3-cd)pyrene

Concen: 81.322 ng/ul

RT: 29.304 min Scan# 4411

Delta R.T. 0.020 min

Lab File: BG059468.D

Acq: 17 Oct 2023 21:43




Tgt Ion:276 Resp: 1110015


Ion Ratio Lower Upper

276 100

138 20.7 16.1 24.1

277 22.6 17.4 26.2









#95
Dibenzo(a,h)anthracene
Concen: 43.606 ng/ul
RT: 29.381 min Scan# 4424
Delta R.T. 0.014 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Instrument :
BNA_G
ClientSampleId :
SSTD080417

Tgt Ion:278 Resp: 495226
Ion Ratio Lower Upper
278 100
139 15.6 12.6 18.8
279 23.4 18.6 27.8

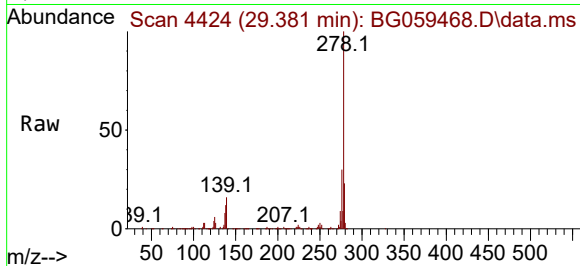

#96
Benzo(g,h,i)perylene
Concen: 100.683 ng/ul
RT: 30.591 min Scan# 4630
Delta R.T. 0.044 min
Lab File: BG059468.D
Acq: 17 Oct 2023 21:43

Tgt Ion:276 Resp: 1123118
Ion Ratio Lower Upper
276 100
138 25.4 15.1 22.7#
277 22.3 17.4 26.2

