
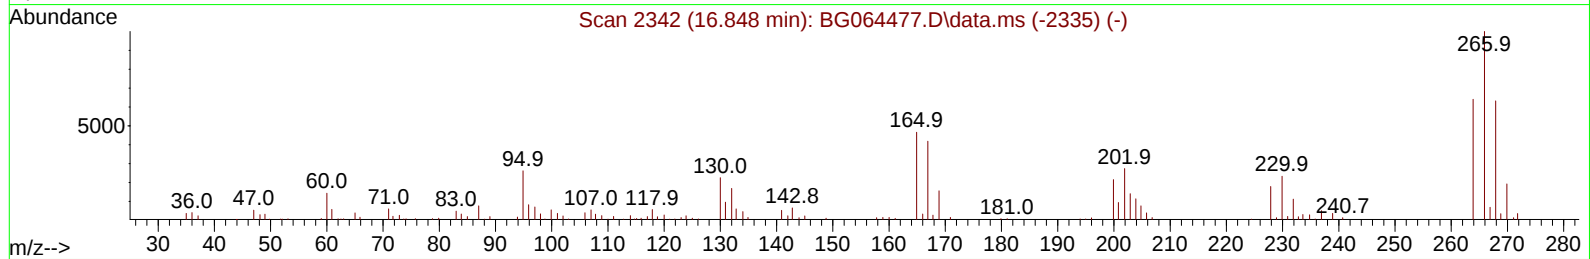
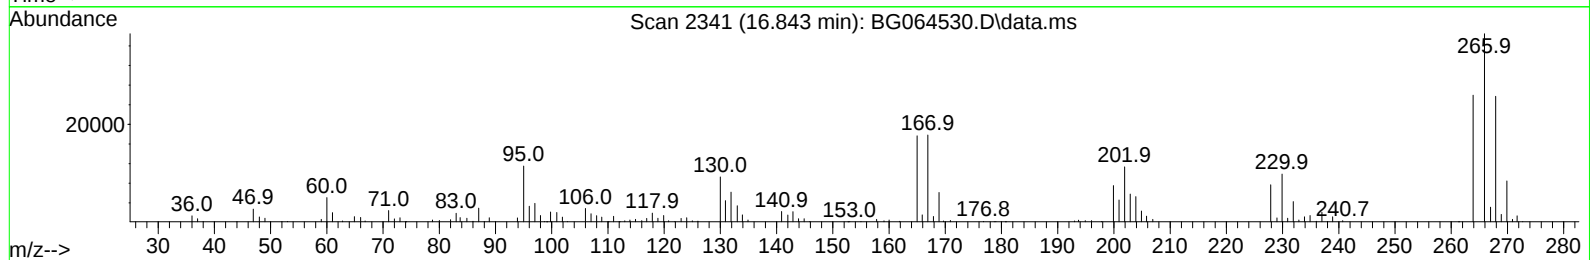


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064530.D
Acq On : 17 Oct 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 11:35:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

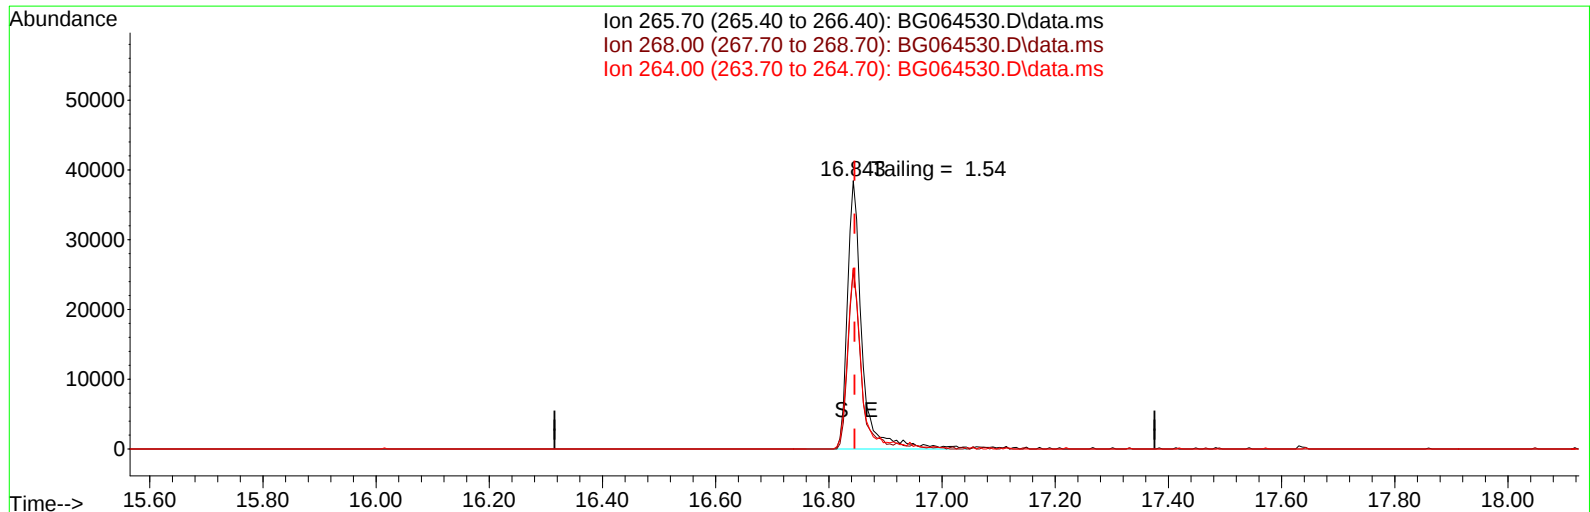

TIC: BG064530.D\data.ms

(70) Pentachlorophenol (C)




16.843min (-0.002) 25263.60 ng

response 67429

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	66.85
264.00	64.00	67.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064530.D
Acq On : 17 Oct 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 11:35:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 02 16:40:42 2025
Response via : Initial Calibration

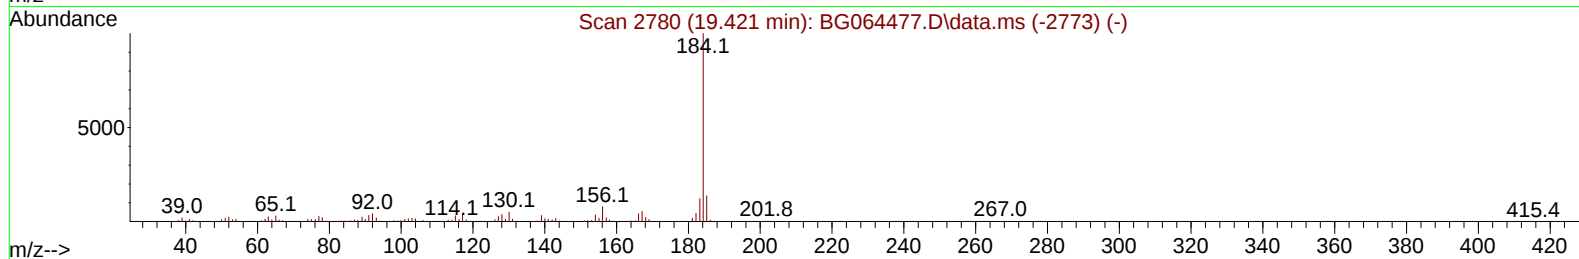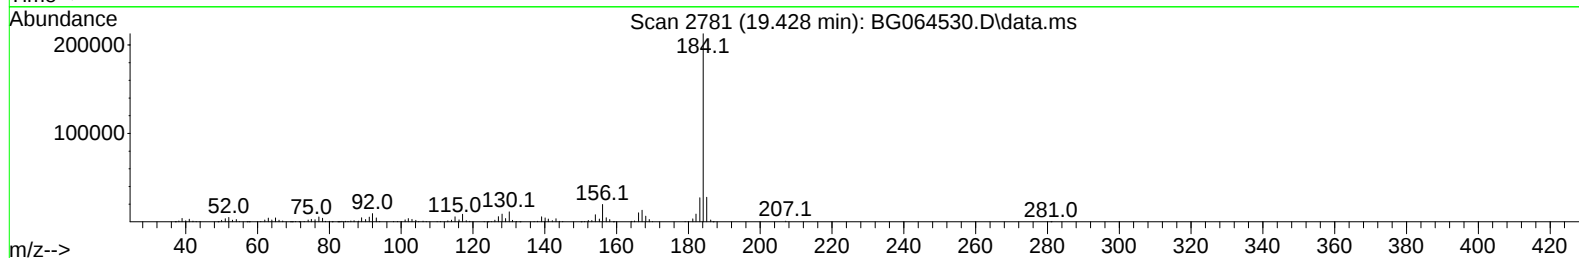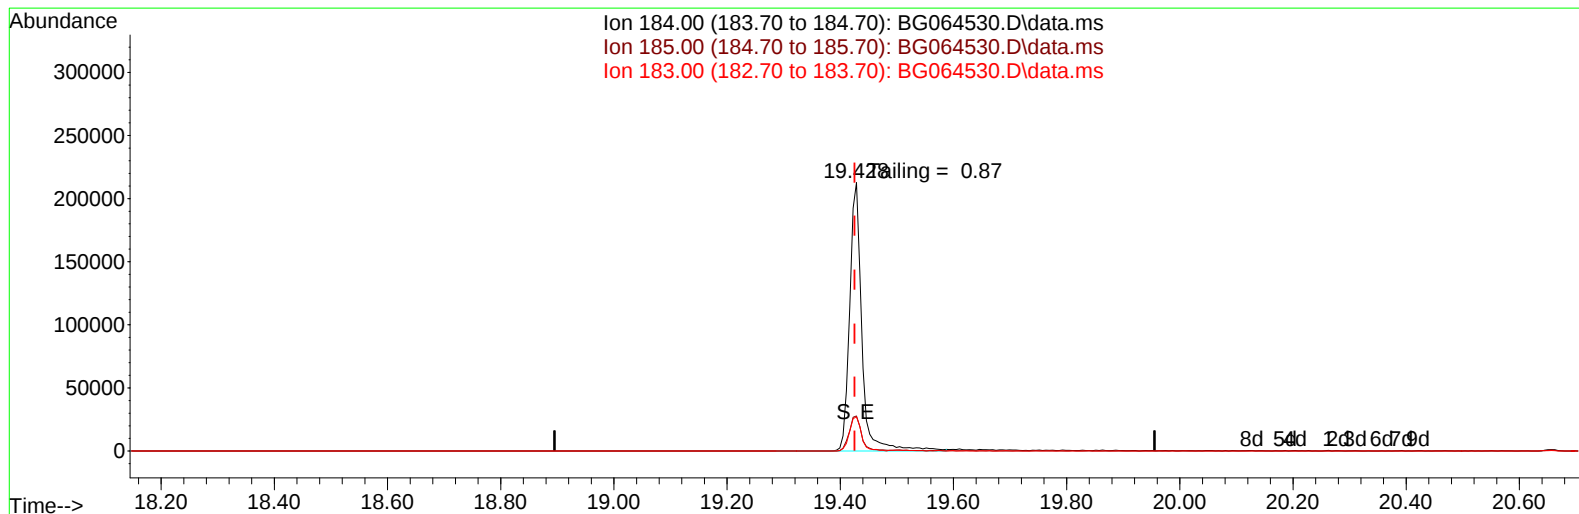

TIC: BG064530.D\data.ms

(77) Benzidine**19.428min (+ 0.003) 197325.20 ng m****response 319160**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.09
183.00	12.20	12.79
0.00	0.00	0.00