

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
 Data File : BG064545.D
 Acq On : 17 Oct 2025 21:15
 Operator : RC/JU
 Sample : Q3369-01 5X
 Misc : 8270/625.1 SPIKE
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MH-22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.415	390	396	404	rVB	43933	68552	15.70%	2.159%
2	7.001	660	666	678	rBV	42155	76972	17.63%	2.424%
3	7.818	799	805	813	rVB2	71789	119434	27.35%	3.762%
4	8.975	996	1002	1009	rBV	26841	50017	11.46%	1.575%
5	10.603	1271	1279	1292	rBV	87538	161256	36.93%	5.079%
6	13.070	1692	1699	1704	rBV	73902	113591	26.02%	3.578%
7	14.445	1927	1933	1940	rBV	133614	203344	46.57%	6.404%
8	15.732	2149	2152	2158	rVB4	3484	5345	1.22%	0.168%
9	15.803	2160	2164	2170	rVV3	11195	16514	3.78%	0.520%
10	15.938	2182	2187	2194	rBV2	68502	103762	23.76%	3.268%
11	17.007	2366	2369	2373	rBV3	2787	4376	1.00%	0.138%
12	17.189	2390	2400	2404	rBV2	200889	304802	69.81%	9.600%
13	17.230	2404	2407	2413	rVB	61686	85344	19.55%	2.688%
14	17.318	2419	2422	2428	rVB4	8837	13418	3.07%	0.423%
15	17.595	2466	2469	2472	rBV4	3561	4900	1.12%	0.154%
16	18.065	2545	2549	2550	rBV3	8082	9575	2.19%	0.302%
17	18.082	2550	2552	2554	rVV2	12015	14473	3.31%	0.456%
18	18.106	2554	2556	2561	rVB5	14200	19751	4.52%	0.622%
19	18.188	2567	2570	2576	rVB5	5608	8874	2.03%	0.279%
20	18.258	2576	2582	2585	rBV6	15347	29198	6.69%	0.920%
21	18.294	2586	2588	2590	rVB3	6641	5946	1.36%	0.187%
22	18.376	2599	2602	2606	rBV4	4889	7116	1.63%	0.224%
23	18.564	2630	2634	2637	rBV2	7910	11474	2.63%	0.361%
24	18.605	2637	2641	2649	rVB8	12089	20248	4.64%	0.638%
25	18.717	2657	2660	2662	rBV3	3899	5266	1.21%	0.166%
26	18.811	2674	2676	2680	rBV5	5048	4529	1.04%	0.143%
27	18.870	2680	2686	2688	rVV5	4356	8944	2.05%	0.282%
28	18.905	2690	2692	2695	rVB4	6741	6379	1.46%	0.201%
29	18.975	2701	2704	2709	rBV6	11143	19038	4.36%	0.600%
30	19.122	2725	2729	2731	rBV4	9309	12183	2.79%	0.384%
31	19.240	2745	2749	2755	rBV	145166	196957	45.11%	6.203%
32	19.334	2763	2765	2766	rBV2	5651	5055	1.16%	0.159%
33	19.604	2803	2811	2816	rBV	126057	212729	48.72%	6.700%
34	19.804	2837	2845	2851	rBV	180968	258663	59.24%	8.147%
35	19.921	2862	2865	2871	rBV6	16861	35736	8.18%	1.126%
36	21.414	3113	3119	3124	rBV2	236681	436629	100.00%	13.752%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064545.D
Acq On : 17 Oct 2025 21:15
Operator : RC/JU
Sample : Q3369-01 5X
Misc : 8270/625.1 SPIKE
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MH-22

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.455	3124	3126	3134	rVB	67948	104773	24.00%	3.300%
38	24.404	3620	3628	3637	rBV2	143507	409875	93.87%	12.909%




Sum of corrected areas: 3175038

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064545.D
Acq On : 17 Oct 2025 21:15
Operator : RC/JU
Sample : Q3369-01 5X
Misc : 8270/625.1 SPIKE
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MH-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

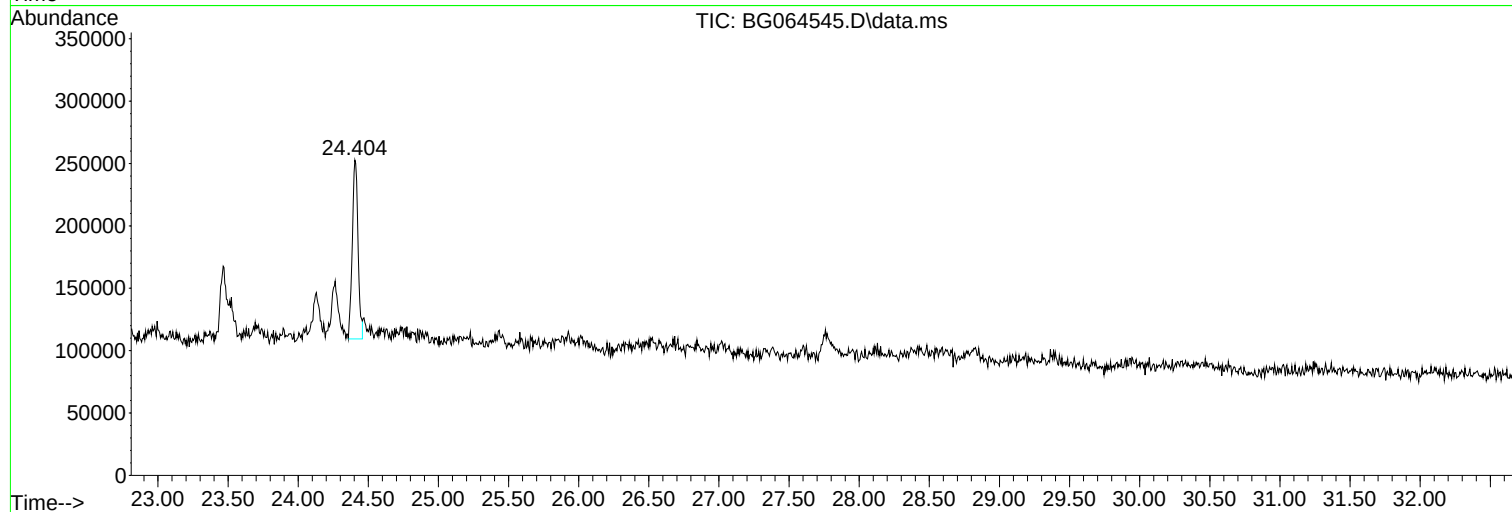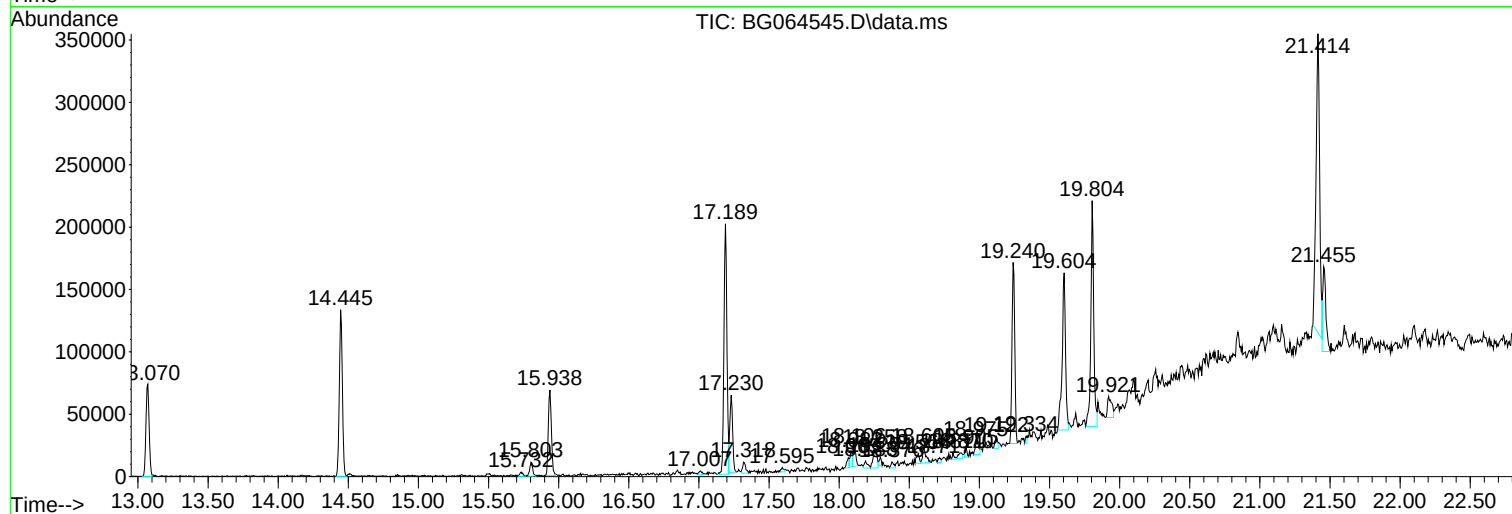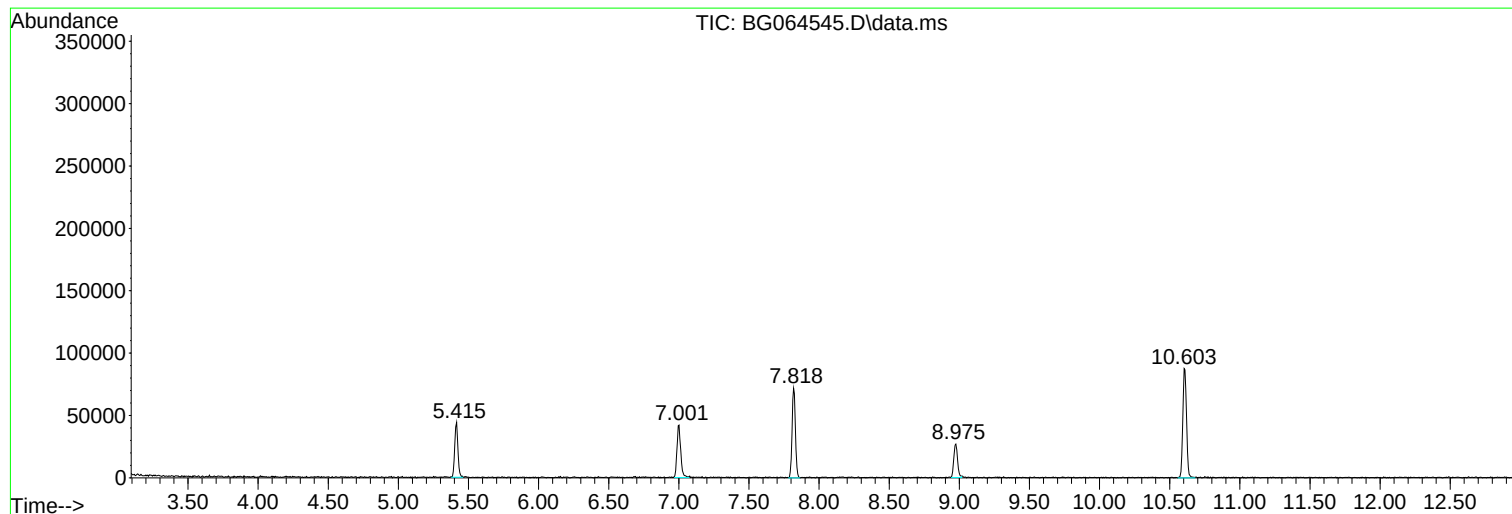

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064545.D
Acq On : 17 Oct 2025 21:15
Operator : RC/JU
Sample : Q3369-01 5X
Misc : 8270/625.1 SPIKE
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MH-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101725\
Data File : BG064545.D
Acq On : 17 Oct 2025 21:15
Operator : RC/JU
Sample : Q3369-01 5X
Misc : 8270/625.1 SPIKE
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MH-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------