


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG101725\  
Data File : BG064530.D  
Acq On : 17 Oct 2025 10:59  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100225.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Oct 02 16:40:42 2025

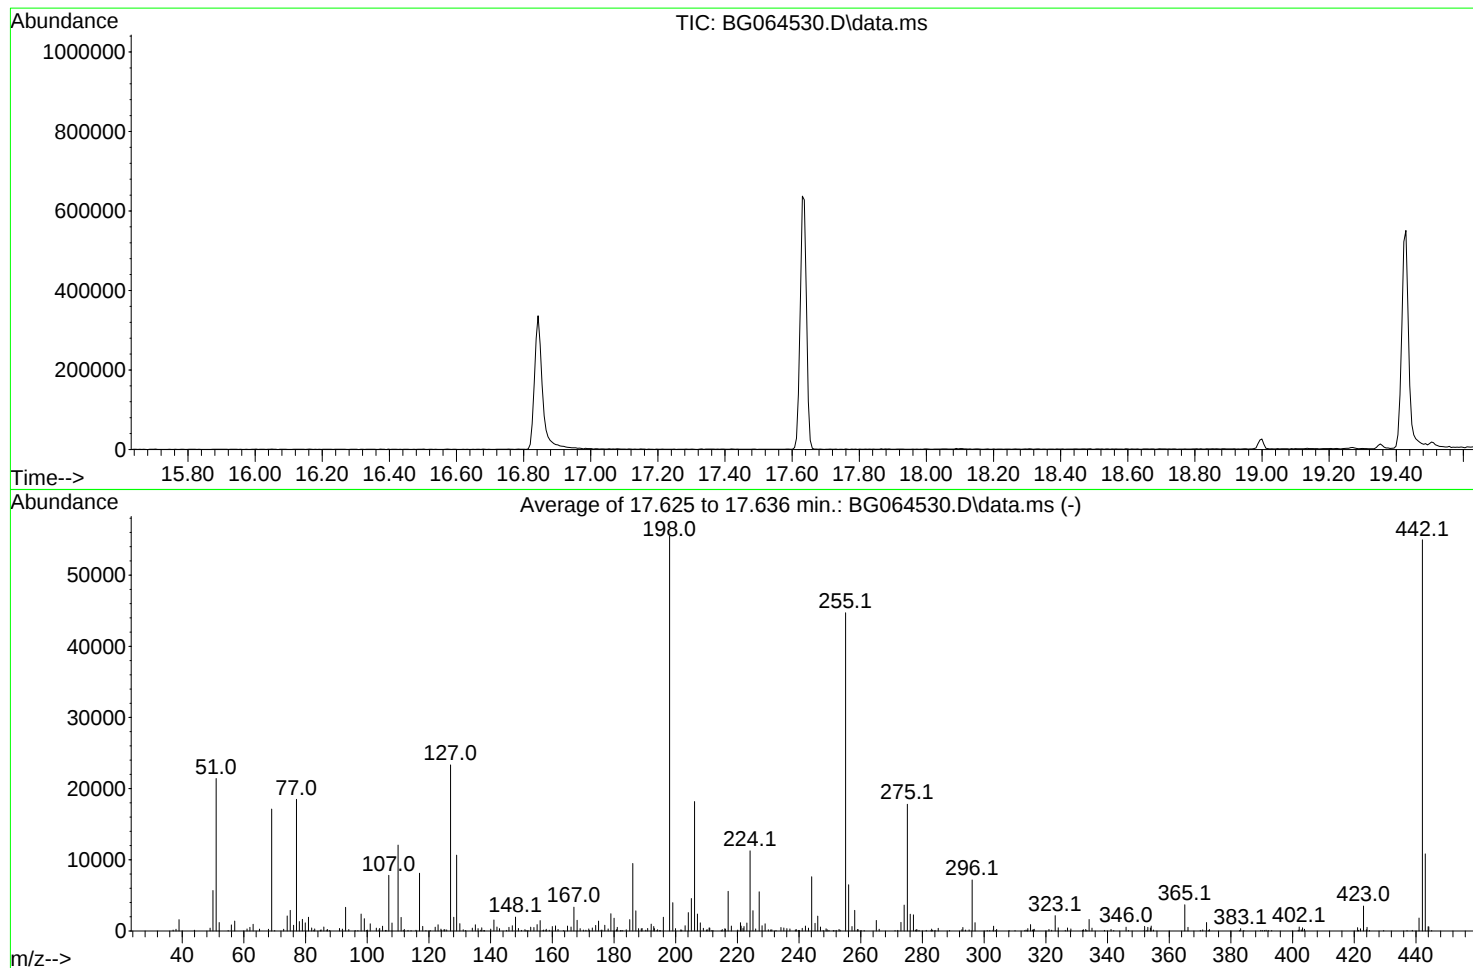




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 68     | 69      | 0.00   | 2      | 1.4   | 234   | PASS      |
| 69     | 69      | 100    | 100    | 100.0 | 17124 | PASS      |
| 70     | 69      | 0.00   | 2      | 0.4   | 68    | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0     | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 55491 | PASS      |
| 199    | 198     | 5      | 9      | 7.2   | 3979  | PASS      |
| 365    | 198     | 1      | 100    | 6.6   | 3684  | PASS      |
| 441    | 443     | 0.01   | 150    | 16.7  | 1803  | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 54965 | PASS      |
| 443    | 442     | 15     | 24     | 19.7  | 10823 | PASS      |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG101725\  
Data File : BG064530.D  
Acq On : 17 Oct 2025 10:59  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Oct 17 11:35:09 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 02 16:40:42 2025  
Response via : Initial Calibration

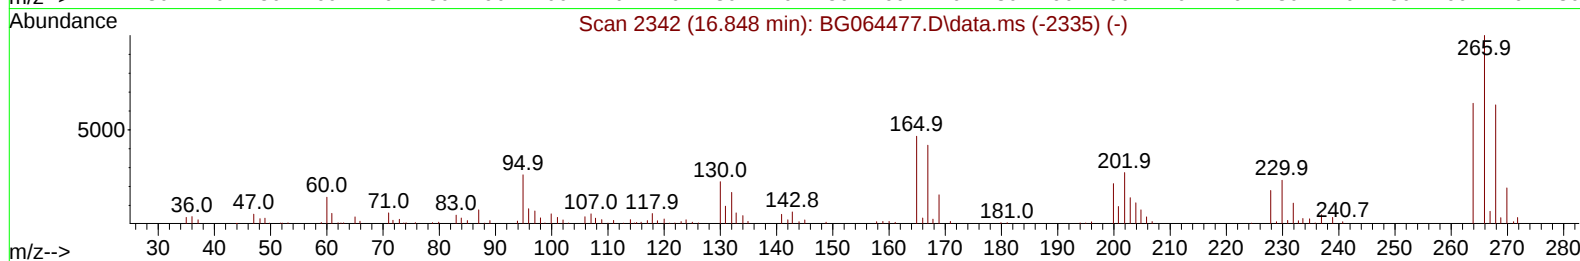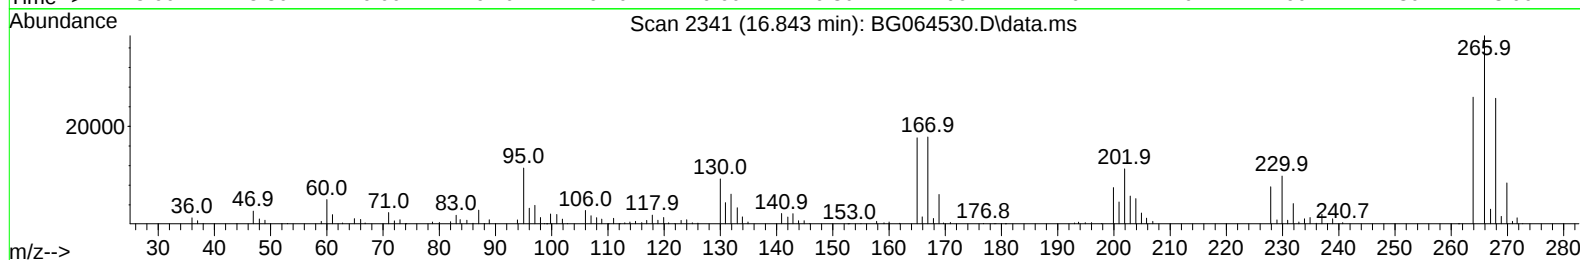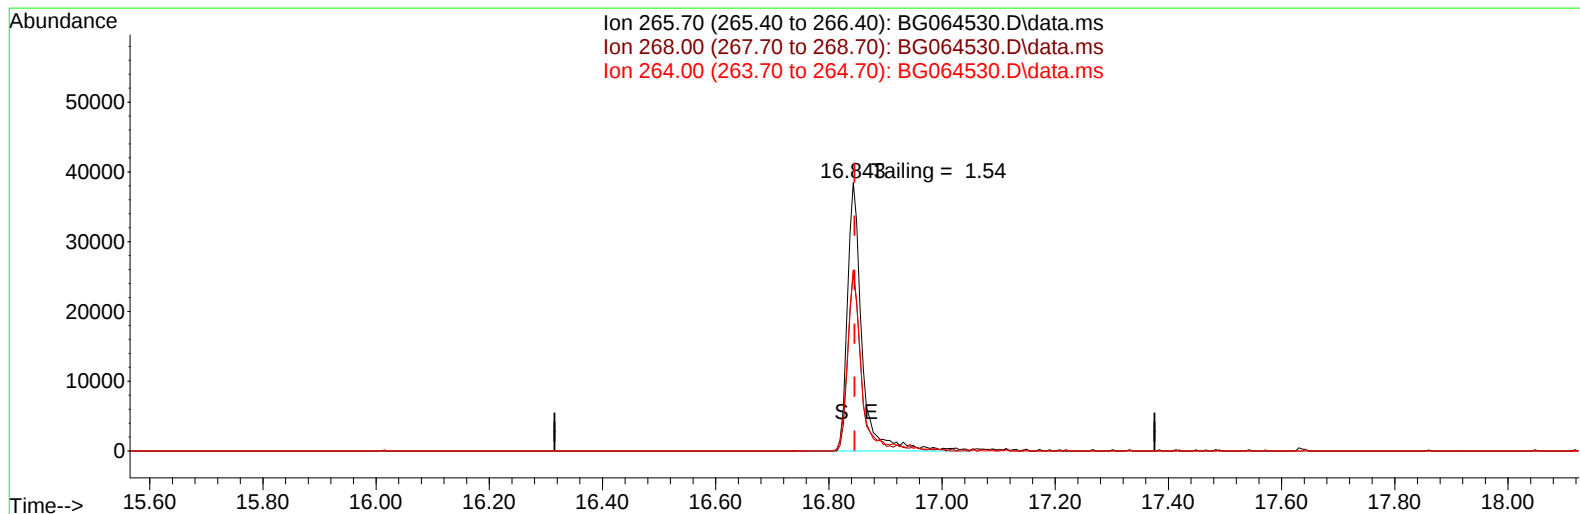

TIC: BG064530.D\data.ms

**(70) Pentachlorophenol (C)**

**16.843min (-0.002) 25263.60 ng**




**response 67429**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.20  | 66.85  |
| 264.00 | 64.00  | 67.43  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG101725\  
Data File : BG064530.D  
Acq On : 17 Oct 2025 10:59  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Oct 17 11:35:09 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 02 16:40:42 2025  
Response via : Initial Calibration

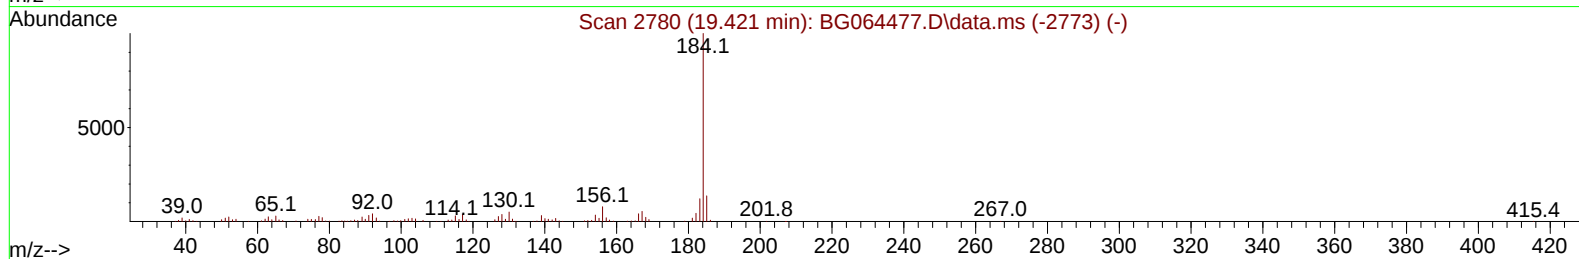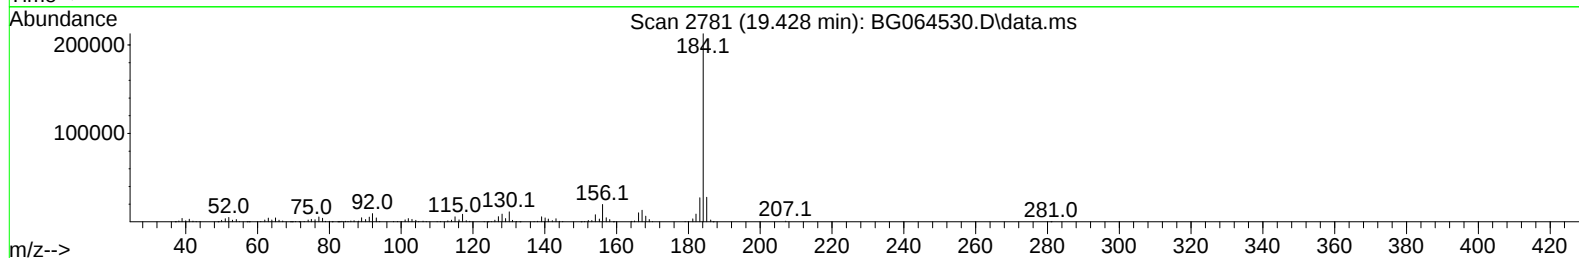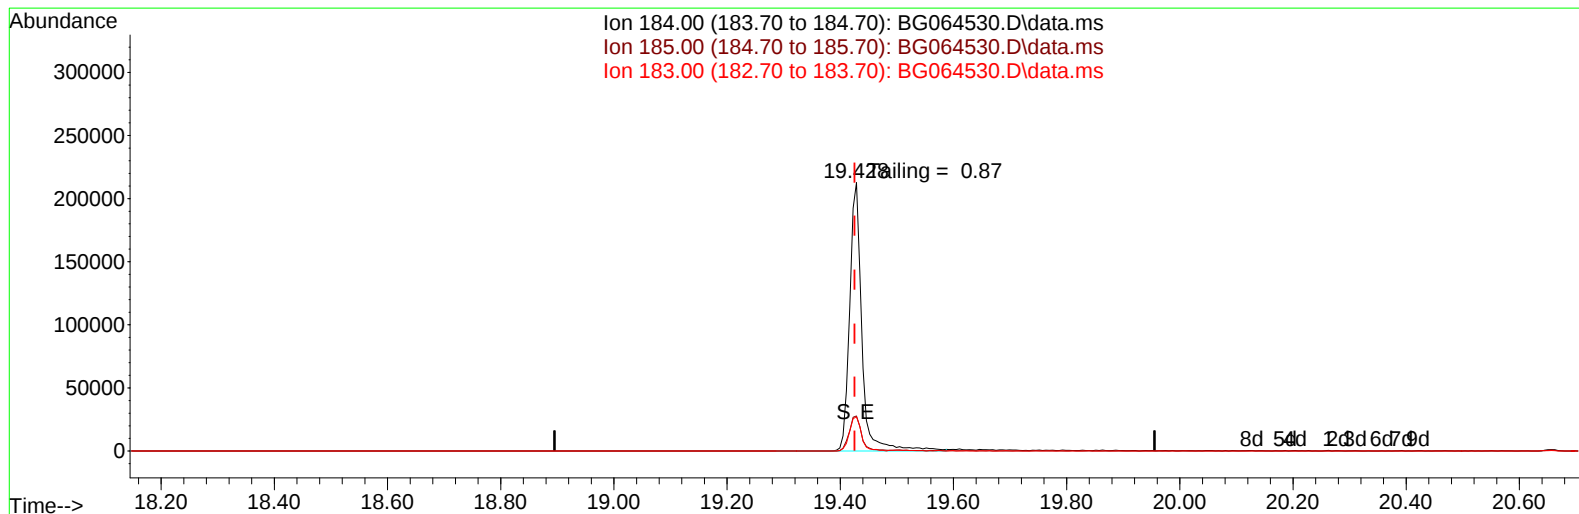

TIC: BG064530.D\data.ms

(77) Benzidine

19.428min (+ 0.003) 197325.20 ng m

response 319160

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.60  | 13.09  |
| 183.00 | 12.20  | 12.79  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/17/2025    | BNA_G            | <u>BG064530.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 235454           | 20.656             |
| DDD           | 2620             | 20.216             |
| DDE           | 61               | 19.946             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 2681          | 238135           | 1.13               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP