
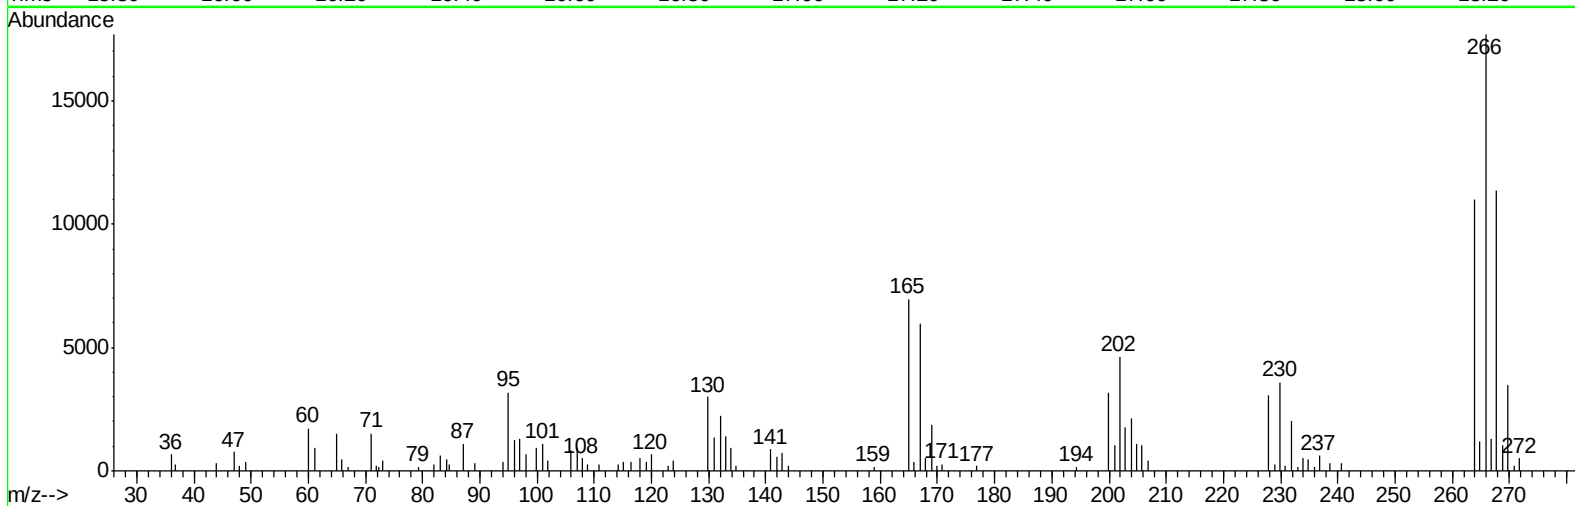


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101819\
Data File : BG043278.D
Acq On : 18 Oct 2019 16:49
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 06:44:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:11:45 2019
Response via : Initial Calibration

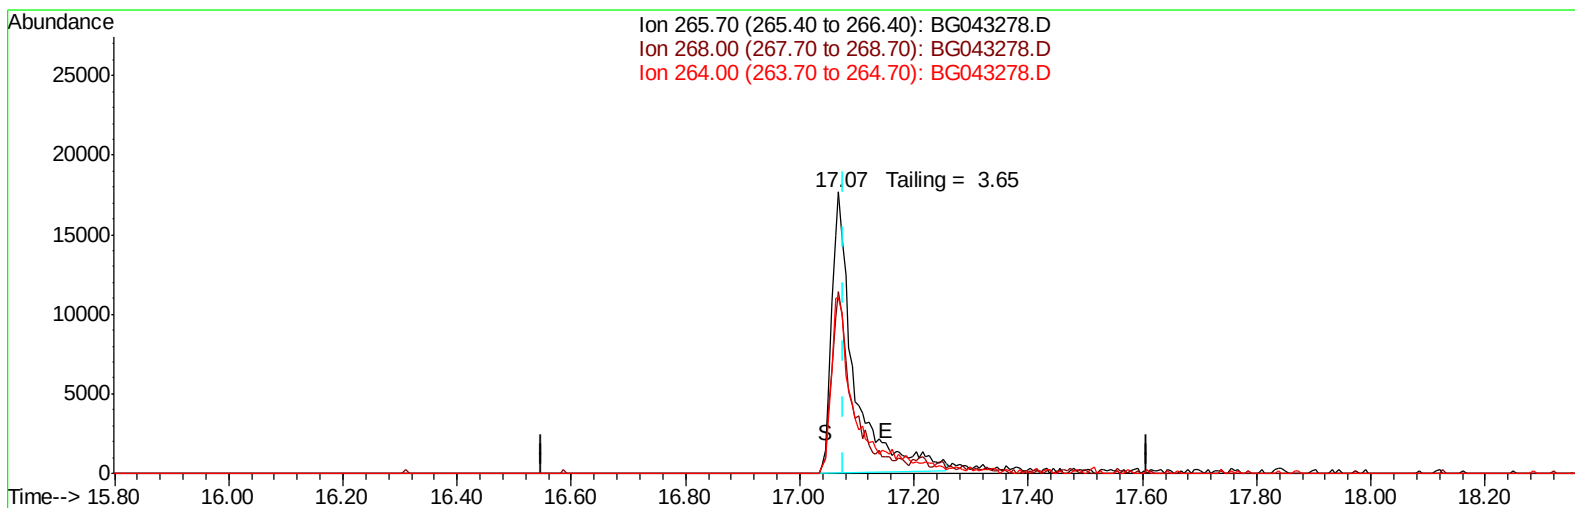

TIC: BG043278.D

(70) Pentachlorophenol (C)



17.068min (-0.010) 13481.89ng

response 43703

Ion	Exp%	Act%
265.70	100	100
268.00	65.20	64.34
264.00	63.40	62.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101819\
Data File : BG043278.D
Acq On : 18 Oct 2019 16:49
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 06:44:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:11:45 2019
Response via : Initial Calibration

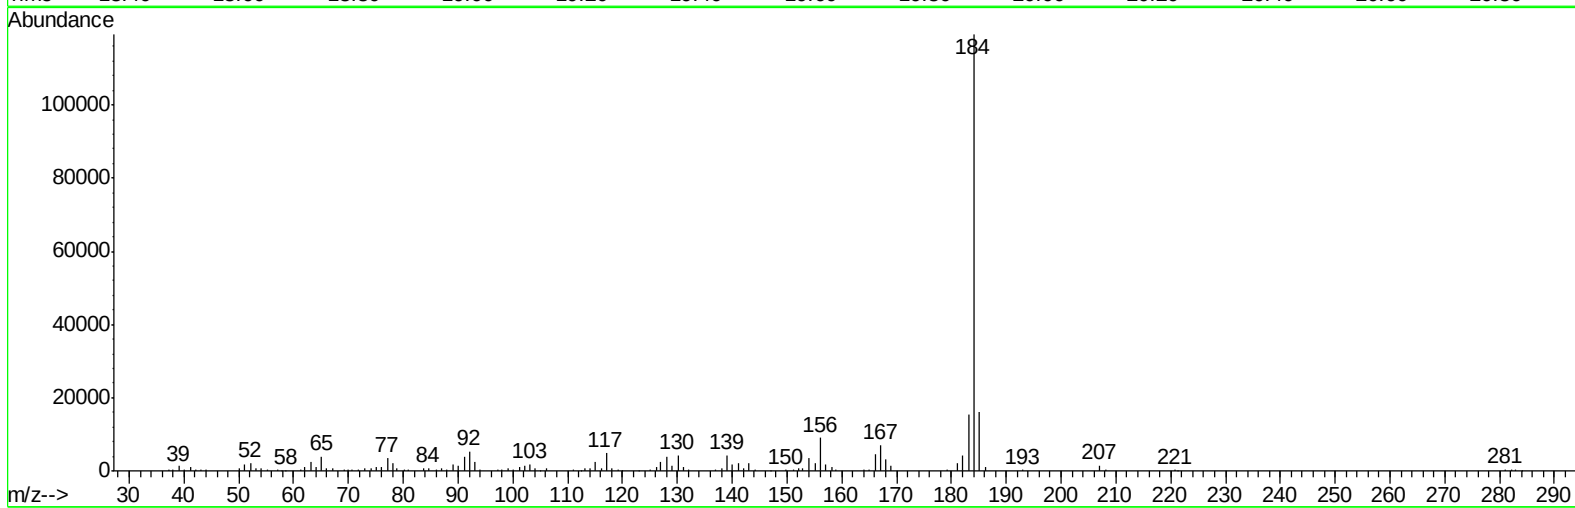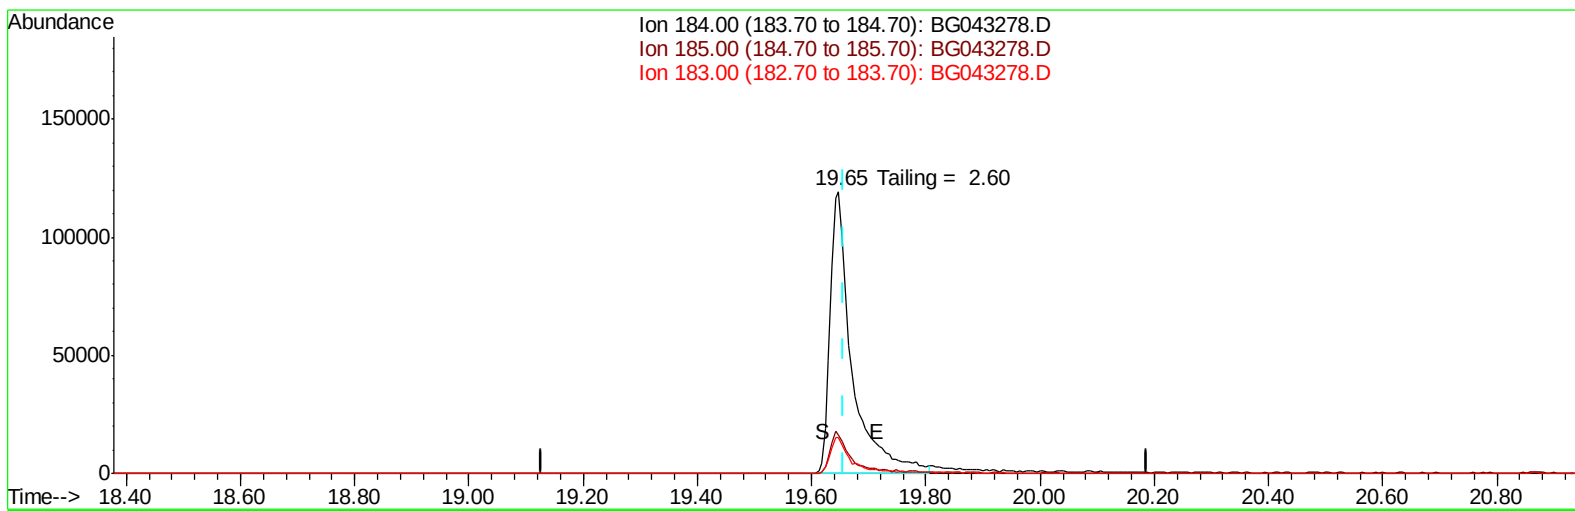

TIC: BG043278.D

(77) Benzidine

19.647min (-0.010) 0.00ng

response 315364

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	13.60
183.00	12.60	12.92
0.00	0.00	0.00