


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101819\
 Data File : BG043278.D
 Acq On : 18 Oct 2019 16:49
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 09 01:11:45 2019

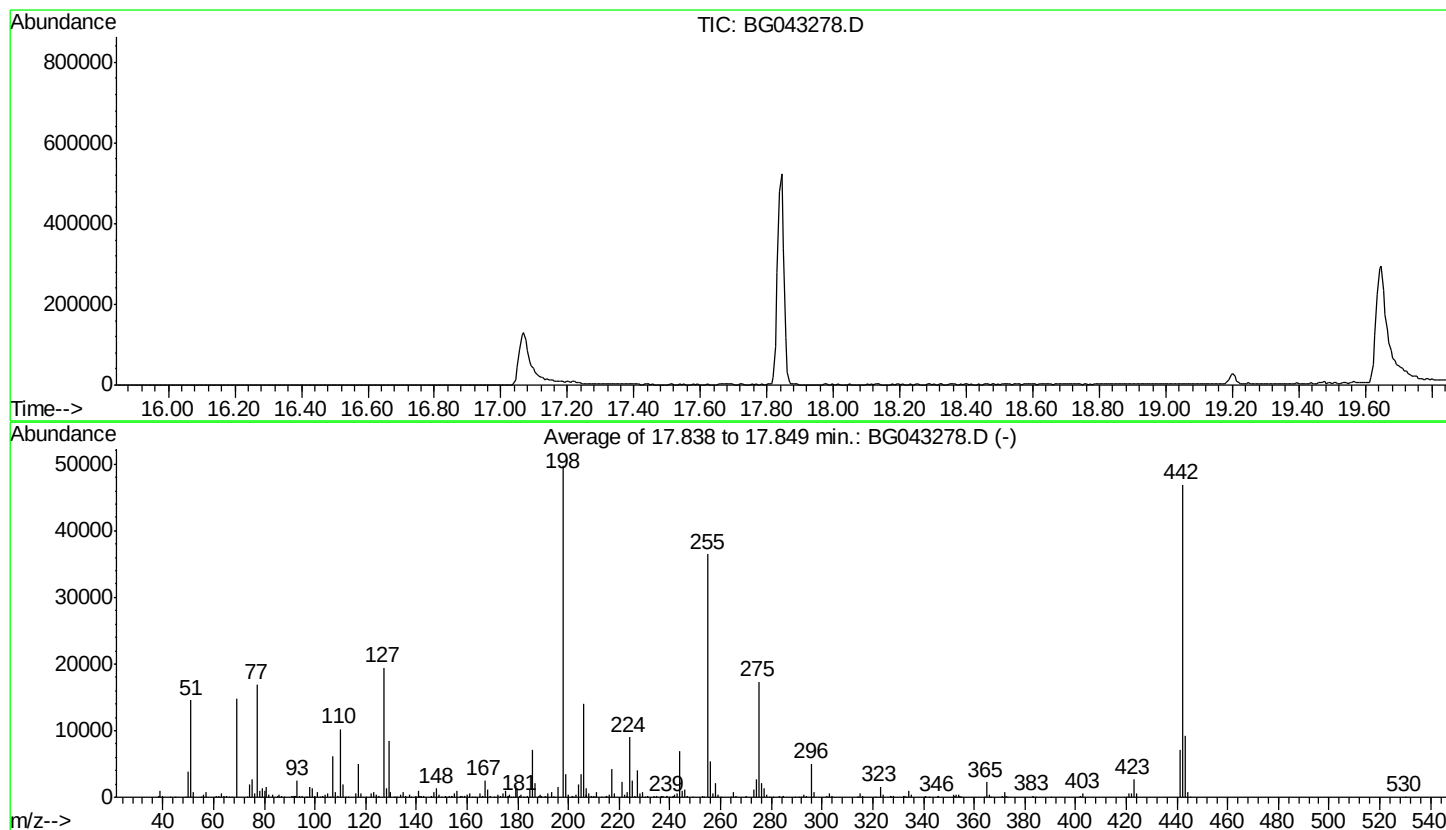

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	14519	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.6	14744	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.2	19484	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49760	PASS
199	198	5	9	6.8	3385	PASS
275	198	10	60	34.8	17322	PASS
365	198	1	100	4.6	2269	PASS
441	198	0.01	100	14.4	7184	PASS
442	198	50	100	94.2	46893	PASS
443	442	15	24	19.6	9205	PASS